
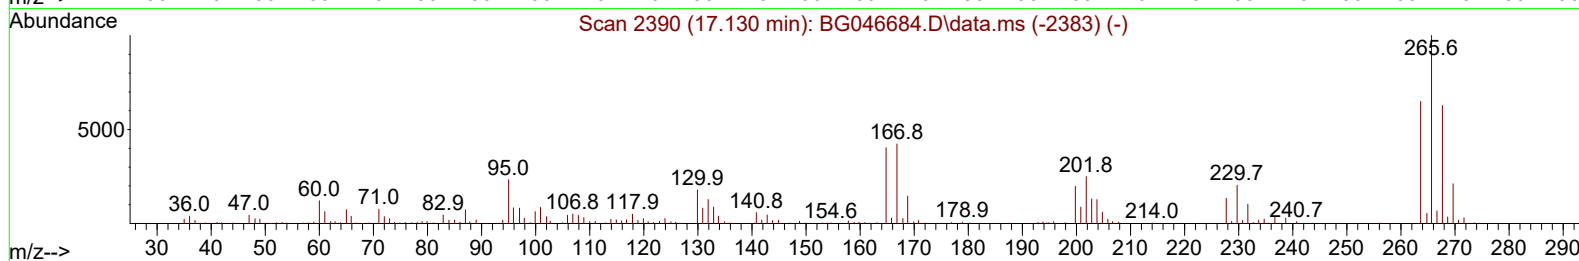
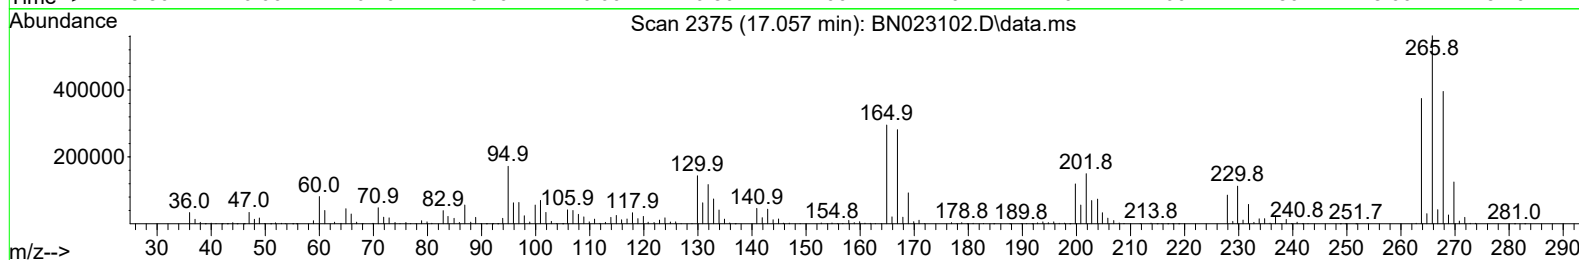


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120922\
Data File : BN023102.D
Acq On : 09 Dec 2022 11:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 08:03:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 10 08:03:48 2022
Response via : Initial Calibration

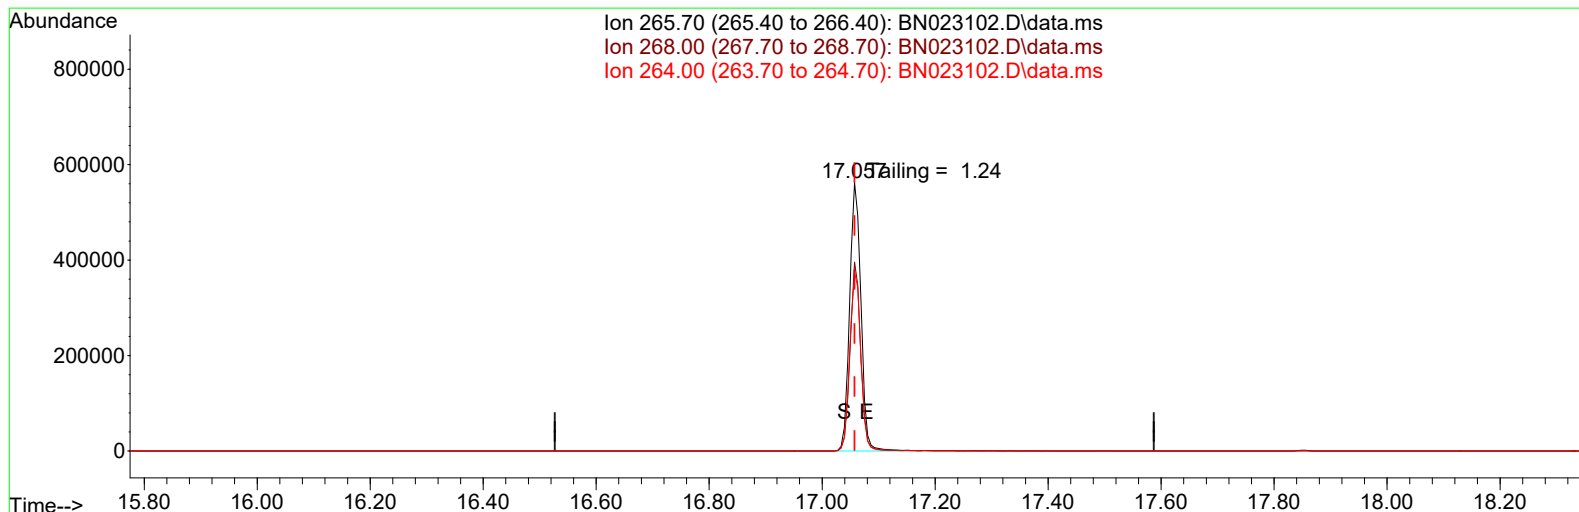

TIC: BN023102.D\data.ms

(70) Pentachlorophenol (C)




17.057min (0.000) 21446.94 ng

response 784157

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.40
264.00	61.60	66.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120922\
Data File : BN023102.D
Acq On : 09 Dec 2022 11:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 08:03:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 10 08:03:48 2022
Response via : Initial Calibration

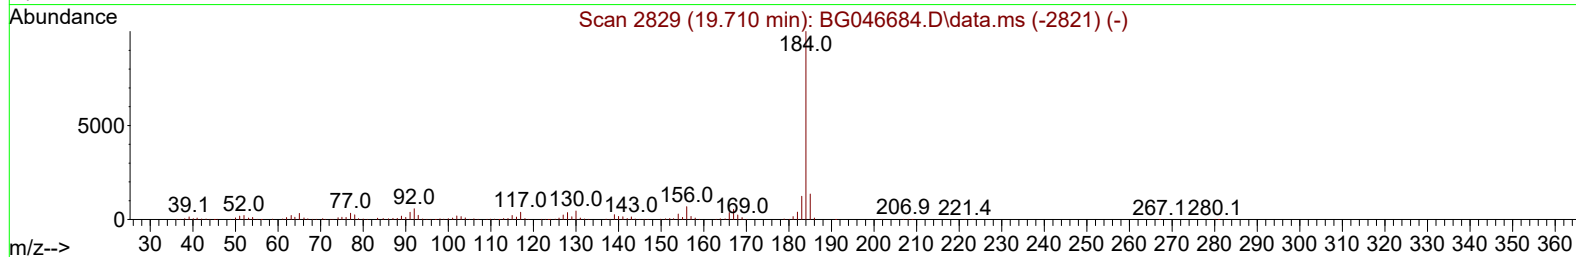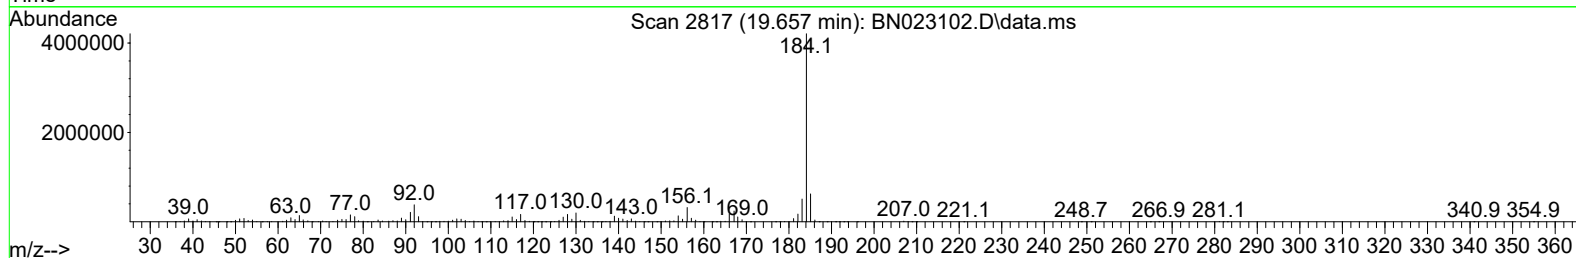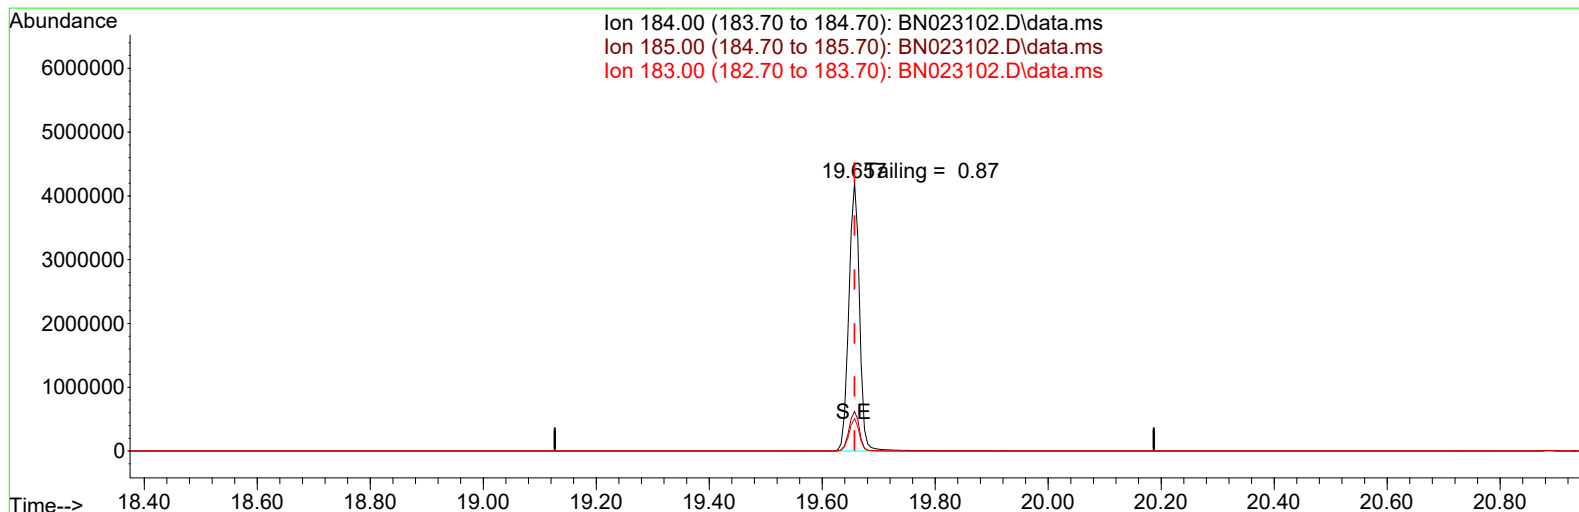

TIC: BN023102.D\data.ms

(77) Benzidine**19.657min (0.000) 1766858.15 ng****response 5500870**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.83
183.00	13.20	12.10
0.00	0.00	0.00