
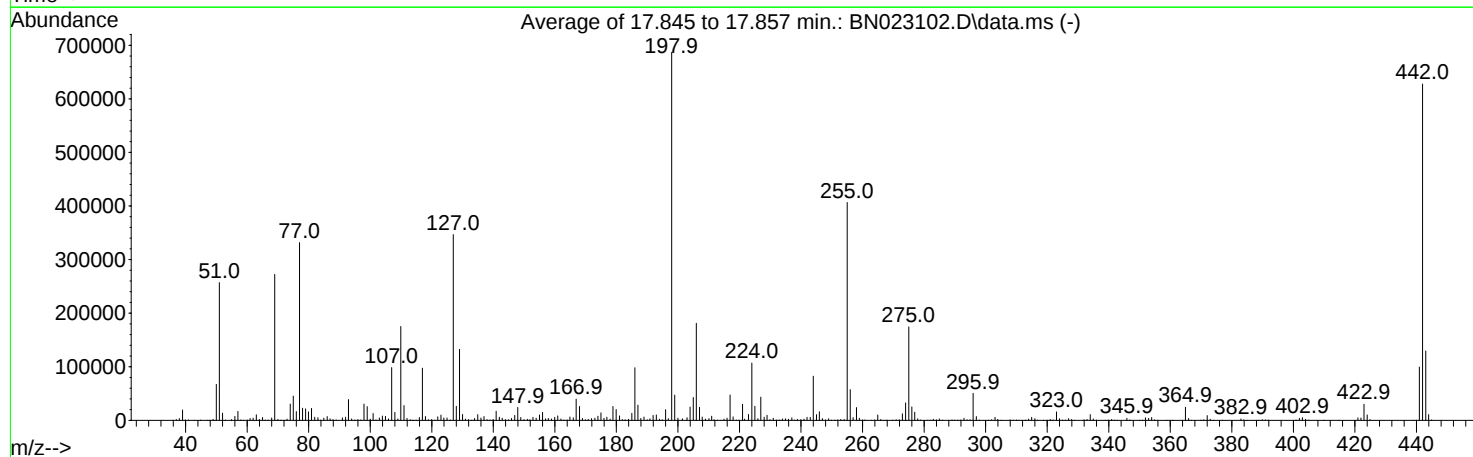


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120922\
 Data File : BN023102.D
 Acq On : 09 Dec 2022 11:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 12 05:18:26 2022

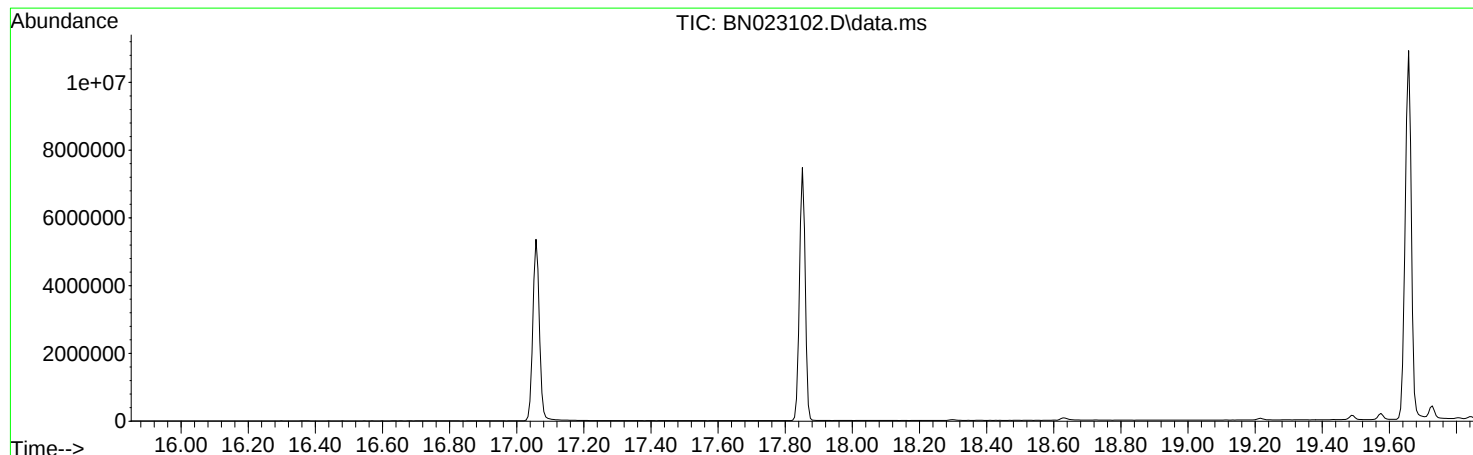




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	257088	PASS
68	69	0.00	2	1.6	4426	PASS
69	198	0.00	100	39.7	272299	PASS
70	69	0.00	2	0.6	1600	PASS
127	198	10	80	50.5	346773	PASS
197	198	0.00	2	0.5	3256	PASS
198	198	100	100	100.0	686677	PASS
199	198	5	9	6.9	47120	PASS
275	198	10	60	25.4	174251	PASS
365	198	1	100	3.5	24341	PASS
441	198	0.01	100	14.4	99213	PASS
442	442	50	100	100.0	627712	PASS
443	442	15	24	20.6	129432	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120922\
Data File : BN023102.D
Acq On : 09 Dec 2022 11:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 10 08:03:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 10 08:03:48 2022
Response via : Initial Calibration

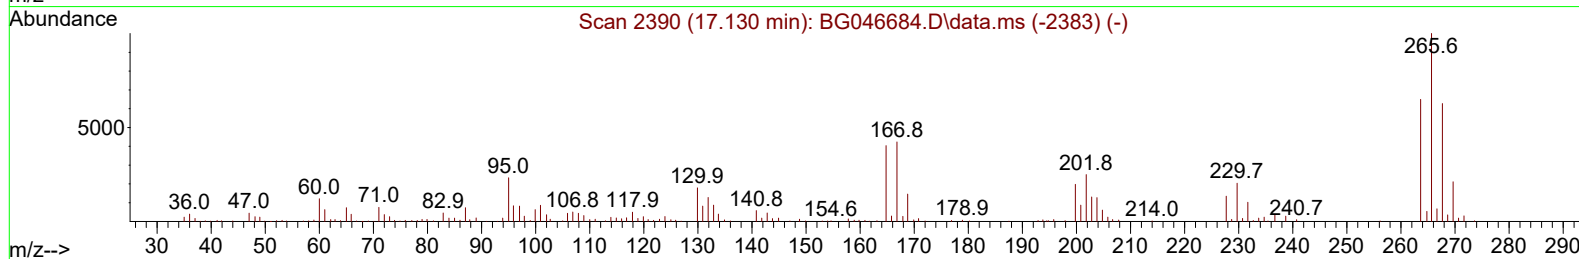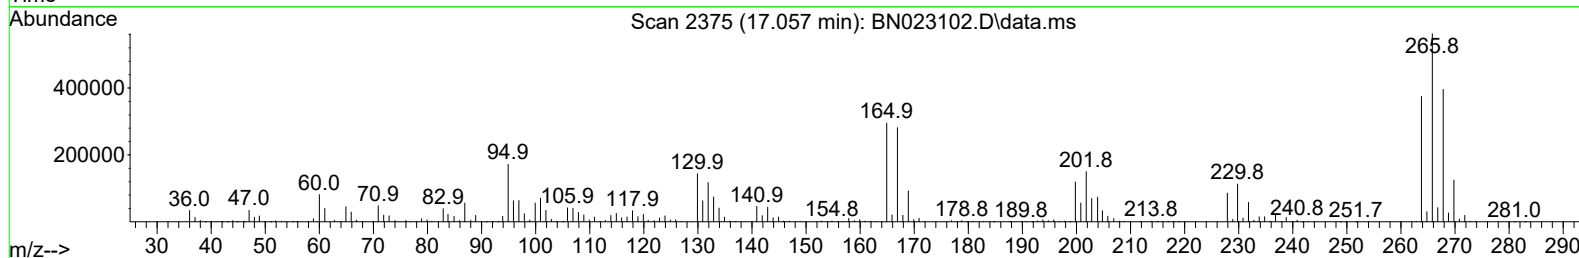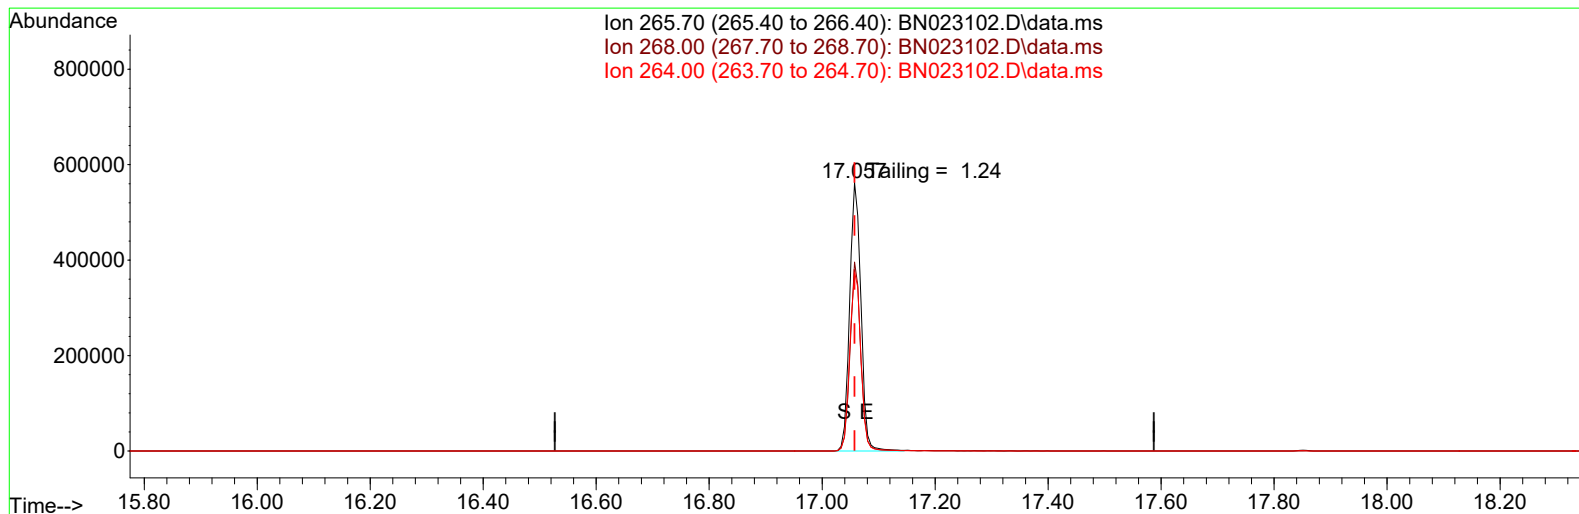

TIC: BN023102.D\data.ms

(70) Pentachlorophenol (C)

17.057min (0.000) 21446.94 ng




response 784157

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.40
264.00	61.60	66.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120922\
 Data File : BN023102.D
 Acq On : 09 Dec 2022 11:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 10 08:03:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 10 08:03:48 2022
 Response via : Initial Calibration

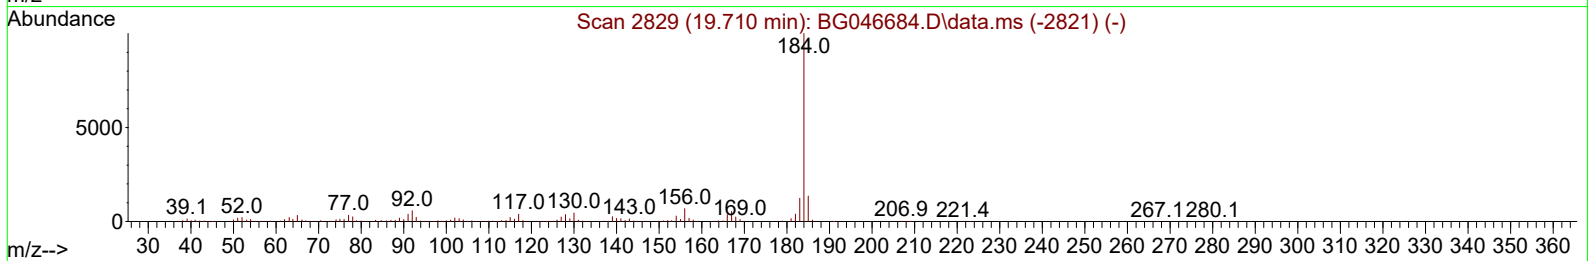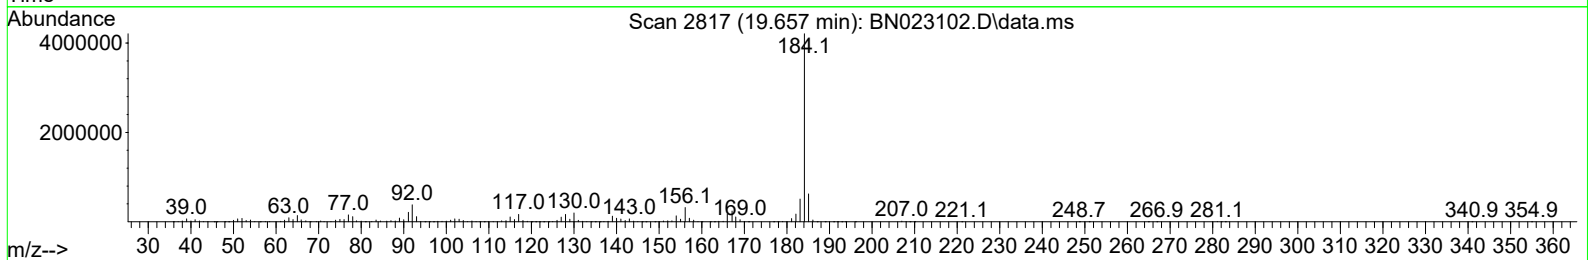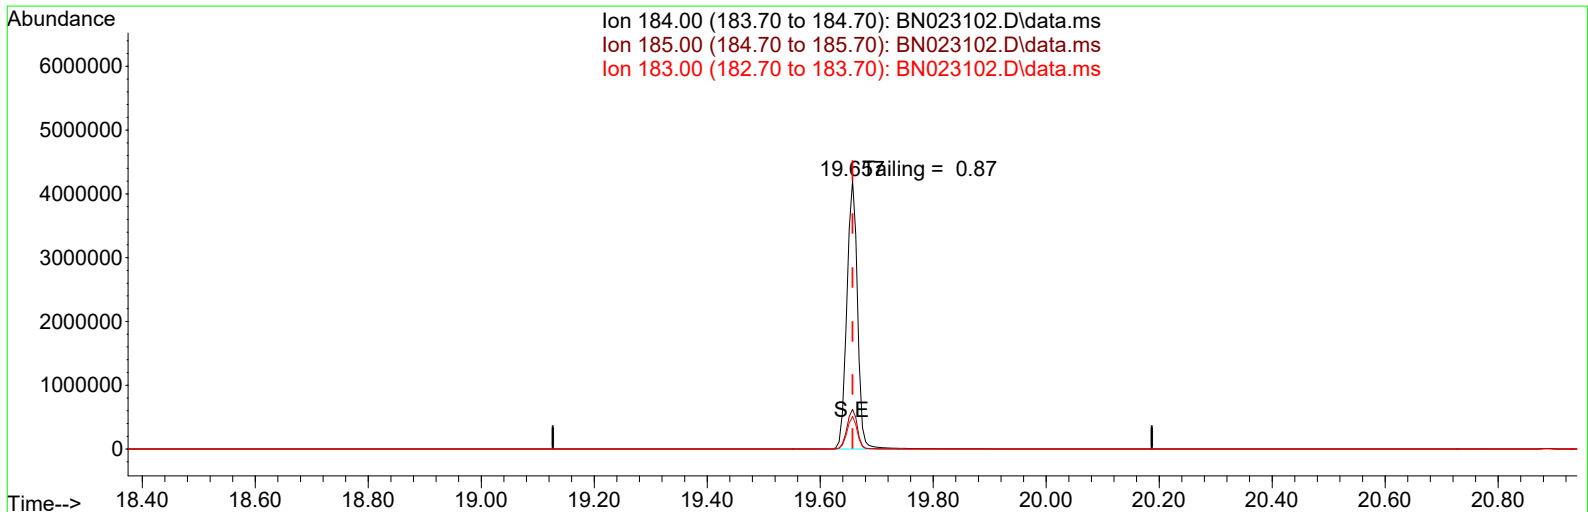

TIC: BN023102.D\data.ms

(77) Benzidine**19.657min (0.000) 1766858.15 ng****response 5500870**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.83
183.00	13.20	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/9/2022	BNA_N	<u>BN023102.D</u>
Compound Name	Response	Retention Time
DDT	2370349	20.886
DDD	20386	20.498
DDE	173	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20559	2390908	0.86

Instrument :
BNA_N
ClientSampleId :
DFTPP