
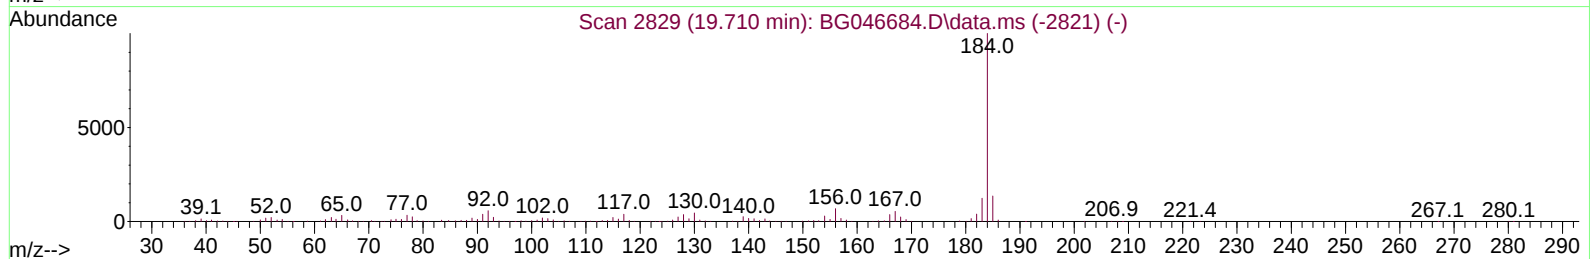
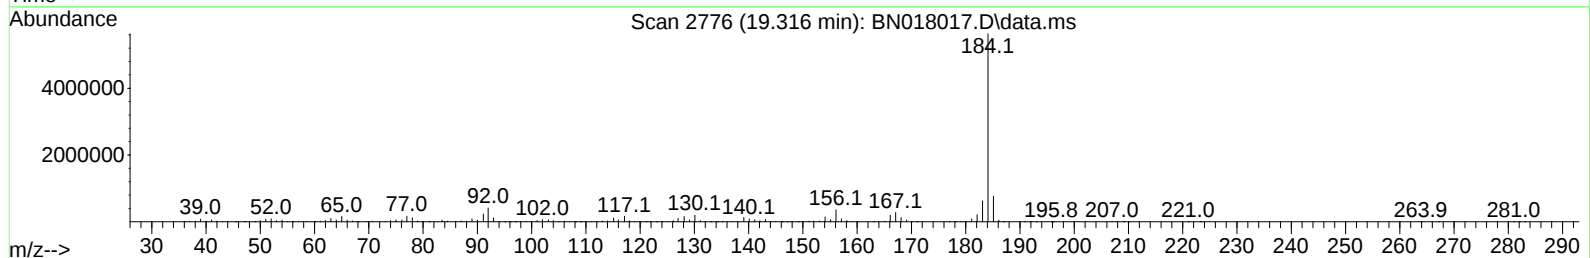


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121521\
Data File : BN018017.D
Acq On : 15 Dec 2021 08:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 10:33:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 10:33:24 2021
Response via : Initial Calibration

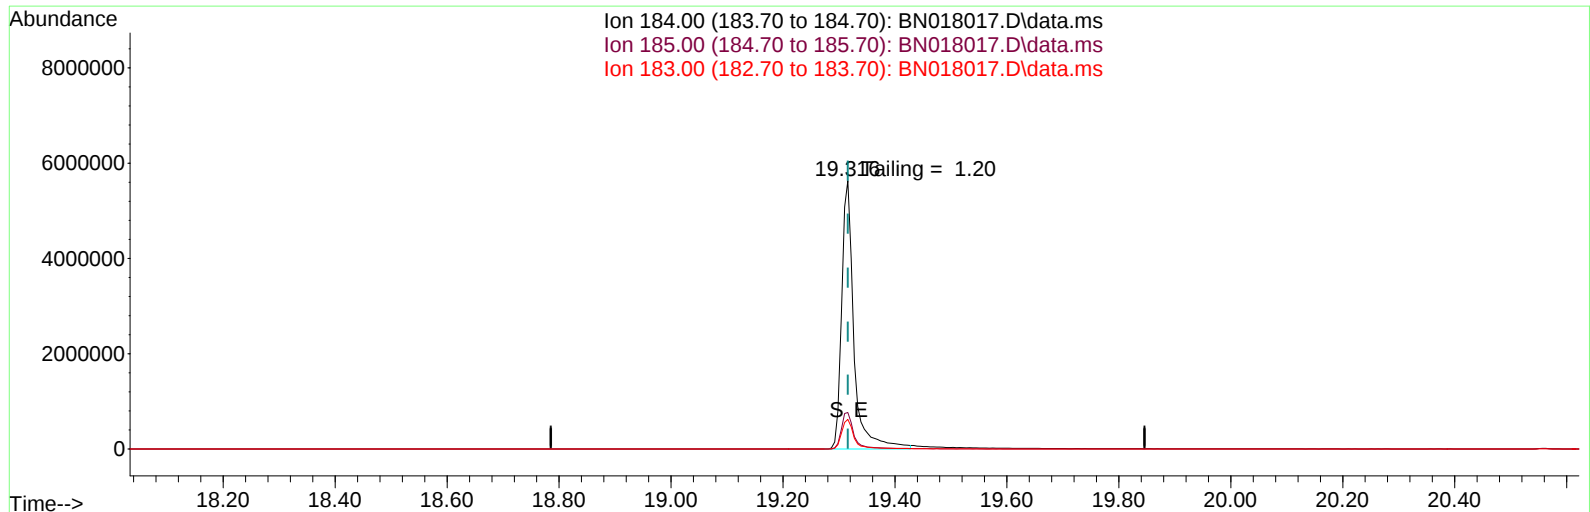

TIC: BN018017.D\data.ms

(77) Benzidine




19.316min (0.000) 0.00 ng

response 8943267

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.64
183.00	13.20	11.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121521\
Data File : BN018017.D
Acq On : 15 Dec 2021 08:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 10:33:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 10:33:24 2021
Response via : Initial Calibration

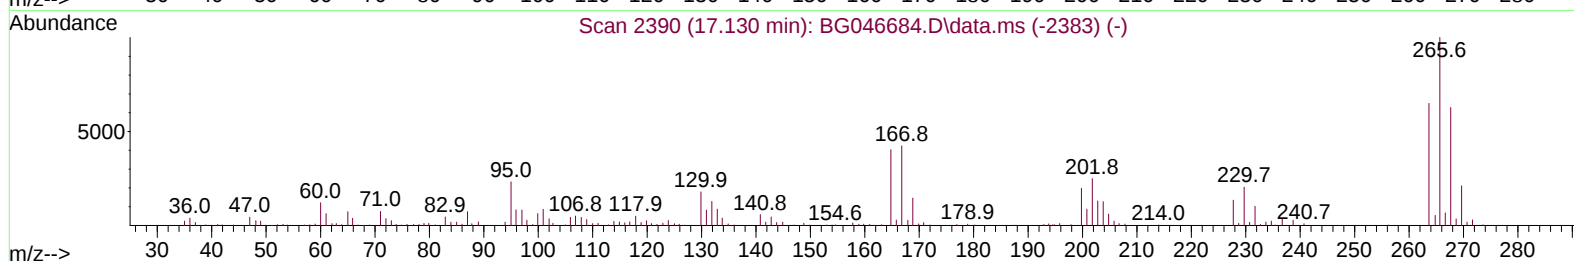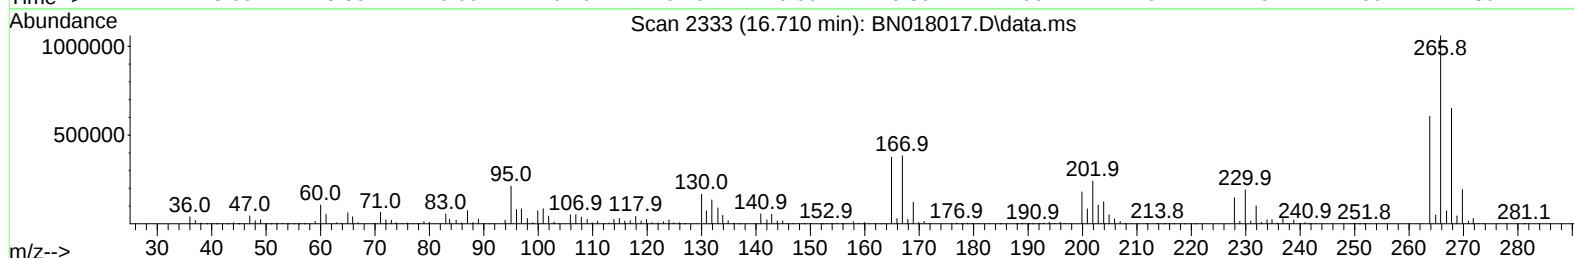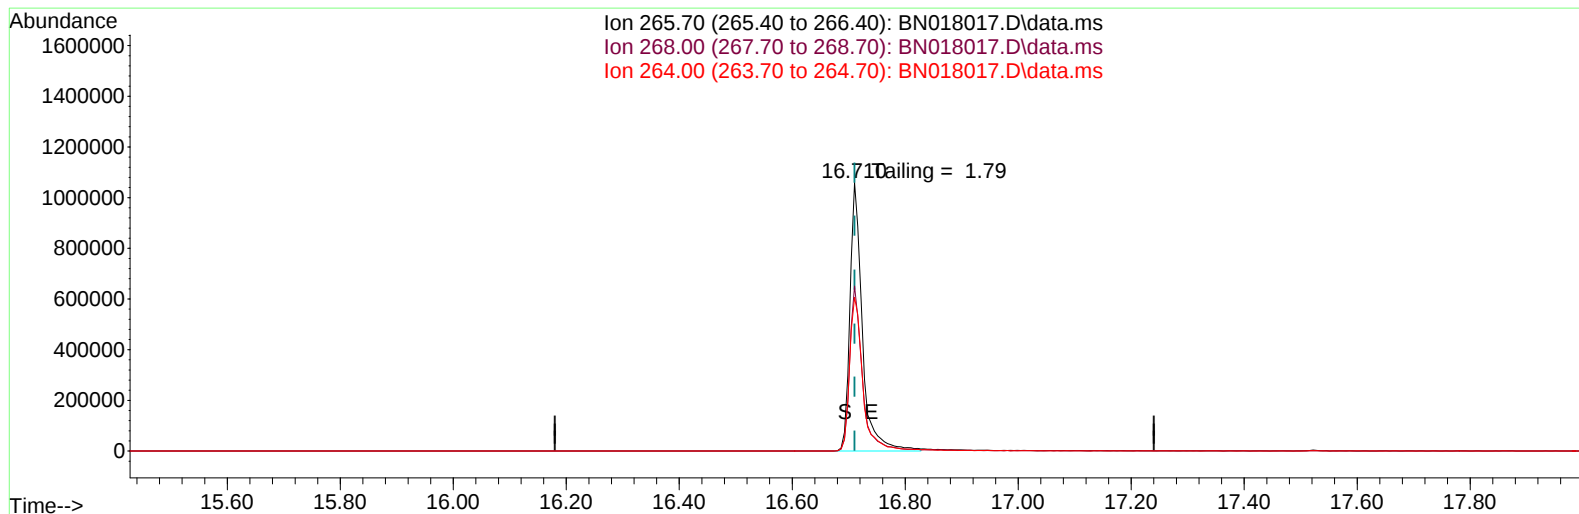

TIC: BN018017.D\data.ms

(70) Pentachlorophenol (C)

16.710min (0.000) 26971.42 ng

response 1656913

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.47
264.00	61.60	57.25
0.00	0.00	0.00