


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121521\
 Data File : BN018017.D
 Acq On : 15 Dec 2021 08:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 14 17:59:47 2021

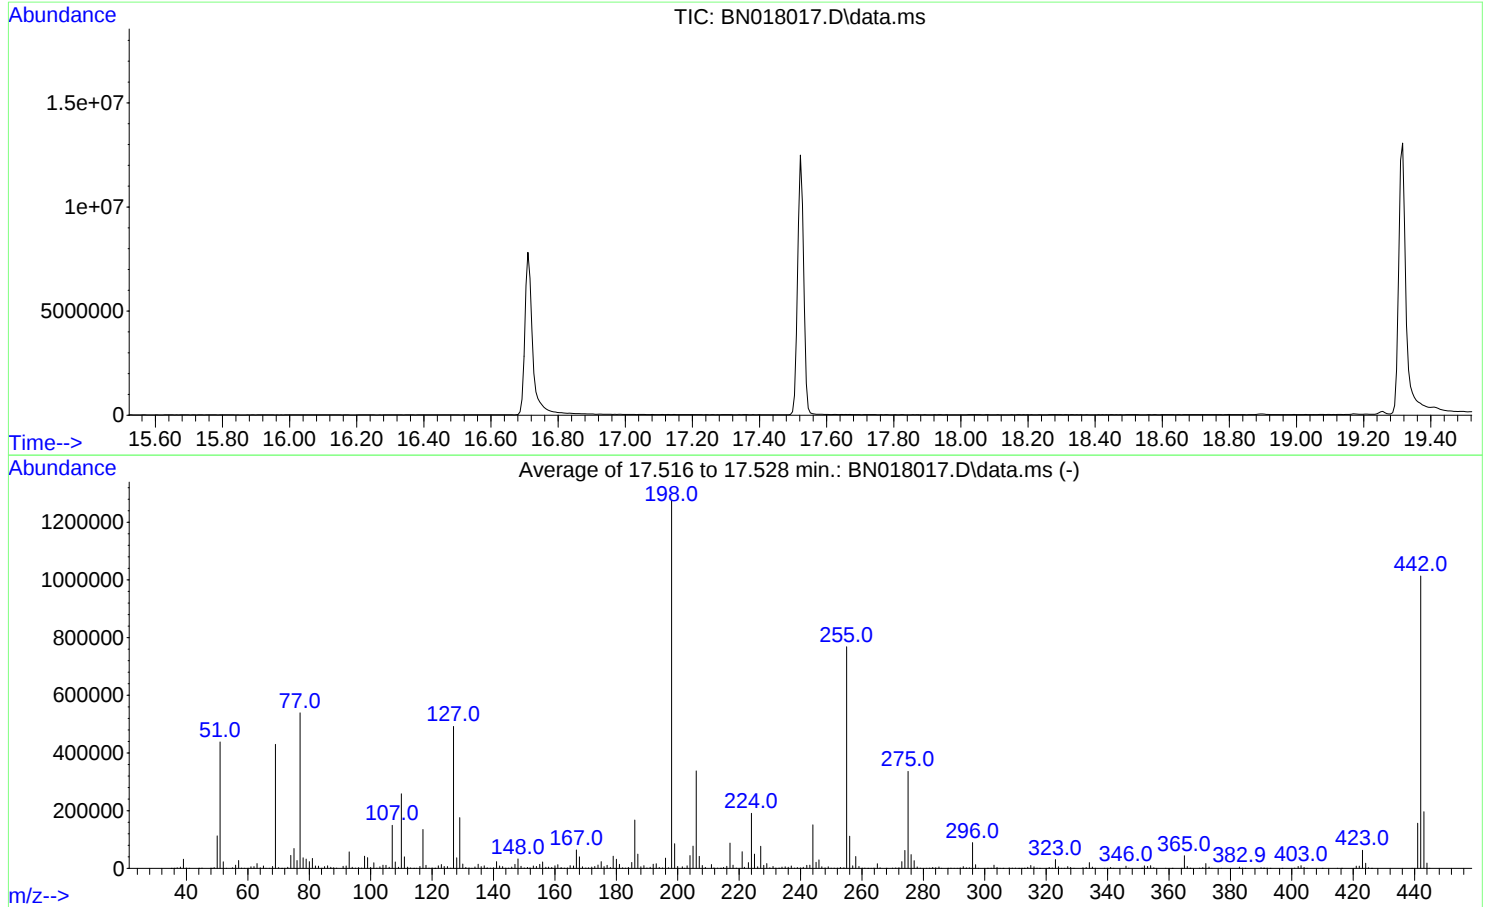

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	438571	PASS
68	69	0.00	2	1.6	6884	PASS
69	198	0.00	100	33.7	430187	PASS
70	69	0.00	2	0.6	2680	PASS
127	198	10	80	38.6	492224	PASS
197	198	0.00	2	0.2	2450	PASS
198	198	100	100	100.0	1275392	PASS
199	198	5	9	6.7	85323	PASS
275	198	10	60	26.4	336299	PASS
365	198	1	100	3.4	43611	PASS
441	198	0.01	100	12.3	156581	PASS
442	442	100	100	100.0	1013355	PASS
443	442	15	24	19.4	196435	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/15/2021	BNA_N	<u>BN018017.D</u>
Compound Name	Response	Retention Time
DDT	4350323	20.557
DDD	72409	20.116
DDE	4930	19.604
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
77339	4427662	1.75

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121521\
 Data File : BN018017.D
 Acq On : 15 Dec 2021 08:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 16 10:33:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 10:33:24 2021
 Response via : Initial Calibration

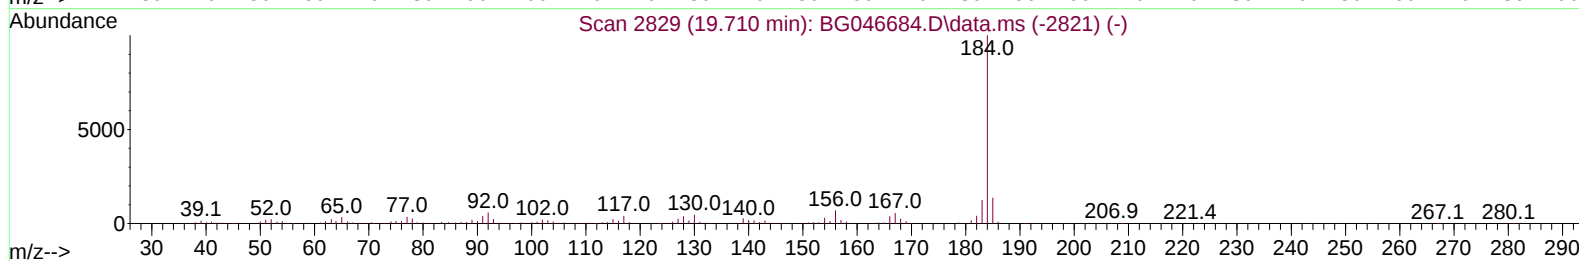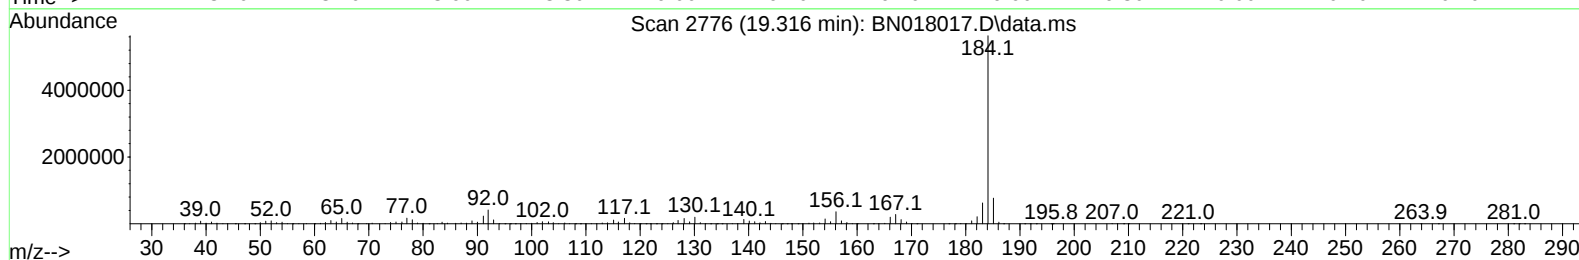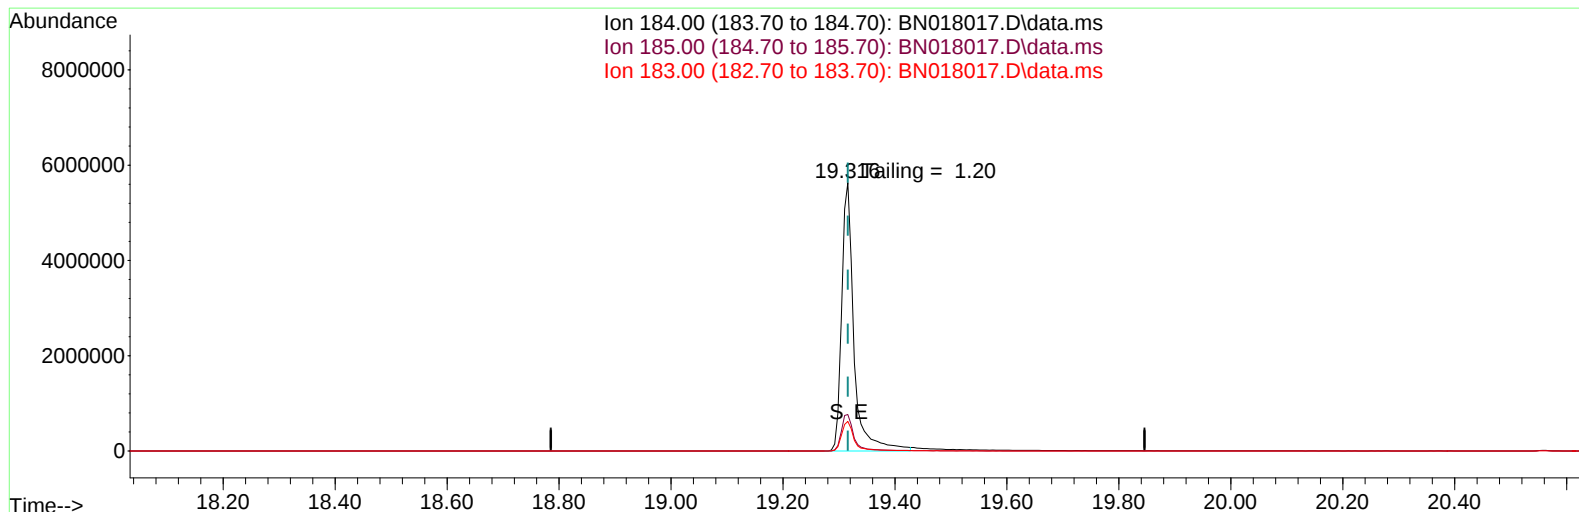

TIC: BN018017.D\data.ms

(77) Benzidine

19.316min (0.000) 0.00 ng




response 8943267

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.64
183.00	13.20	11.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121521\
 Data File : BN018017.D
 Acq On : 15 Dec 2021 08:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 16 10:33:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 10:33:24 2021
 Response via : Initial Calibration

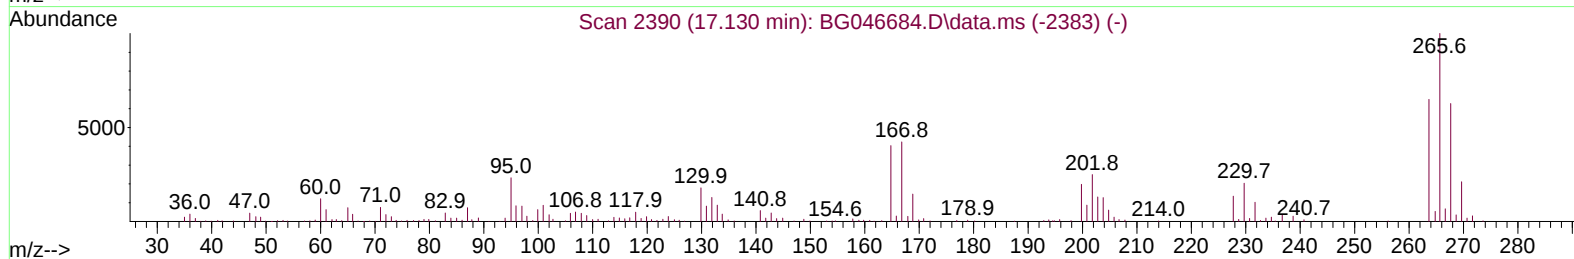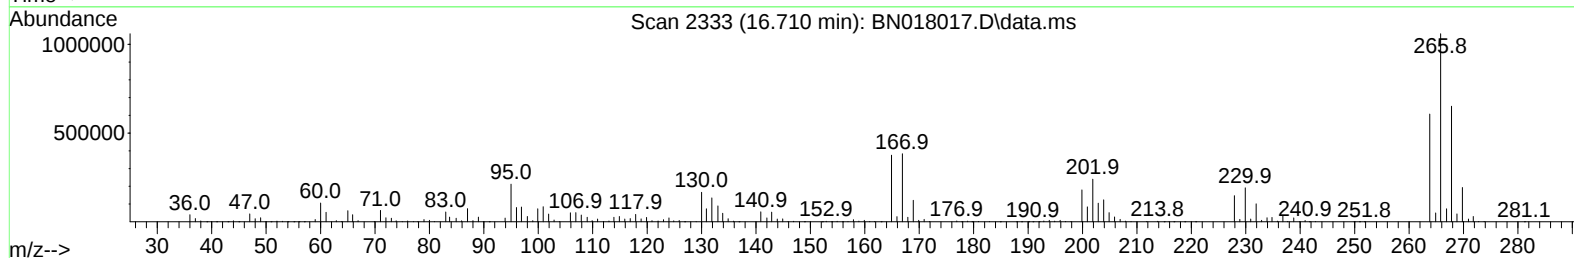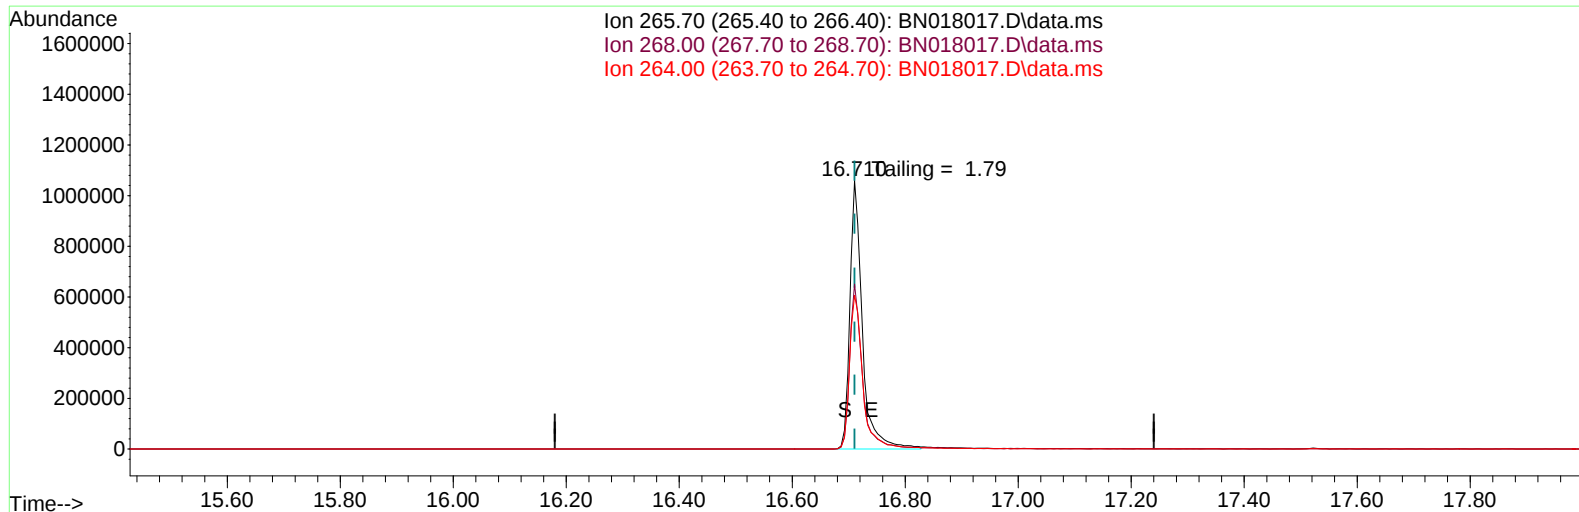

TIC: BN018017.D\data.ms

(70) Pentachlorophenol (C)

16.710min (0.000) 26971.42 ng

response 1656913

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.47
264.00	61.60	57.25
0.00	0.00	0.00