

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
 Data File : BN018033.D
 Acq On : 15 Dec 2021 20:20
 Operator : CG/JU
 Sample : M4995-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW5Q3

Quant Time: Dec 16 04:37:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 17:47:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.662	152	4669	0.400	ng/ul	0.00
4) Naphthalene-d8	10.447	136	15162	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.308	164	9834	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.053	188	22632	0.400	ng/ul	-0.01
17) Chrysene-d12	21.260	240	19591	0.400	ng/ul	# 0.00
23) Perylene-d12	23.522	264	23944	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	23847	4.920	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.053	152	7303	0.413	ng/ul	-0.01
18) Fluoranthene-d10	19.091	212	30785	0.551	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.172	88	59751	10.496	ng/ul#	42


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
Data File : BN018033.D
Acq On : 15 Dec 2021 20:20
Operator : CG/JU
Sample : M4995-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW5Q3


Quant Time: Dec 16 04:37:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 17:47:27 2021
Response via : Initial Calibration

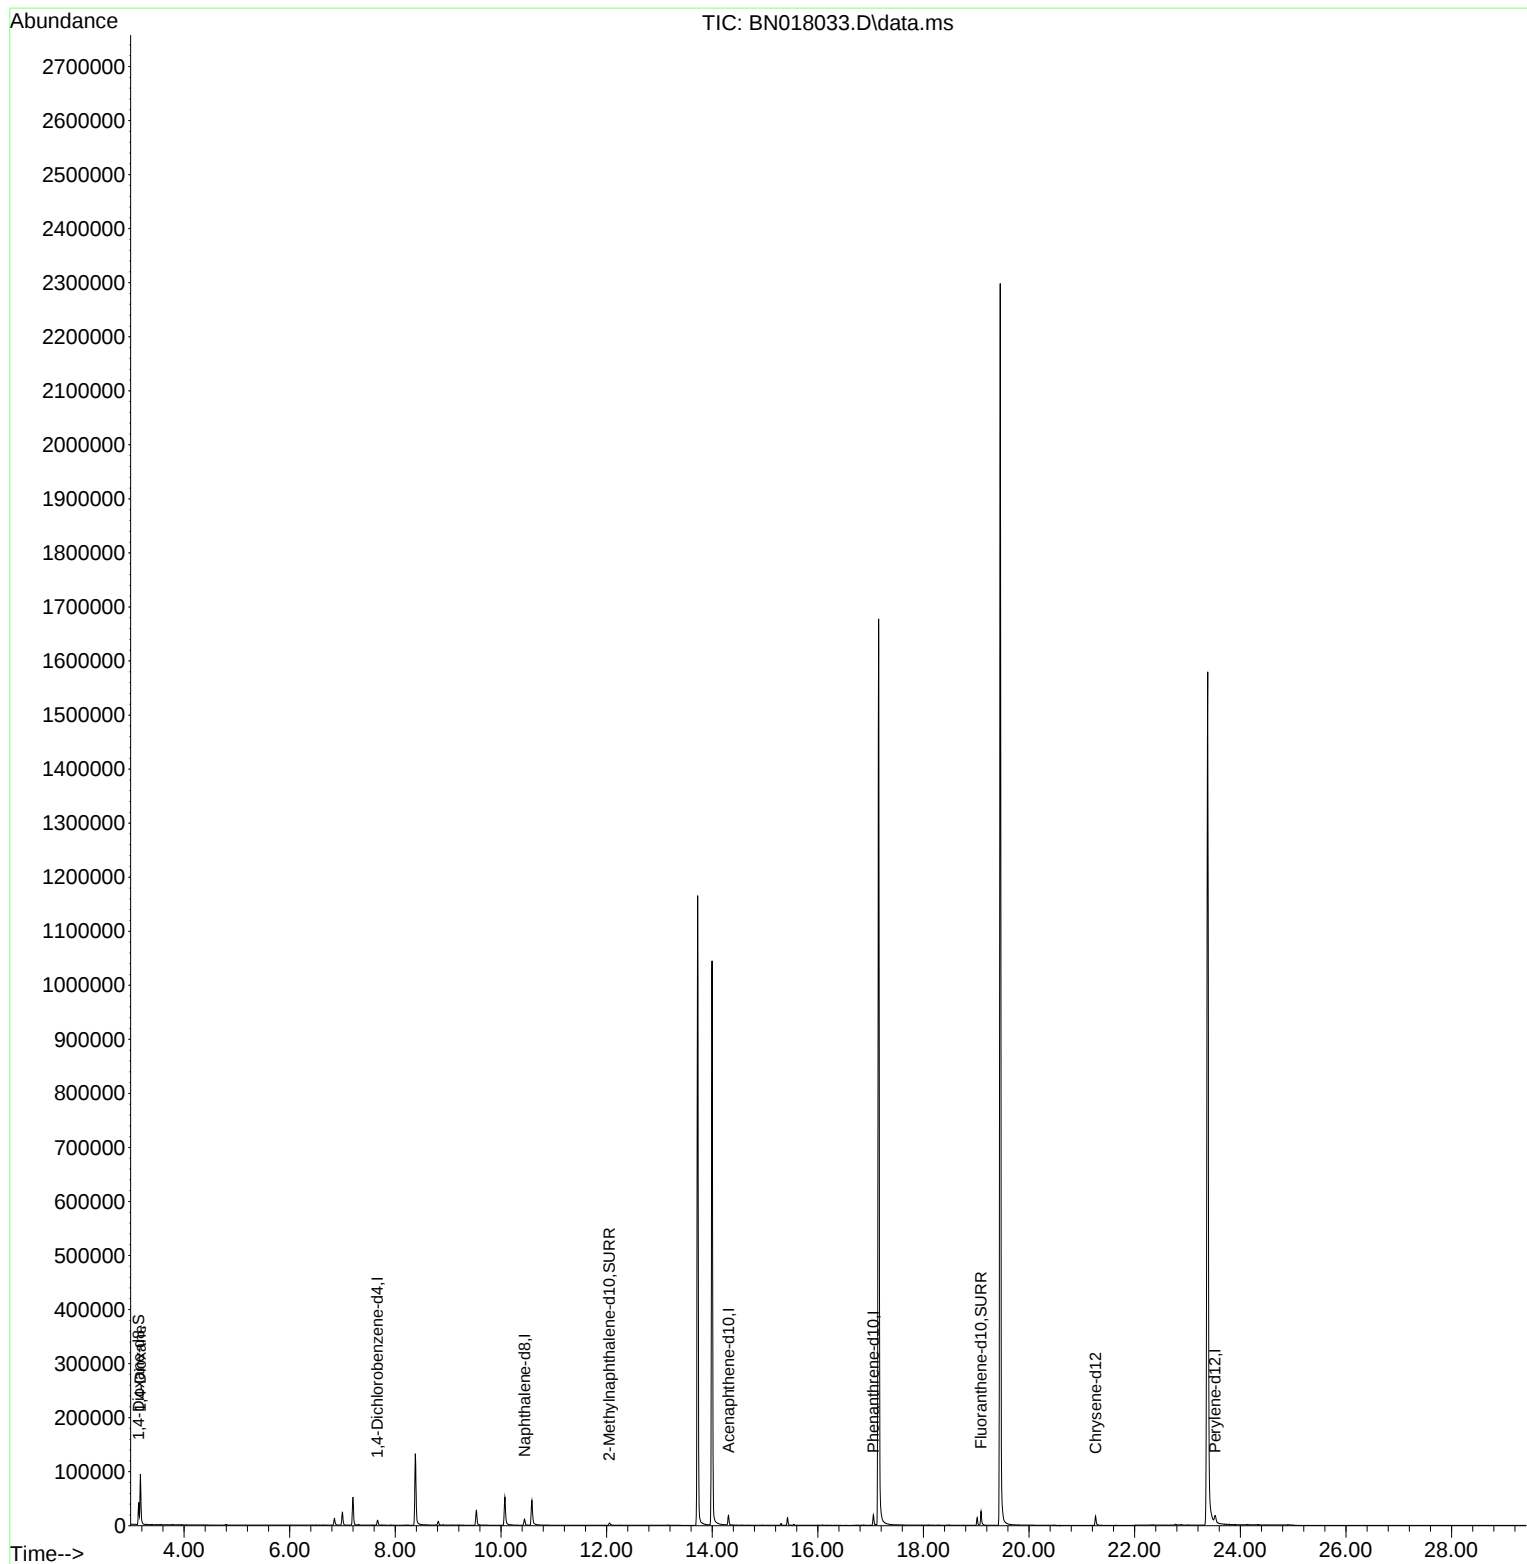

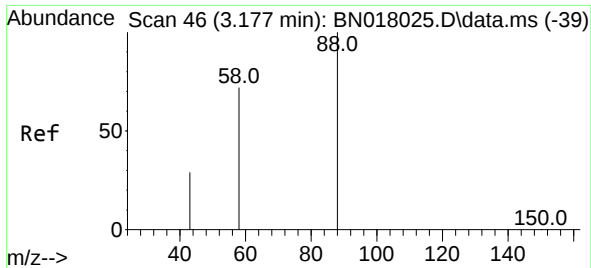

#2
 1,4-Dioxane
 Concen: 10.496 ng/ul
 RT: 3.172 min Scan# 41
 Delta R.T. -0.004 min
 Lab File: BN018033.D
 Acq: 15 Dec 2021 20:20

Instrument :
 BNA_N
 ClientSampleId :
 EW5Q3

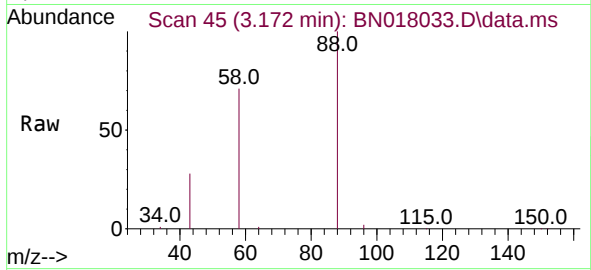

Tgt Ion: 88 Resp: 59751
 Ion Ratio Lower Upper
 88 100
 43 28.2 85.8 128.6#
 58 71.1 43.4 65.0#

