

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
 Data File : BN018041.D
 Acq On : 16 Dec 2021 01:45
 Operator : CG/JU
 Sample : M4985-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW5S6

Quant Time: Dec 16 04:45:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 17:47:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.662	152	7628	0.400	ng/ul	0.00
4) Naphthalene-d8	10.447	136	24813	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.308	164	16691	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.053	188	39499	0.400	ng/ul	-0.01
17) Chrysene-d12	21.257	240	37865	0.400	ng/ul	# 0.00
23) Perylene-d12	23.525	264	39887	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	36527	4.613	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.053	152	12440	0.430	ng/ul	-0.01
18) Fluoranthene-d10	19.091	212	49987	0.463	ng/ul	-0.01
Target Compounds						
						Qvalue
5) Naphthalene	10.497	128	4233	0.062	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
Data File : BN018041.D
Acq On : 16 Dec 2021 01:45
Operator : CG/JU
Sample : M4985-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW5S6


Quant Time: Dec 16 04:45:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 17:47:27 2021
Response via : Initial Calibration

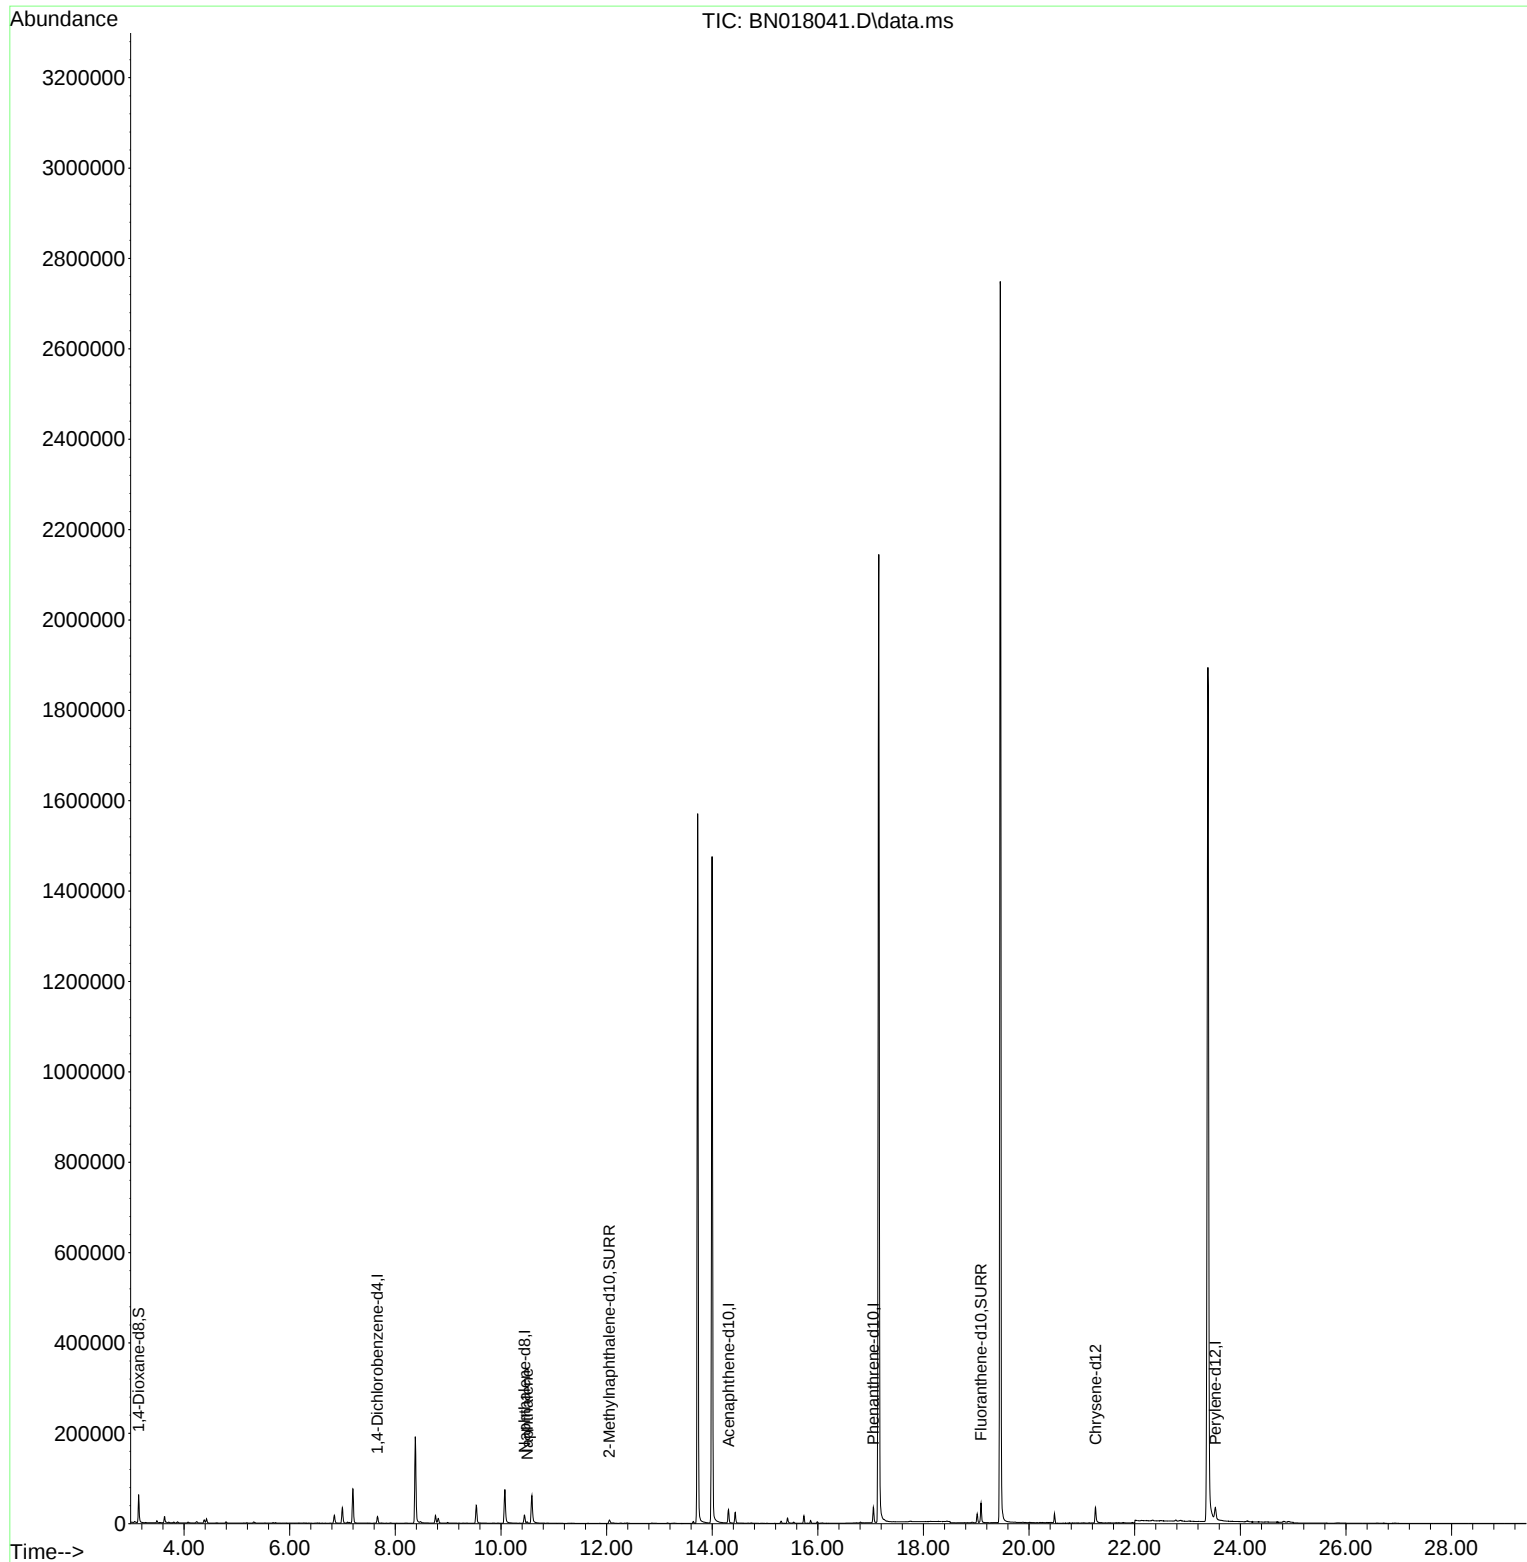

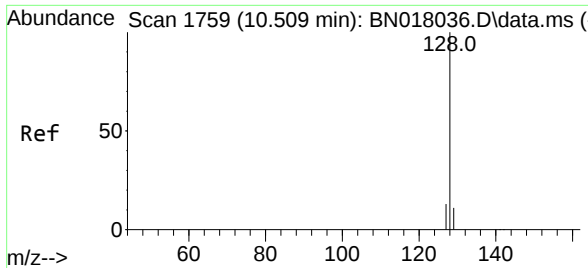

#5
Naphthalene
Concen: 0.062 ng/ul
RT: 10.497 min Scan# 11
Delta R.T. -0.012 min
Lab File: BN018041.D
Acq: 16 Dec 2021 01:45

Instrument :
BNA_N
ClientSampleId :
EW5S6

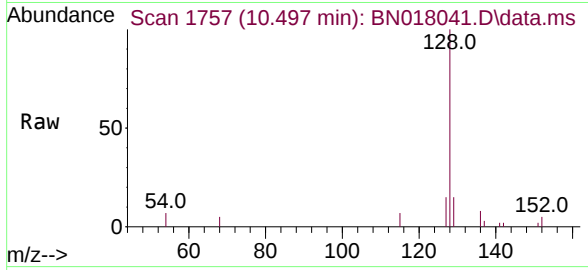

Tgt Ion:	128	Resp:	4233
Ion	Ratio	Lower	Upper
128	100		
129	15.2	10.4	15.6
127	15.4	11.8	17.6

