

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
 Data File : BN018058.D
 Acq On : 16 Dec 2021 12:35
 Operator : CG/JU
 Sample : M5037-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C00V7

Quant Time: Dec 17 02:12:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 17:47:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.662	152	4745	0.400	ng/ul	0.00
4) Naphthalene-d8	10.448	136	15414	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.308	164	10072	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.053	188	22675	0.400	ng/ul	-0.01
17) Chrysene-d12	21.263	240	18650	0.400	ng/ul	# 0.00
23) Perylene-d12	23.525	264	21547	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	21887	4.443	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.059	152	6591	0.367	ng/ul	0.00
18) Fluoranthene-d10	19.091	212	23895	0.449	ng/ul	-0.01
Target Compounds						
					Qvalue	
5) Naphthalene	10.497	128	1294	0.031	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
Data File : BN018058.D
Acq On : 16 Dec 2021 12:35
Operator : CG/JU
Sample : M5037-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C00V7

Quant Time: Dec 17 02:12:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 17:47:27 2021
Response via : Initial Calibration

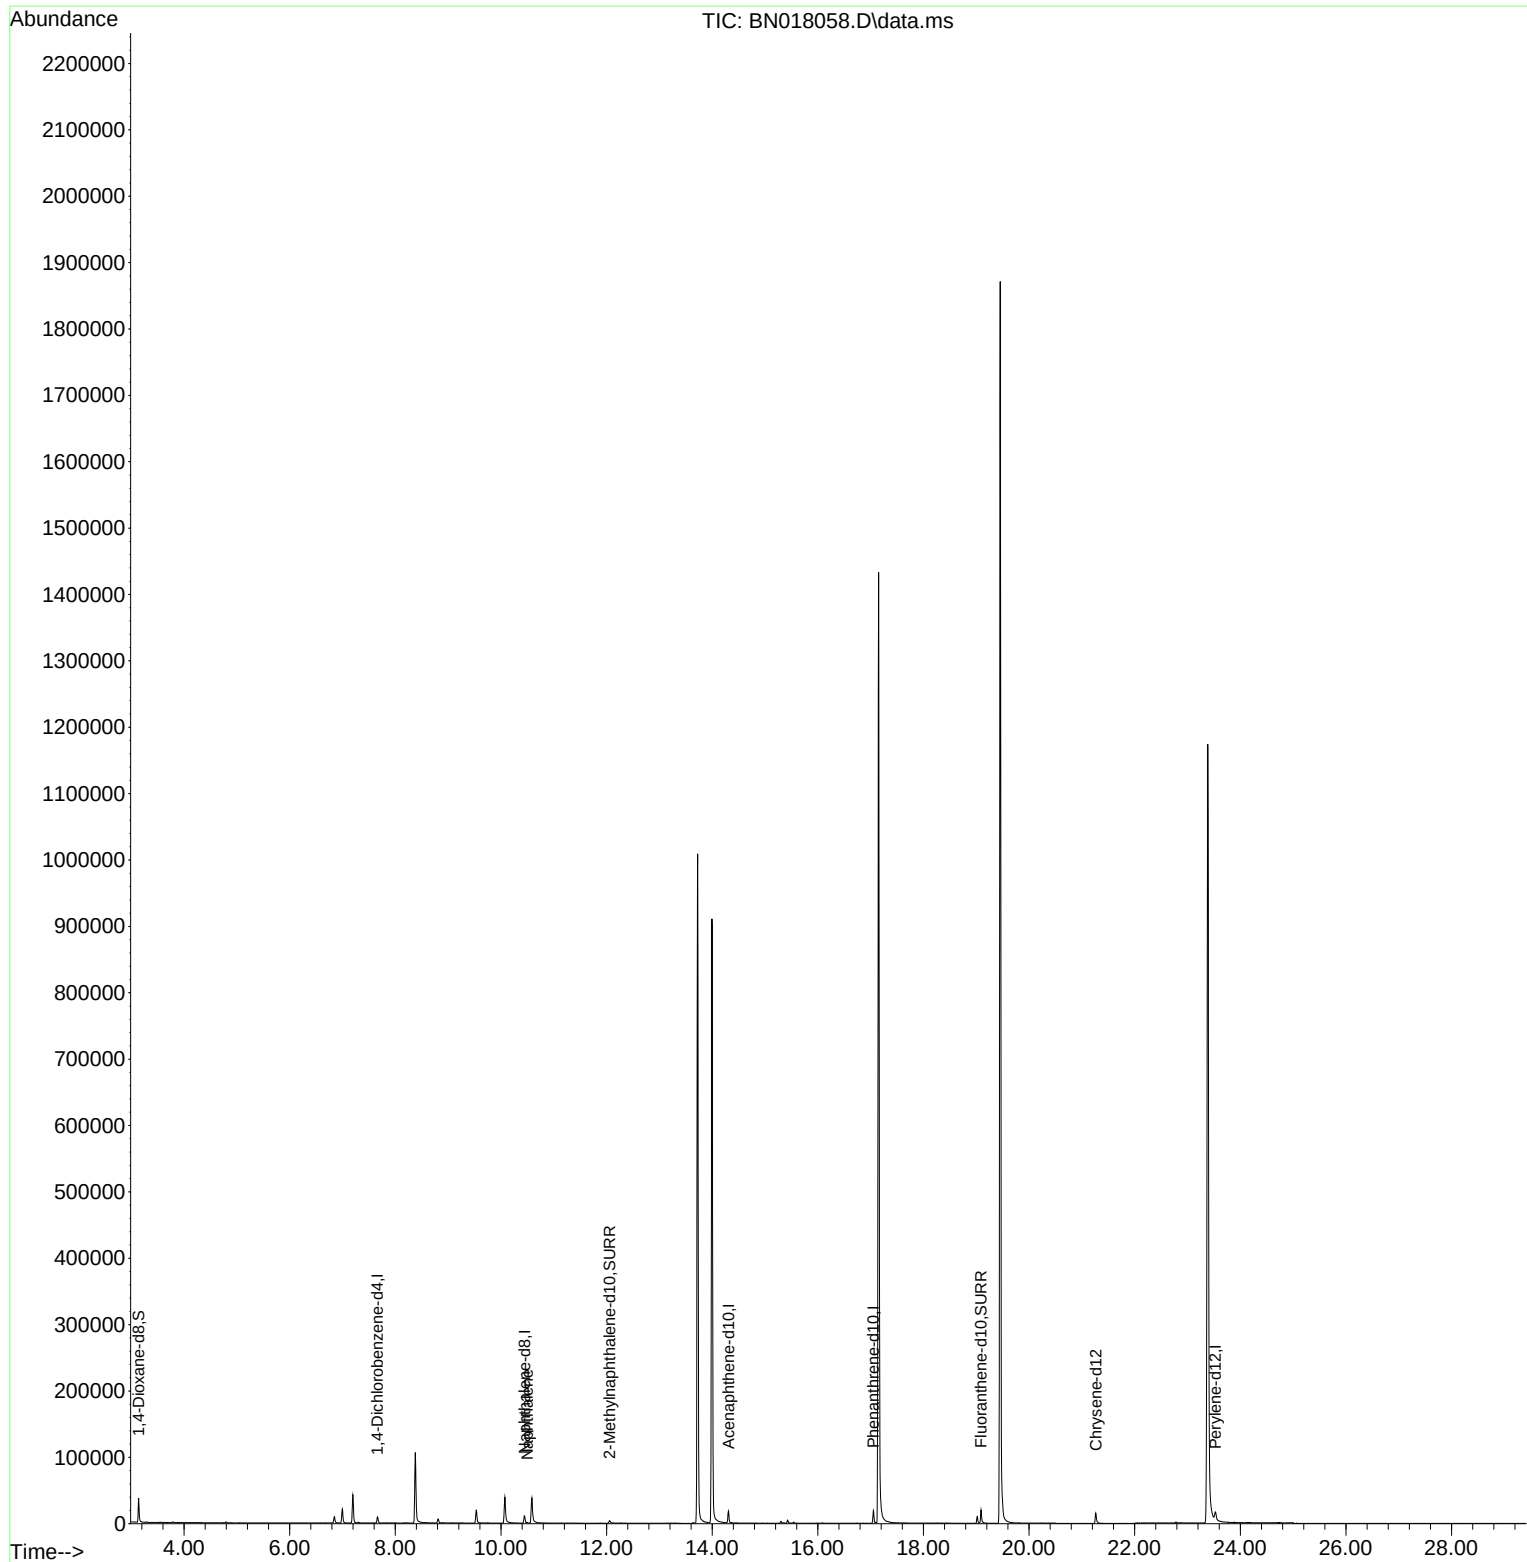

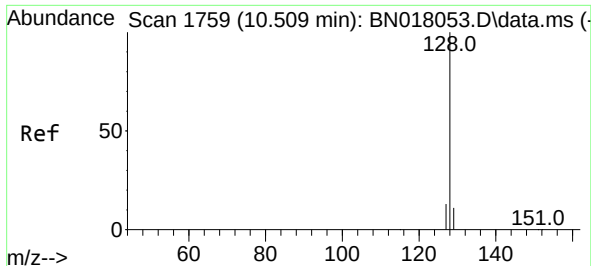

#5

Naphthalene

Concen: 0.031 ng/ul

RT: 10.497 min Scan# 11

Delta R.T. -0.012 min

Lab File: BN018058.D


Acq: 16 Dec 2021 12:35

Instrument :

BNA_N

ClientSampleId :

C00V7

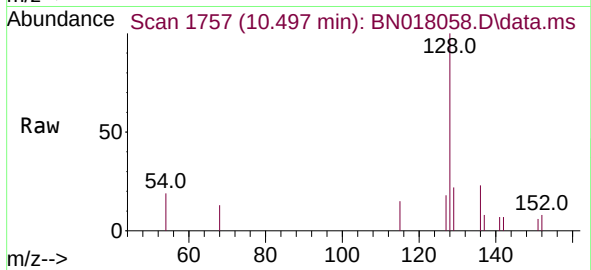

Tgt Ion:128 Resp: 1294

Ion Ratio Lower Upper

128 100

129 22.1 10.4 15.6#

127 17.7 11.8 17.6#

