

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
 Data File : BN018060.D
 Acq On : 16 Dec 2021 13:48
 Operator : CG/JU
 Sample : M5037-04
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C00V9

Quant Time: Dec 17 02:12:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 17:47:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.662	152	4635	0.400	ng/ul	0.00
4) Naphthalene-d8	10.443	136	14946	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.309	164	9691	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.054	188	21619	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.264	240	17712	0.400	ng/ul	# 0.00
23) Perylene-d12	23.527	264	21444	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	21739	4.518	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.060	152	6558	0.377	ng/ul	0.00
18) Fluoranthene-d10	19.092	212	25163	0.498	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.493	128	2563	0.063	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
Data File : BN018060.D
Acq On : 16 Dec 2021 13:48
Operator : CG/JU
Sample : M5037-04
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C00V9


Quant Time: Dec 17 02:12:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 17:47:27 2021
Response via : Initial Calibration

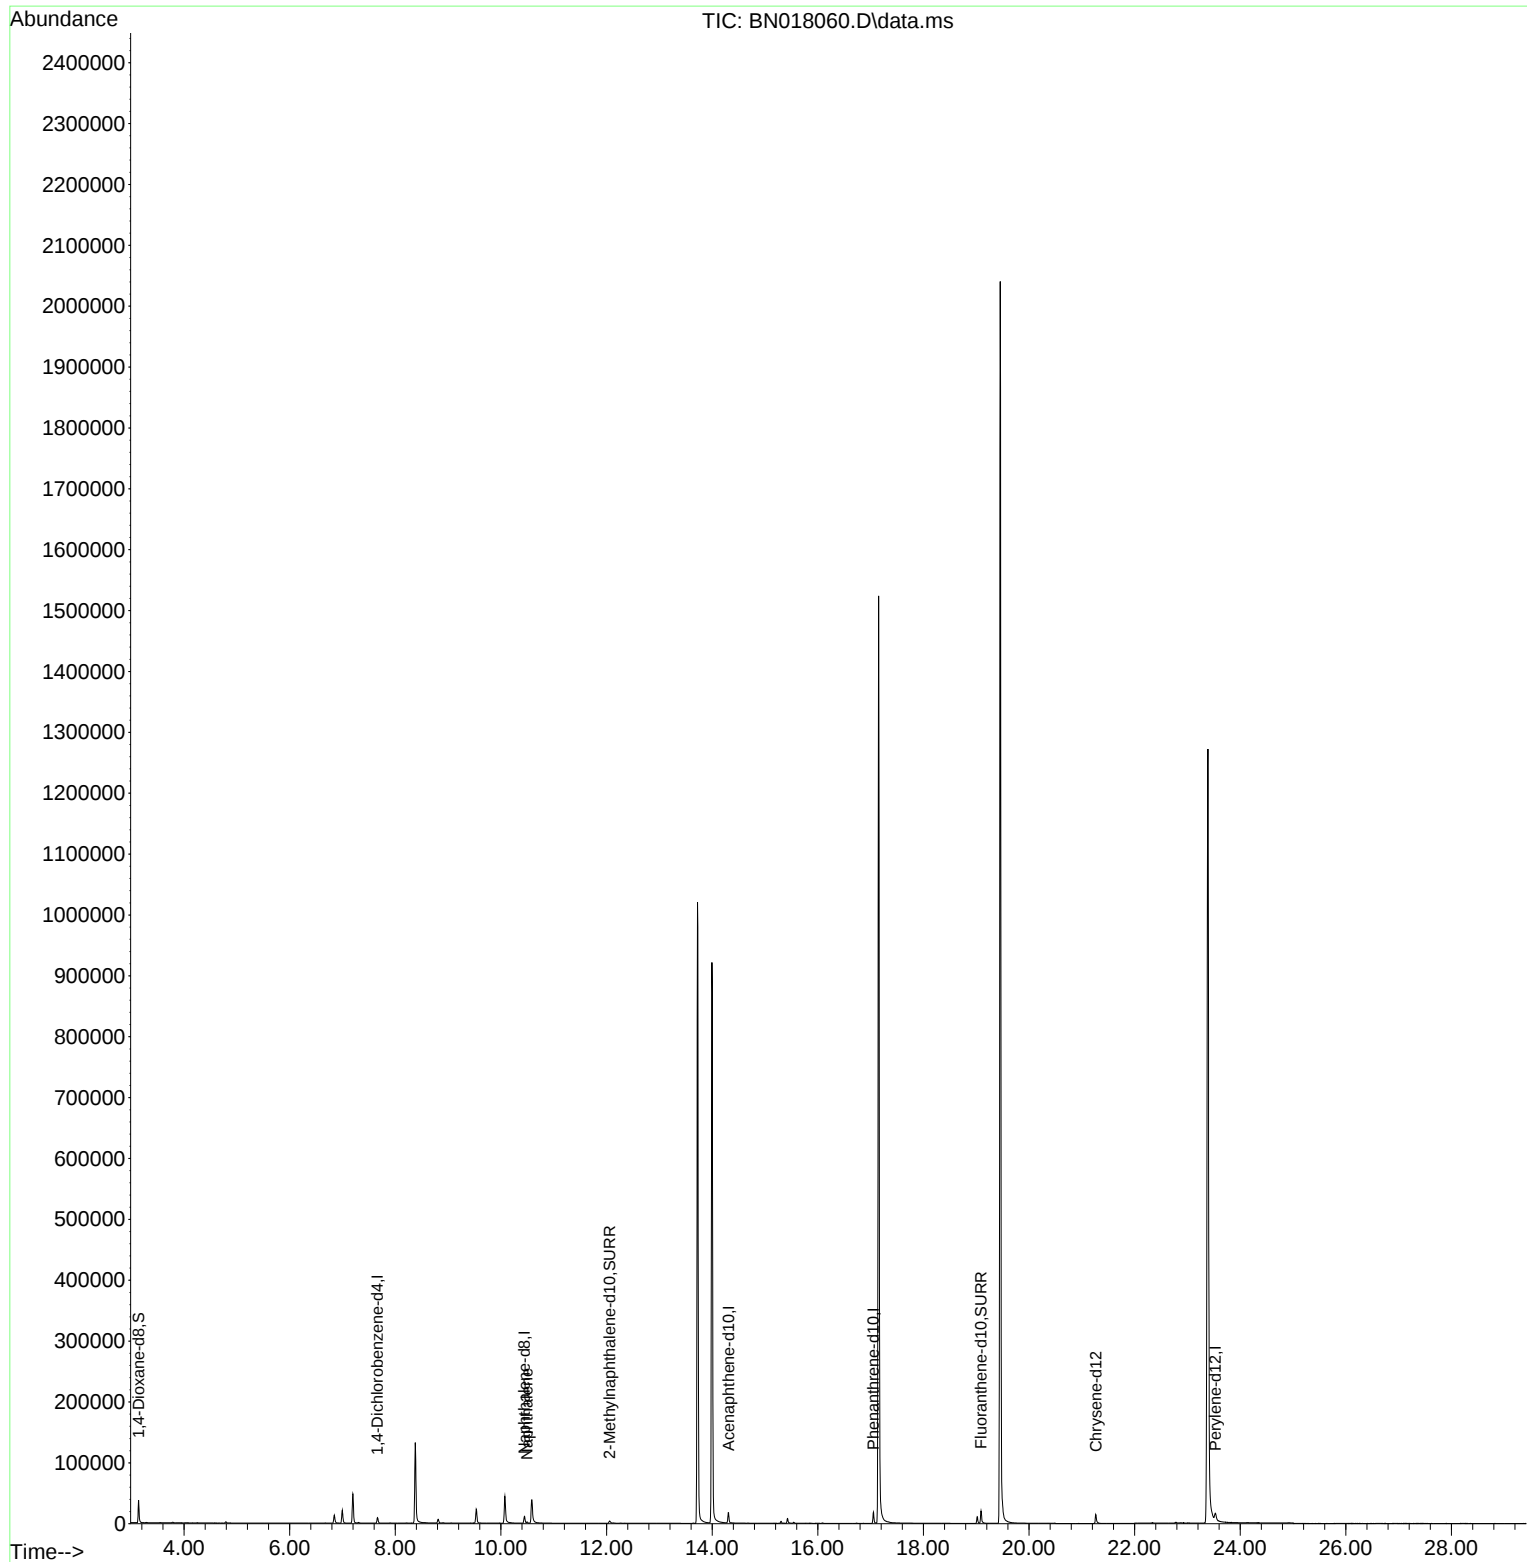

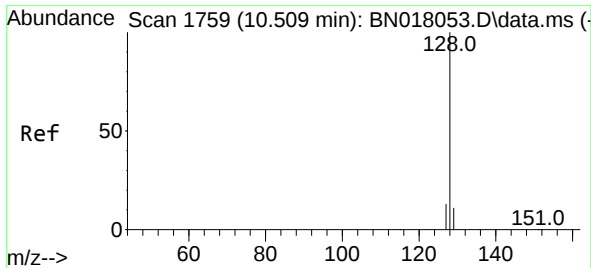

#5
Naphthalene
Concen: 0.063 ng/ul
RT: 10.493 min Scan# 11
Delta R.T. -0.017 min
Lab File: BN018060.D
Acq: 16 Dec 2021 13:48

Instrument :
BNA_N
ClientSampleId :
C00V9

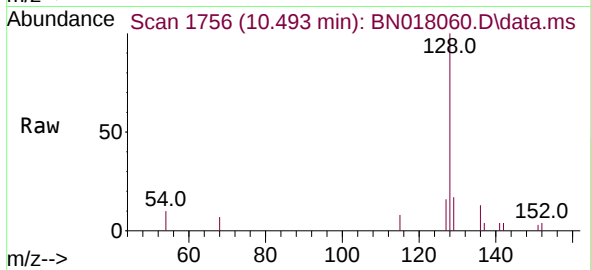

Tgt Ion:128 Resp: 2563
Ion Ratio Lower Upper
128 100
129 17.0 10.4 15.6#
127 16.1 11.8 17.6

