

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
 Data File : BN018061.D
 Acq On : 16 Dec 2021 14:24
 Operator : CG/JU
 Sample : M5037-02
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C00V5

Quant Time: Dec 17 02:12:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 17:47:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.662	152	4547	0.400	ng/ul	0.00
4) Naphthalene-d8	10.443	136	14688	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.305	164	9501	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.054	188	22257	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.259	240	20128	0.400	ng/ul	# 0.00
23) Perylene-d12	23.524	264	22235	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	25063	5.310	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.049	152	6327	0.370	ng/ul	-0.02
18) Fluoranthene-d10	19.092	212	25048	0.437	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.493	128	1530	0.038	ng/ul#	88
16) Anthracene	17.185	178	1250	0.021	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
Data File : BN018061.D
Acq On : 16 Dec 2021 14:24
Operator : CG/JU
Sample : M5037-02
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C00V5


Quant Time: Dec 17 02:12:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 17:47:27 2021
Response via : Initial Calibration

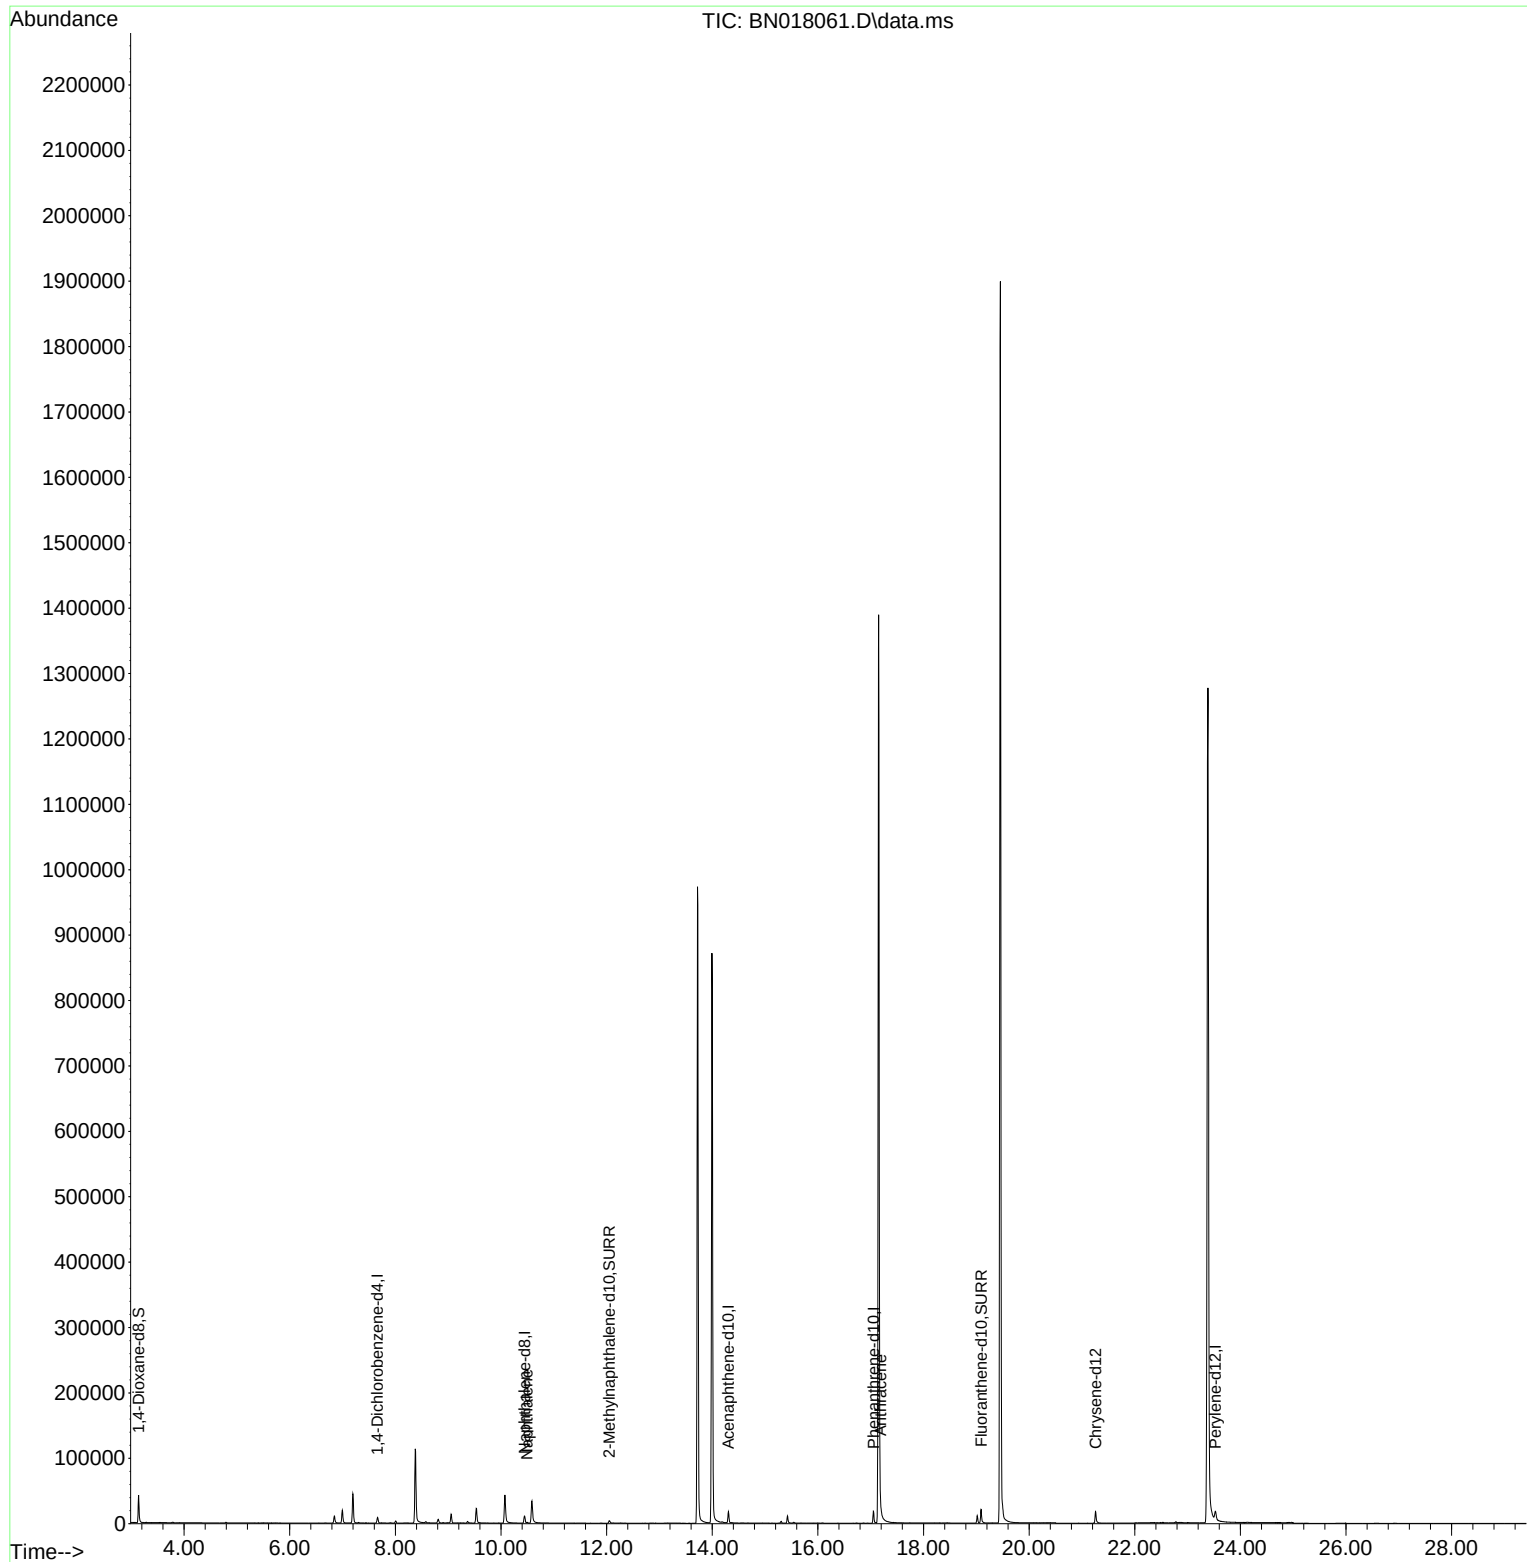



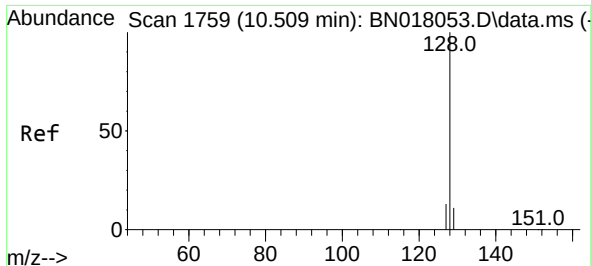


#5
Naphthalene
Concen: 0.038 ng/ul
RT: 10.493 min Scan# 1756
Delta R.T. -0.017 min
Lab File: BN018061.D
Acq: 16 Dec 2021 14:24

Instrument :
BNA_N
ClientSampleId :
C00V5

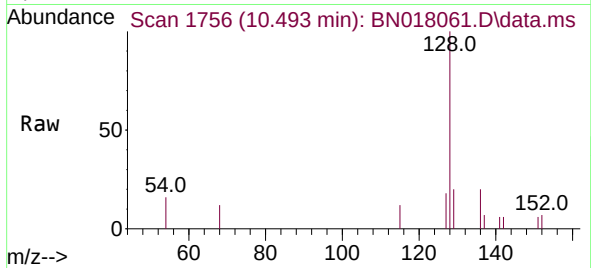

Tgt Ion:128 Resp: 1530
Ion Ratio Lower Upper
128 100
129 20.2 10.4 15.6#
127 17.7 11.8 17.6#

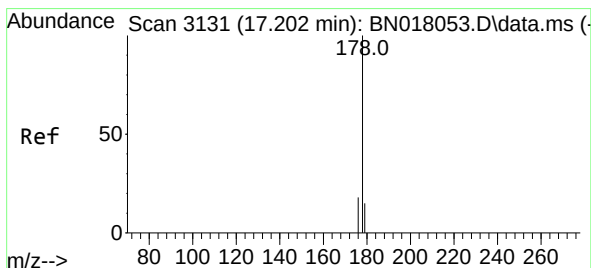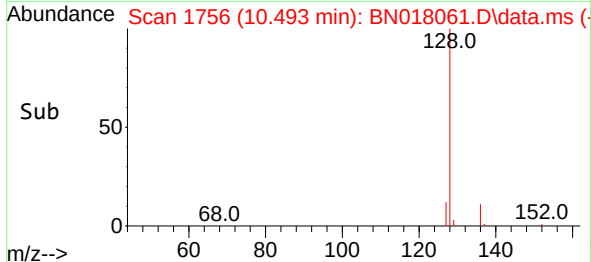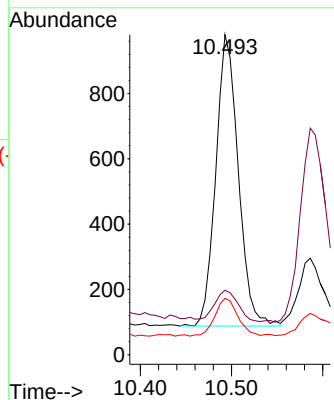

#16
Anthracene
Concen: 0.021 ng/ul
RT: 17.185 min Scan# 3127
Delta R.T. -0.021 min
Lab File: BN018061.D
Acq: 16 Dec 2021 14:24

Tgt Ion:178 Resp: 1250
Ion Ratio Lower Upper
178 100
179 31.2 13.3 19.9#
176 29.7 15.1 22.7#

