

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
 Data File : BN018074.D
 Acq On : 16 Dec 2021 22:53
 Operator : CG/JU
 Sample : M4971-10
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3D9

Quant Time: Dec 17 02:25:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 17:47:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.661	152	4554	0.400	ng/ul	0.00
4) Naphthalene-d8	10.442	136	13867	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.308	164	8734	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.053	188	16929	0.400	ng/ul	-0.01
17) Chrysene-d12	21.266	240	11824	0.400	ng/ul	# 0.00
23) Perylene-d12	23.531	264	14146	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.138	96	26066	5.514	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.053	152	7391	0.457	ng/ul	-0.01
18) Fluoranthene-d10	19.091	212	19018	0.564	ng/ul	-0.01
Target Compounds						
						Qvalue
5) Naphthalene	10.491	128	5889	0.155	ng/ul	99
7) 2-Methylnaphthalene	12.124	142	1159	0.054	ng/ul	99
8) 1-Methylnaphthalene	12.339	142	688	0.028	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
Data File : BN018074.D
Acq On : 16 Dec 2021 22:53
Operator : CG/JU
Sample : M4971-10
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3D9


Quant Time: Dec 17 02:25:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 17:47:27 2021
Response via : Initial Calibration

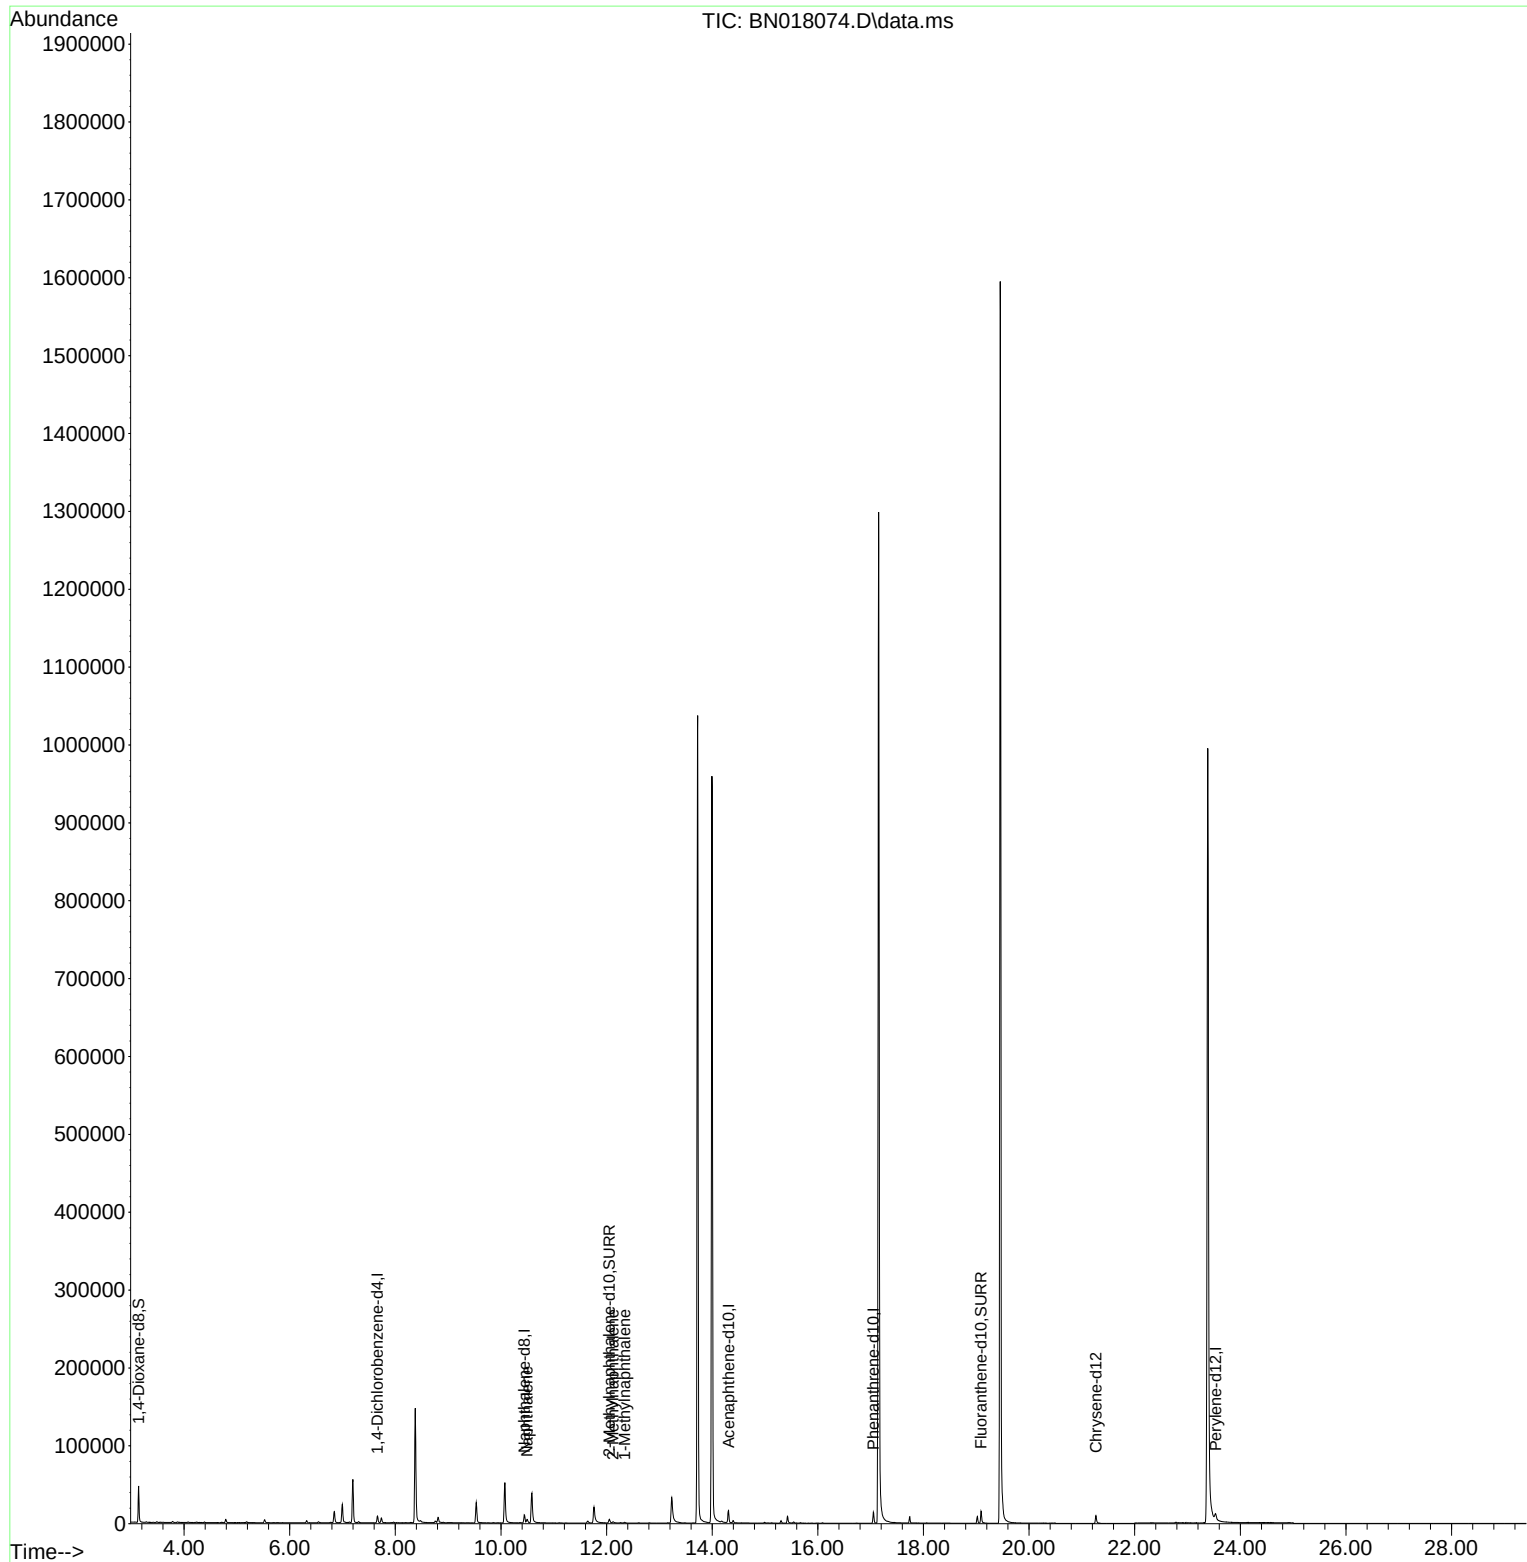



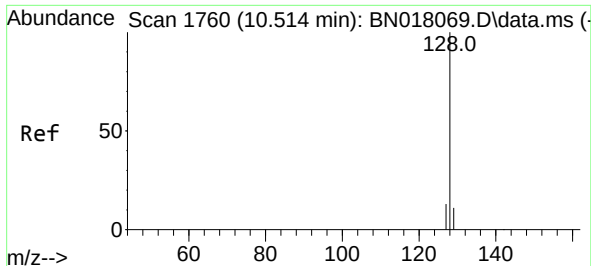


#5
Naphthalene
Concen: 0.155 ng/ul
RT: 10.491 min Scan# 1756
Delta R.T. -0.018 min
Lab File: BN018074.D
Acq: 16 Dec 2021 22:53

Instrument :
BNA_N
ClientSampleId :
BG3D9



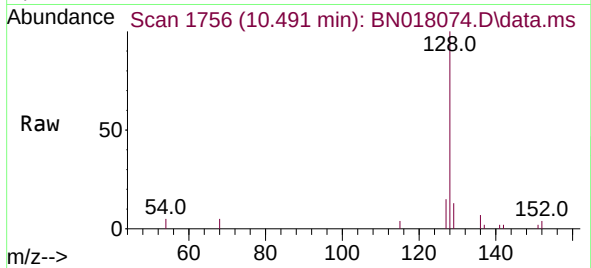



Tgt Ion:	128	Resp:	5889
Ion Ratio	Lower	Upper	
128	100		
129	13.1	10.4	15.6
127	15.0	11.8	17.6

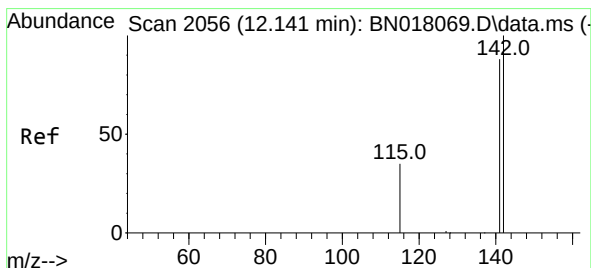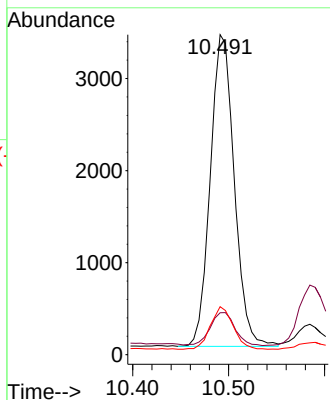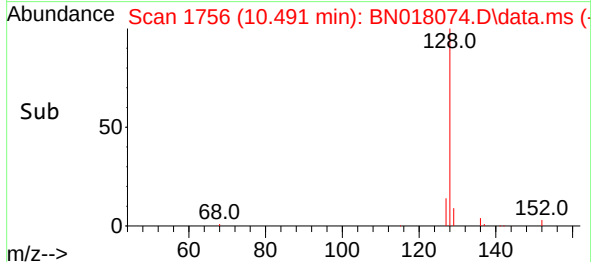

#7
2-Methylnaphthalene
Concen: 0.054 ng/ul
RT: 12.124 min Scan# 2053
Delta R.T. -0.013 min
Lab File: BN018074.D
Acq: 16 Dec 2021 22:53

Tgt Ion:	142	Resp:	1159
Ion Ratio	Lower	Upper	
142	100		
141	90.5	71.5	107.3

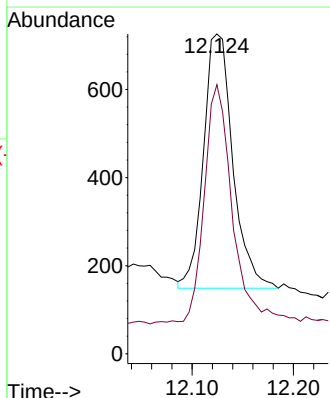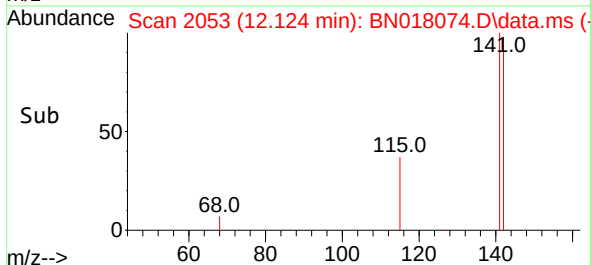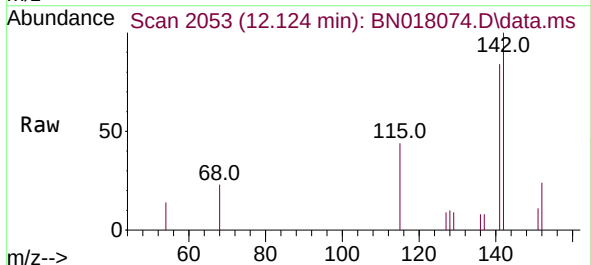

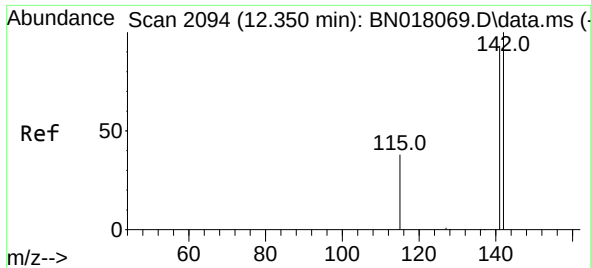

#8
 1-Methylnaphthalene
 Concen: 0.028 ng/ul
 RT: 12.339 min Scan# 2092
 Delta R.T. -0.013 min
 Lab File: BN018074.D
 Acq: 16 Dec 2021 22:53

Instrument :
 BNA_N
 ClientSampleId :
 BG3D9

Tgt Ion:142 Resp: 688
 Ion Ratio Lower Upper
 142 100
 141 92.7 73.3 109.9

