

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
 Data File : BN018077.D
 Acq On : 17 Dec 2021 00:42
 Operator : CG/JU
 Sample : M4971-09
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3D7

Quant Time: Dec 17 03:05:45 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 17:47:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.662	152	5066	0.400	ng/ul	0.00
4) Naphthalene-d8	10.442	136	16729	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.308	164	11080	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.053	188	24467	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.266	240	19969	0.400	ng/ul	# 0.00
23) Perylene-d12	23.528	264	24219	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	26902	5.115	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.053	152	8475	0.435	ng/ul	-0.01
18) Fluoranthene-d10	19.091	212	31145	0.547	ng/ul	-0.01
Target Compounds						
					Qvalue	
5) Naphthalene	10.491	128	1025	0.022	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
Data File : BN018077.D
Acq On : 17 Dec 2021 00:42
Operator : CG/JU
Sample : M4971-09
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3D7


Quant Time: Dec 17 03:05:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 17:47:27 2021
Response via : Initial Calibration

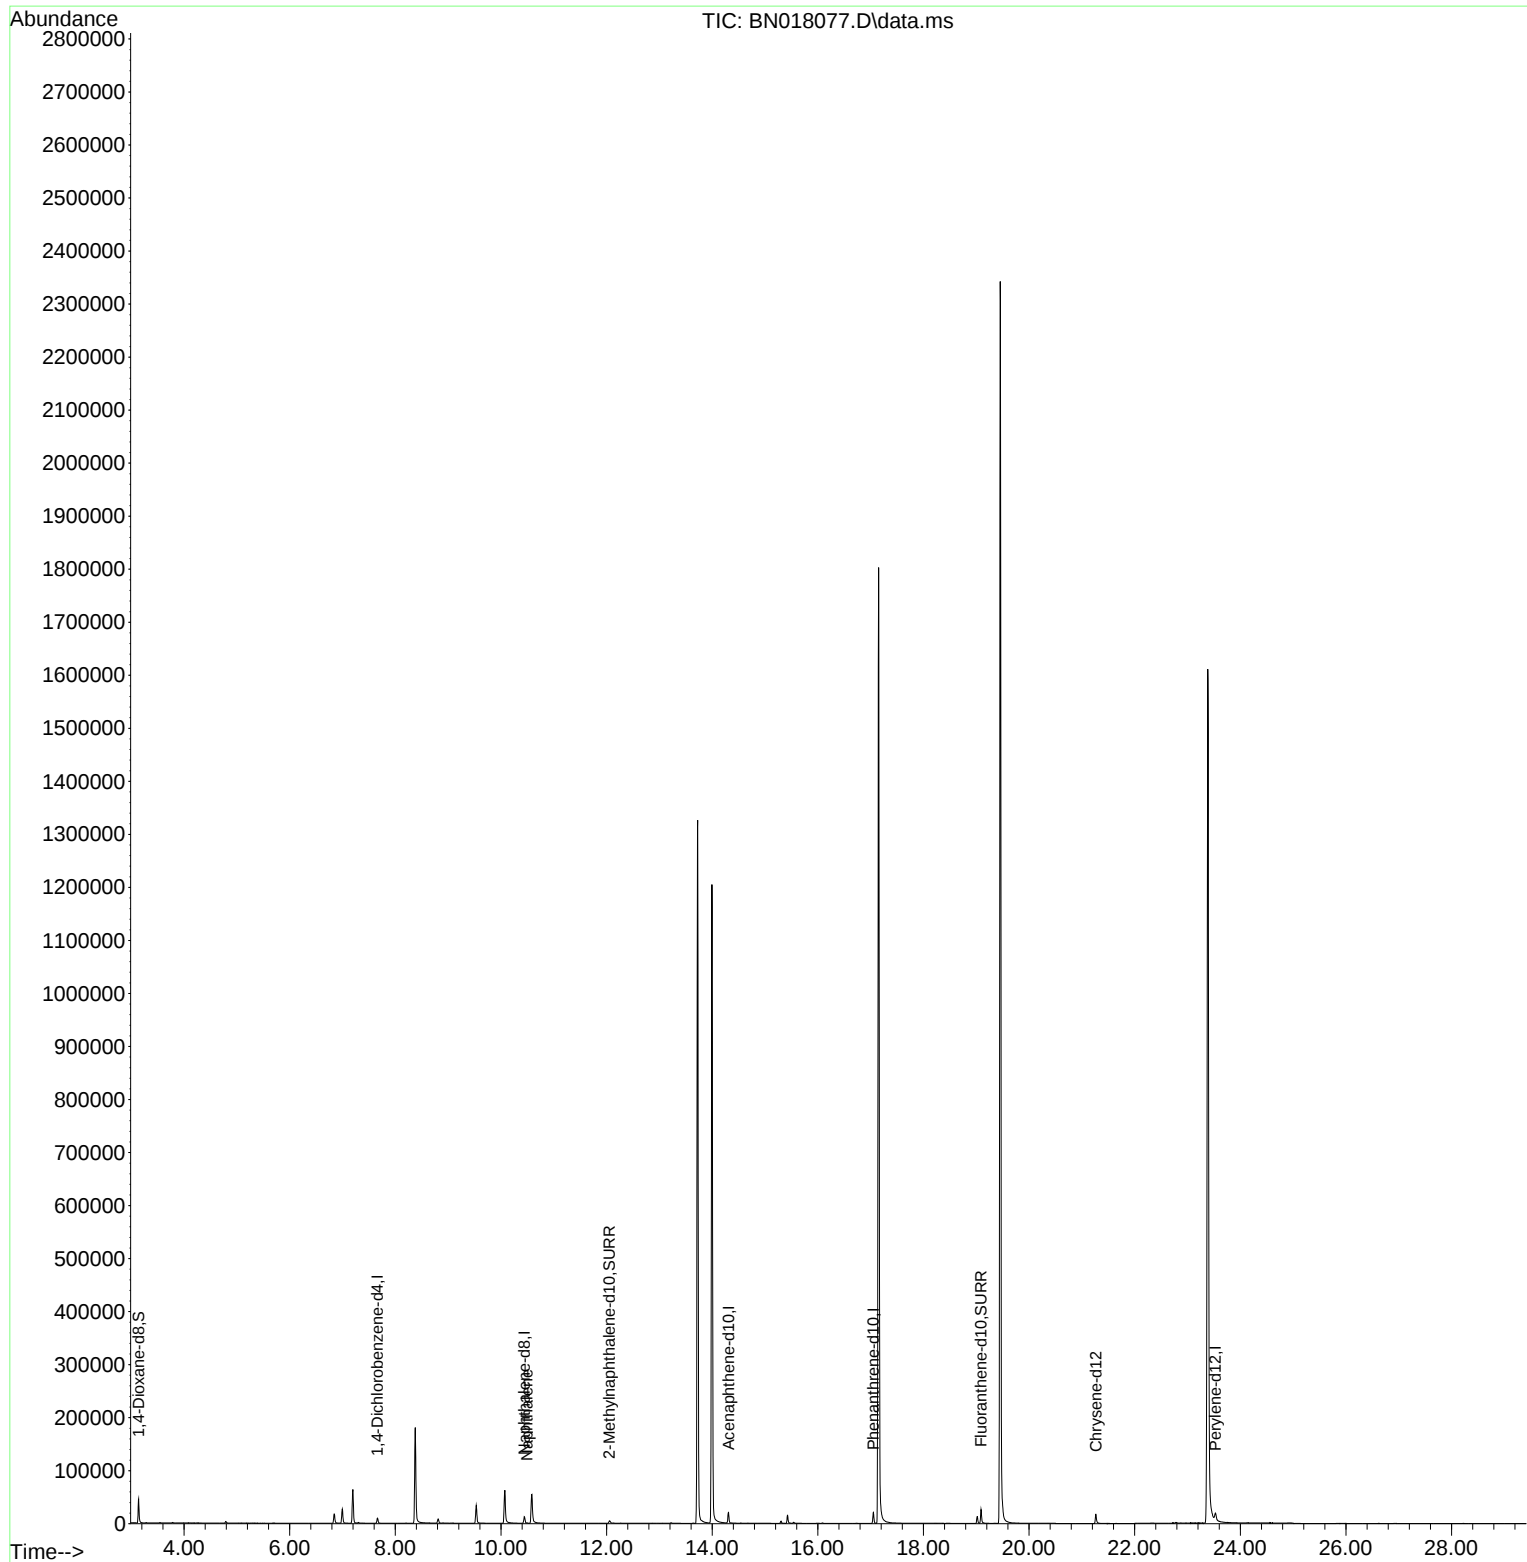

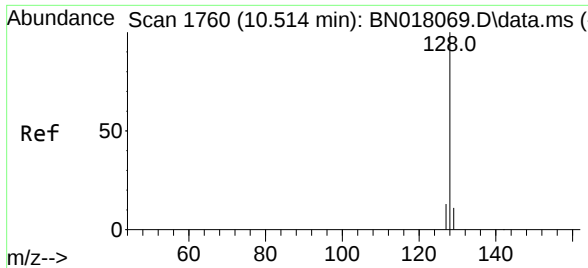

#5
Naphthalene
Concen: 0.022 ng/ul
RT: 10.491 min Scan# 11
Delta R.T. -0.018 min
Lab File: BN018077.D
Acq: 17 Dec 2021 00:42

Instrument :
BNA_N
ClientSampleId :
BG3D7

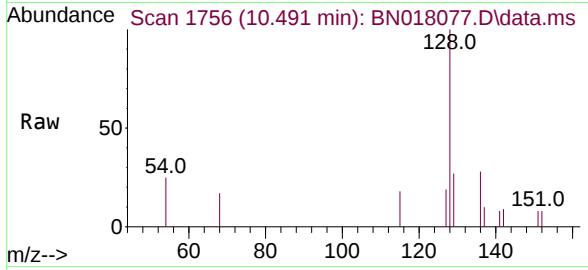

Tgt Ion:128 Resp: 1025
Ion Ratio Lower Upper
128 100
129 26.6 10.4 15.6#
127 19.1 11.8 17.6#

