

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
 Data File : BN018079.D
 Acq On : 17 Dec 2021 01:55
 Operator : CG/JU
 Sample : M4991-02
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3D8

Quant Time: Dec 17 03:09:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 17:47:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.662	152	4406	0.400	ng/ul	0.00
4) Naphthalene-d8	10.442	136	14111	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.304	164	9512	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.053	188	19877	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.263	240	14009	0.400	ng/ul	# 0.00
23) Perylene-d12	23.525	264	15024	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	23387	5.113	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.048	152	7835	0.476	ng/ul	-0.02
18) Fluoranthene-d10	19.091	212	23377	0.585	ng/ul	-0.01
Target Compounds						
						Qvalue
5) Naphthalene	10.492	128	6175	0.160	ng/ul	100
7) 2-Methylnaphthalene	12.119	142	1251	0.058	ng/ul	98
8) 1-Methylnaphthalene	12.339	142	760	0.030	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
Data File : BN018079.D
Acq On : 17 Dec 2021 01:55
Operator : CG/JU
Sample : M4991-02
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3D8


Quant Time: Dec 17 03:09:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 17:47:27 2021
Response via : Initial Calibration

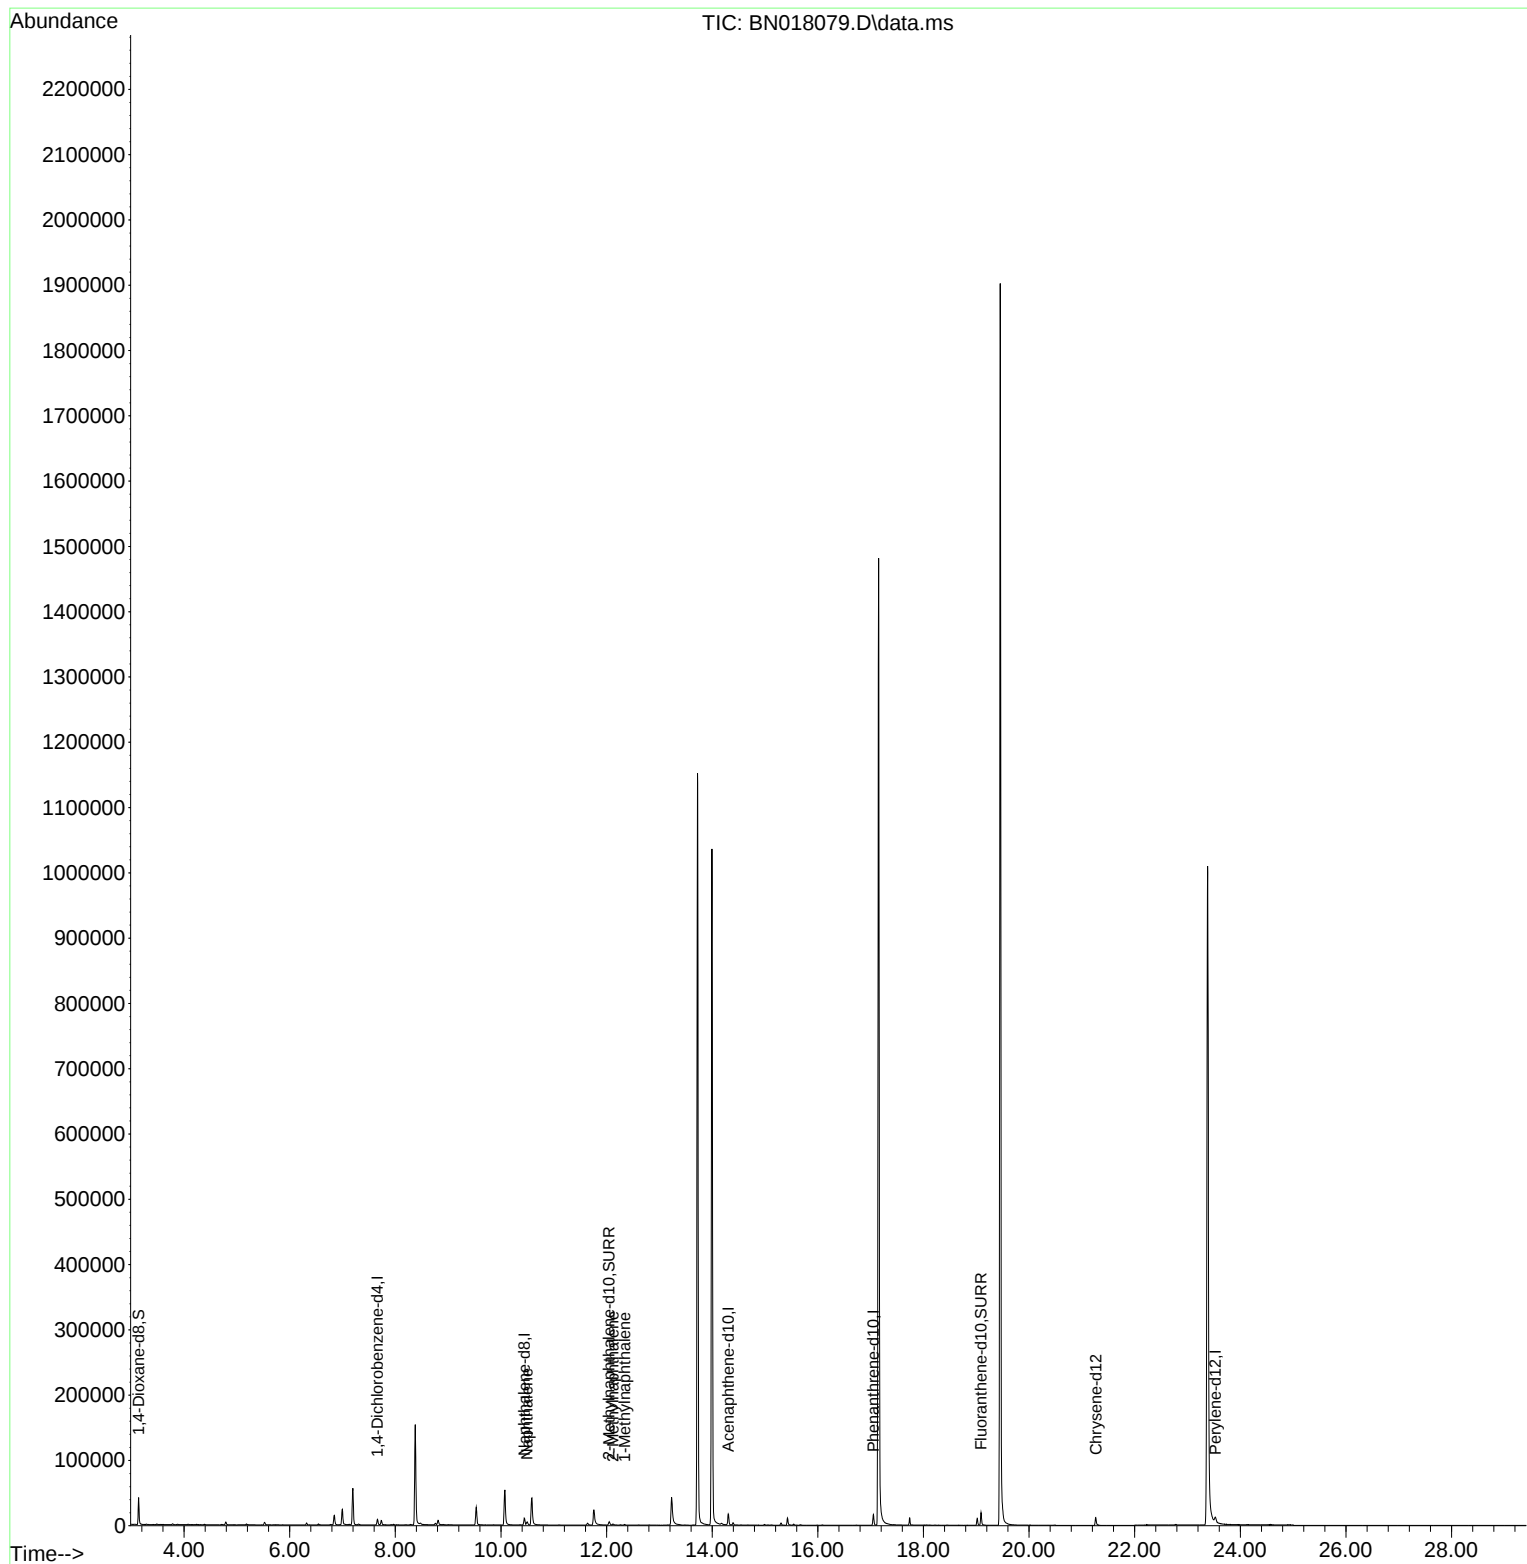



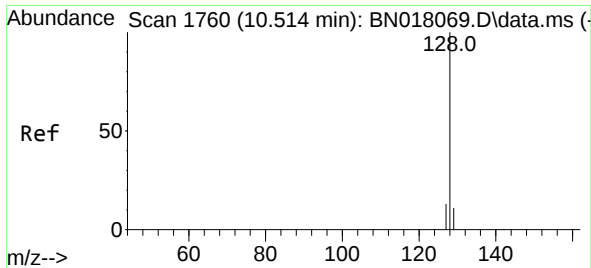


#5
Naphthalene
Concen: 0.160 ng/ul
RT: 10.492 min Scan# 1756
Delta R.T. -0.018 min
Lab File: BN018079.D
Acq: 17 Dec 2021 01:55

Instrument :
BNA_N
ClientSampleId :
BG3D8



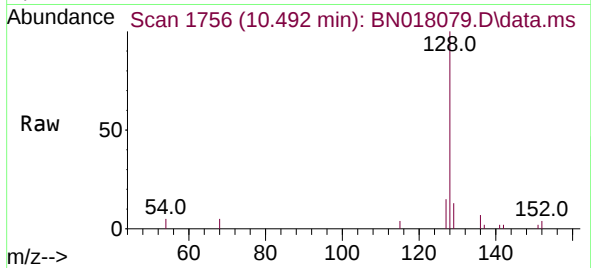



Tgt Ion:	128	Resp:	6175
Ion Ratio	100	Lower	Upper
128	100		
129	12.9	10.4	15.6
127	14.6	11.8	17.6

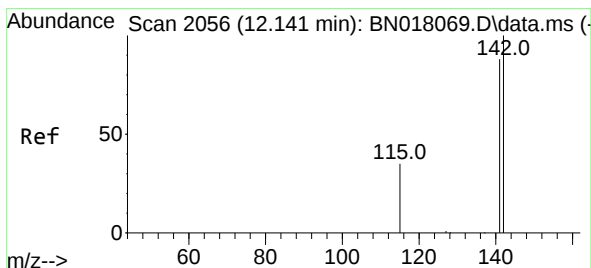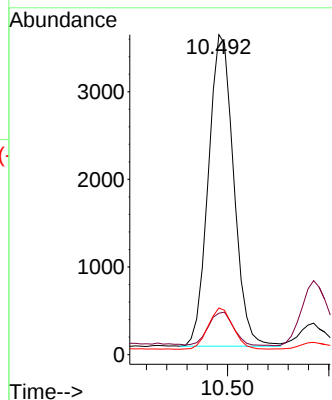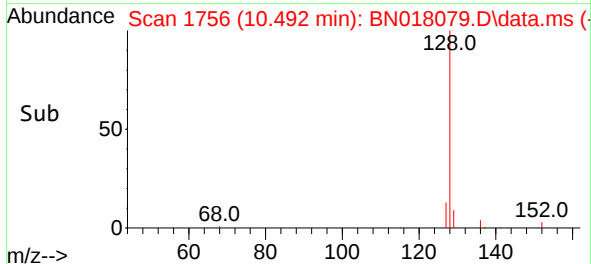

#7
2-Methylnaphthalene
Concen: 0.058 ng/ul
RT: 12.119 min Scan# 2052
Delta R.T. -0.018 min
Lab File: BN018079.D
Acq: 17 Dec 2021 01:55


Tgt Ion:	142	Resp:	1251
Ion Ratio	100	Lower	Upper
142	100		
141	91.4	71.5	107.3

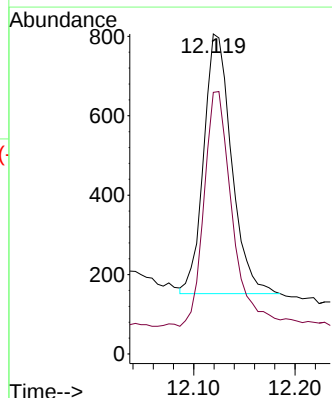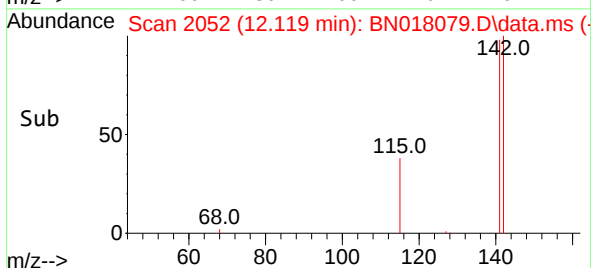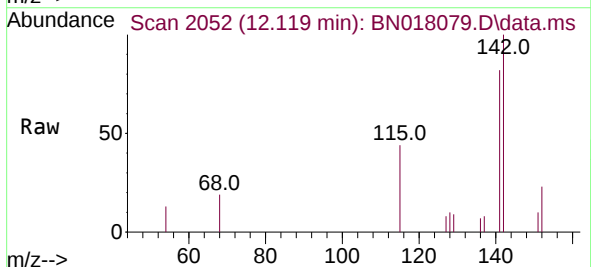

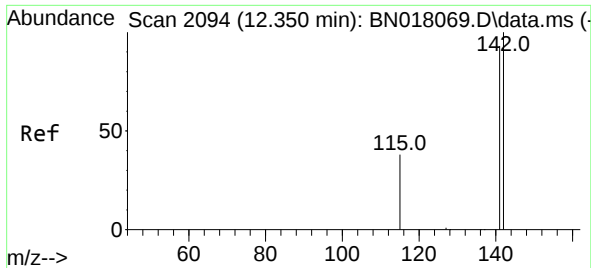

#8
 1-Methylnaphthalene
 Concen: 0.030 ng/ul
 RT: 12.339 min Scan# 2092
 Delta R.T. -0.012 min
 Lab File: BN018079.D
 Acq: 17 Dec 2021 01:55

Instrument :
 BNA_N
 ClientSampleId :
 BG3D8

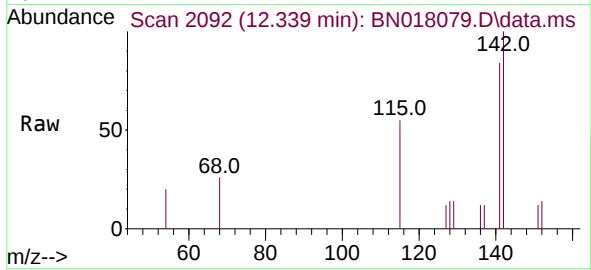

Tgt Ion:142 Resp: 760
 Ion Ratio Lower Upper
 142 100
 141 90.3 73.3 109.9

