

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
 Data File : BN018082.D
 Acq On : 17 Dec 2021 03:43
 Operator : CG/JU
 Sample : M4991-04
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3D7

Quant Time: Dec 17 04:23:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 17:47:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.662	152	5064	0.400	ng/ul	0.00
4) Naphthalene-d8	10.442	136	16520	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.308	164	10869	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.053	188	23855	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.263	240	18861	0.400	ng/ul	# 0.00
23) Perylene-d12	23.522	264	22331	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	25691	4.887	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.053	152	8242	0.428	ng/ul	-0.01
18) Fluoranthene-d10	19.091	212	29457	0.548	ng/ul	-0.01
Target Compounds						
					Qvalue	
5) Naphthalene	10.491	128	1224	0.027	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
Data File : BN018082.D
Acq On : 17 Dec 2021 03:43
Operator : CG/JU
Sample : M4991-04
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3D7

Quant Time: Dec 17 04:23:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 17:47:27 2021
Response via : Initial Calibration

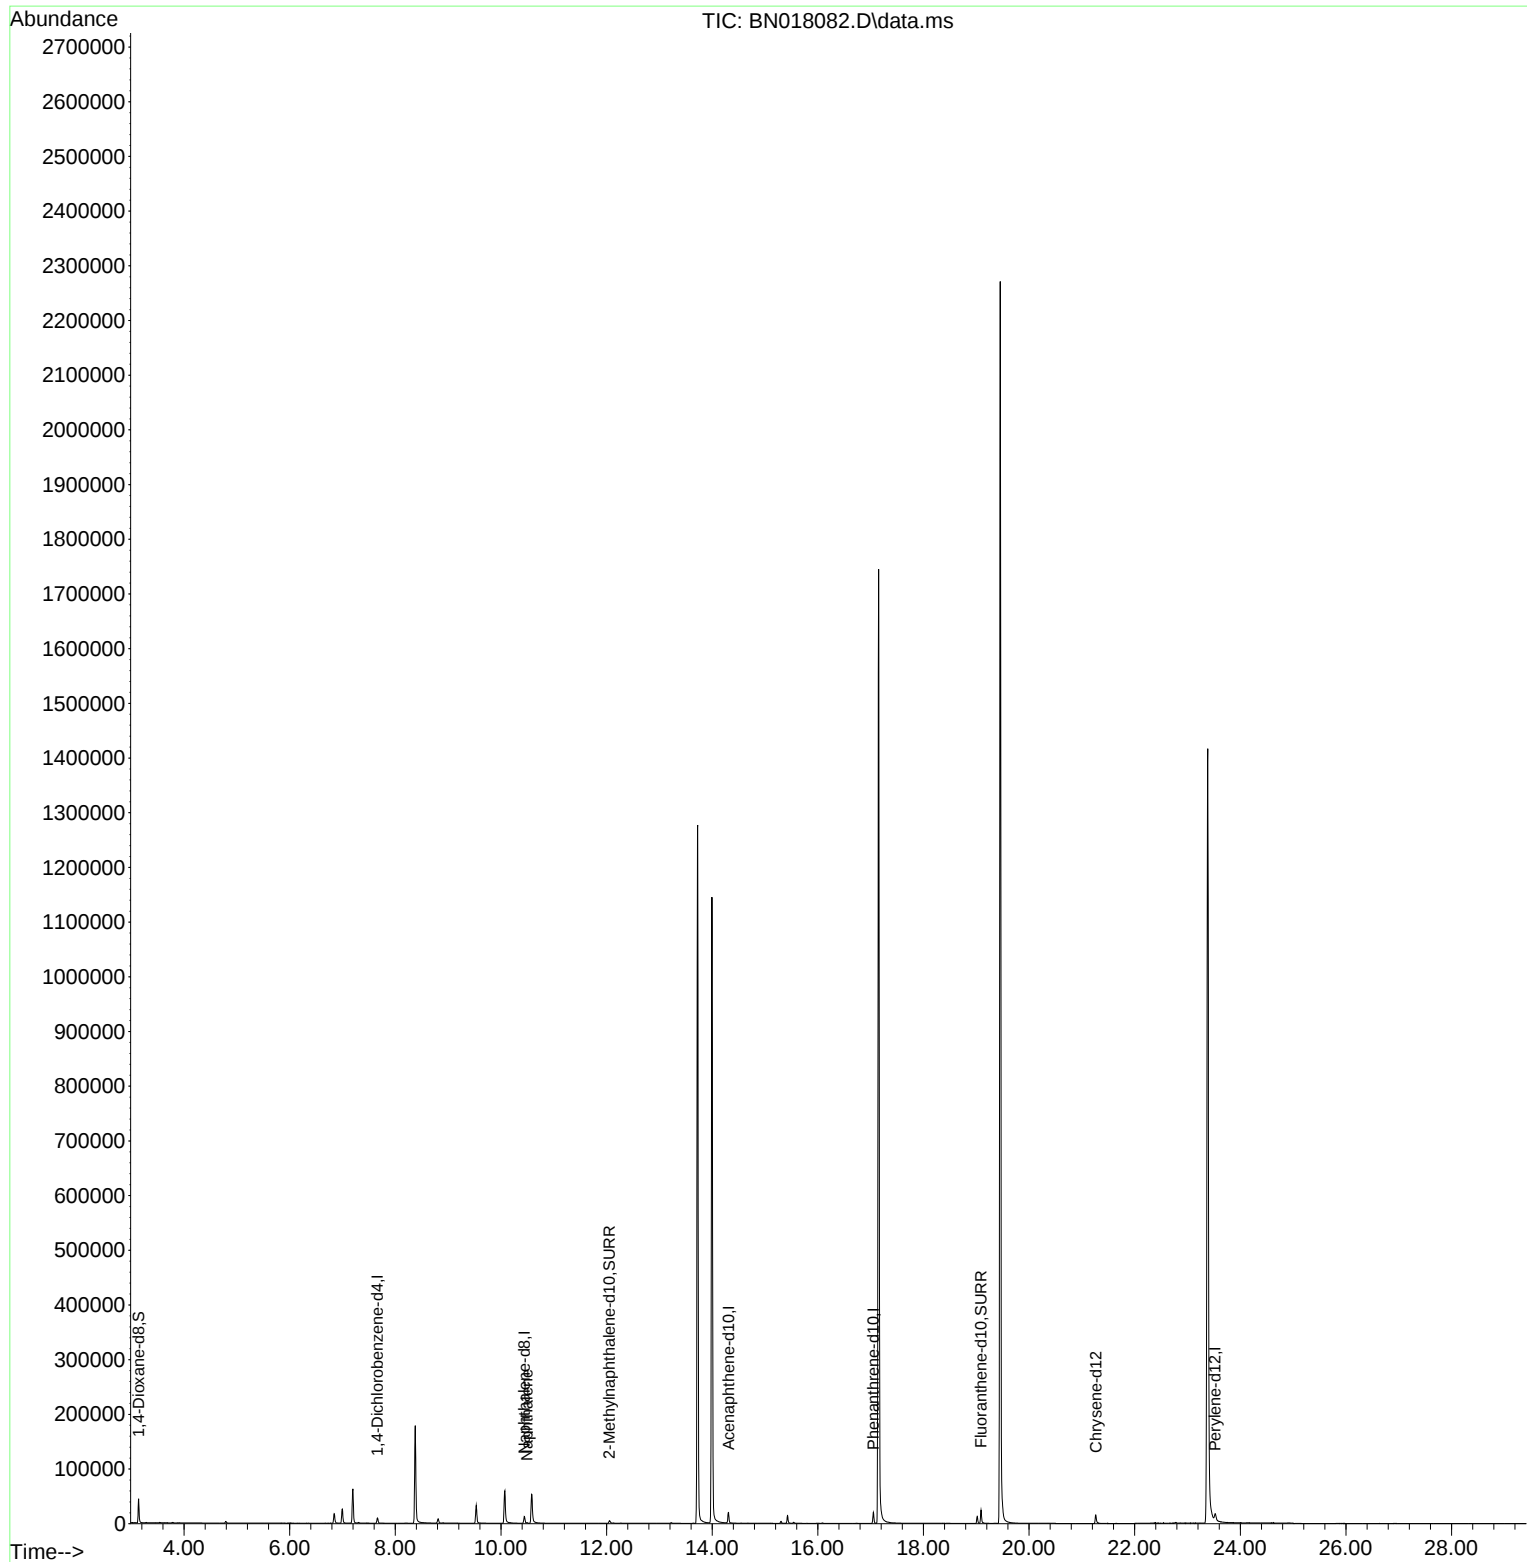

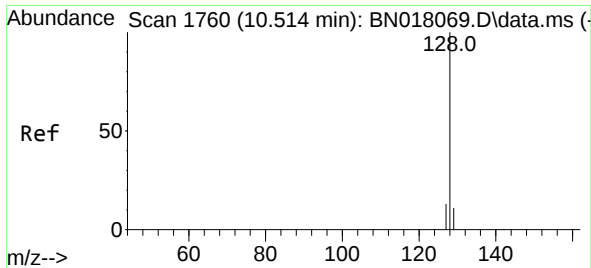

#5

Naphthalene

Concen: 0.027 ng/ul

RT: 10.491 min Scan# 11

Delta R.T. -0.018 min

Lab File: BN018082.D


Acq: 17 Dec 2021 03:43

Instrument :

BNA_N

ClientSampleId :

BG3D7

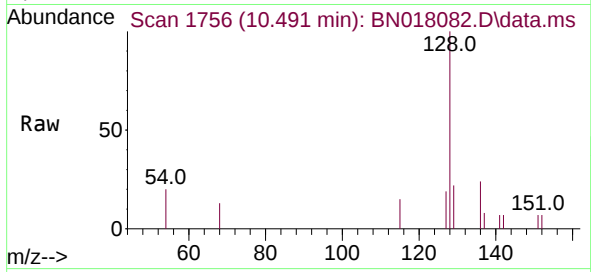

Tgt Ion:128 Resp: 1224

Ion Ratio Lower Upper

128 100

129 22.2 10.4 15.6#

127 19.3 11.8 17.6#

