

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
 Data File : BN018109.D
 Acq On : 17 Dec 2021 20:45
 Operator : CG/JU
 Sample : M5037-20
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C00Y8

Quant Time: Dec 18 02:17:34 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 17:47:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.662	152	4411	0.400	ng/ul	0.00
4) Naphthalene-d8	10.443	136	14475	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.305	164	9425	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.050	188	22124	0.400	ng/ul	-0.02
17) Chrysene-d12	21.262	240	18089	0.400	ng/ul	# 0.00
23) Perylene-d12	23.527	264	19619	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	18089	3.950	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.049	152	5955	0.353	ng/ul	-0.02
18) Fluoranthene-d10	19.088	212	23427	0.454	ng/ul	-0.01
Target Compounds						
					Qvalue	
19) Fluoranthene	19.120	202	1517	0.021	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
Data File : BN018109.D
Acq On : 17 Dec 2021 20:45
Operator : CG/JU
Sample : M5037-20
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C00Y8

Quant Time: Dec 18 02:17:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 17:47:27 2021
Response via : Initial Calibration

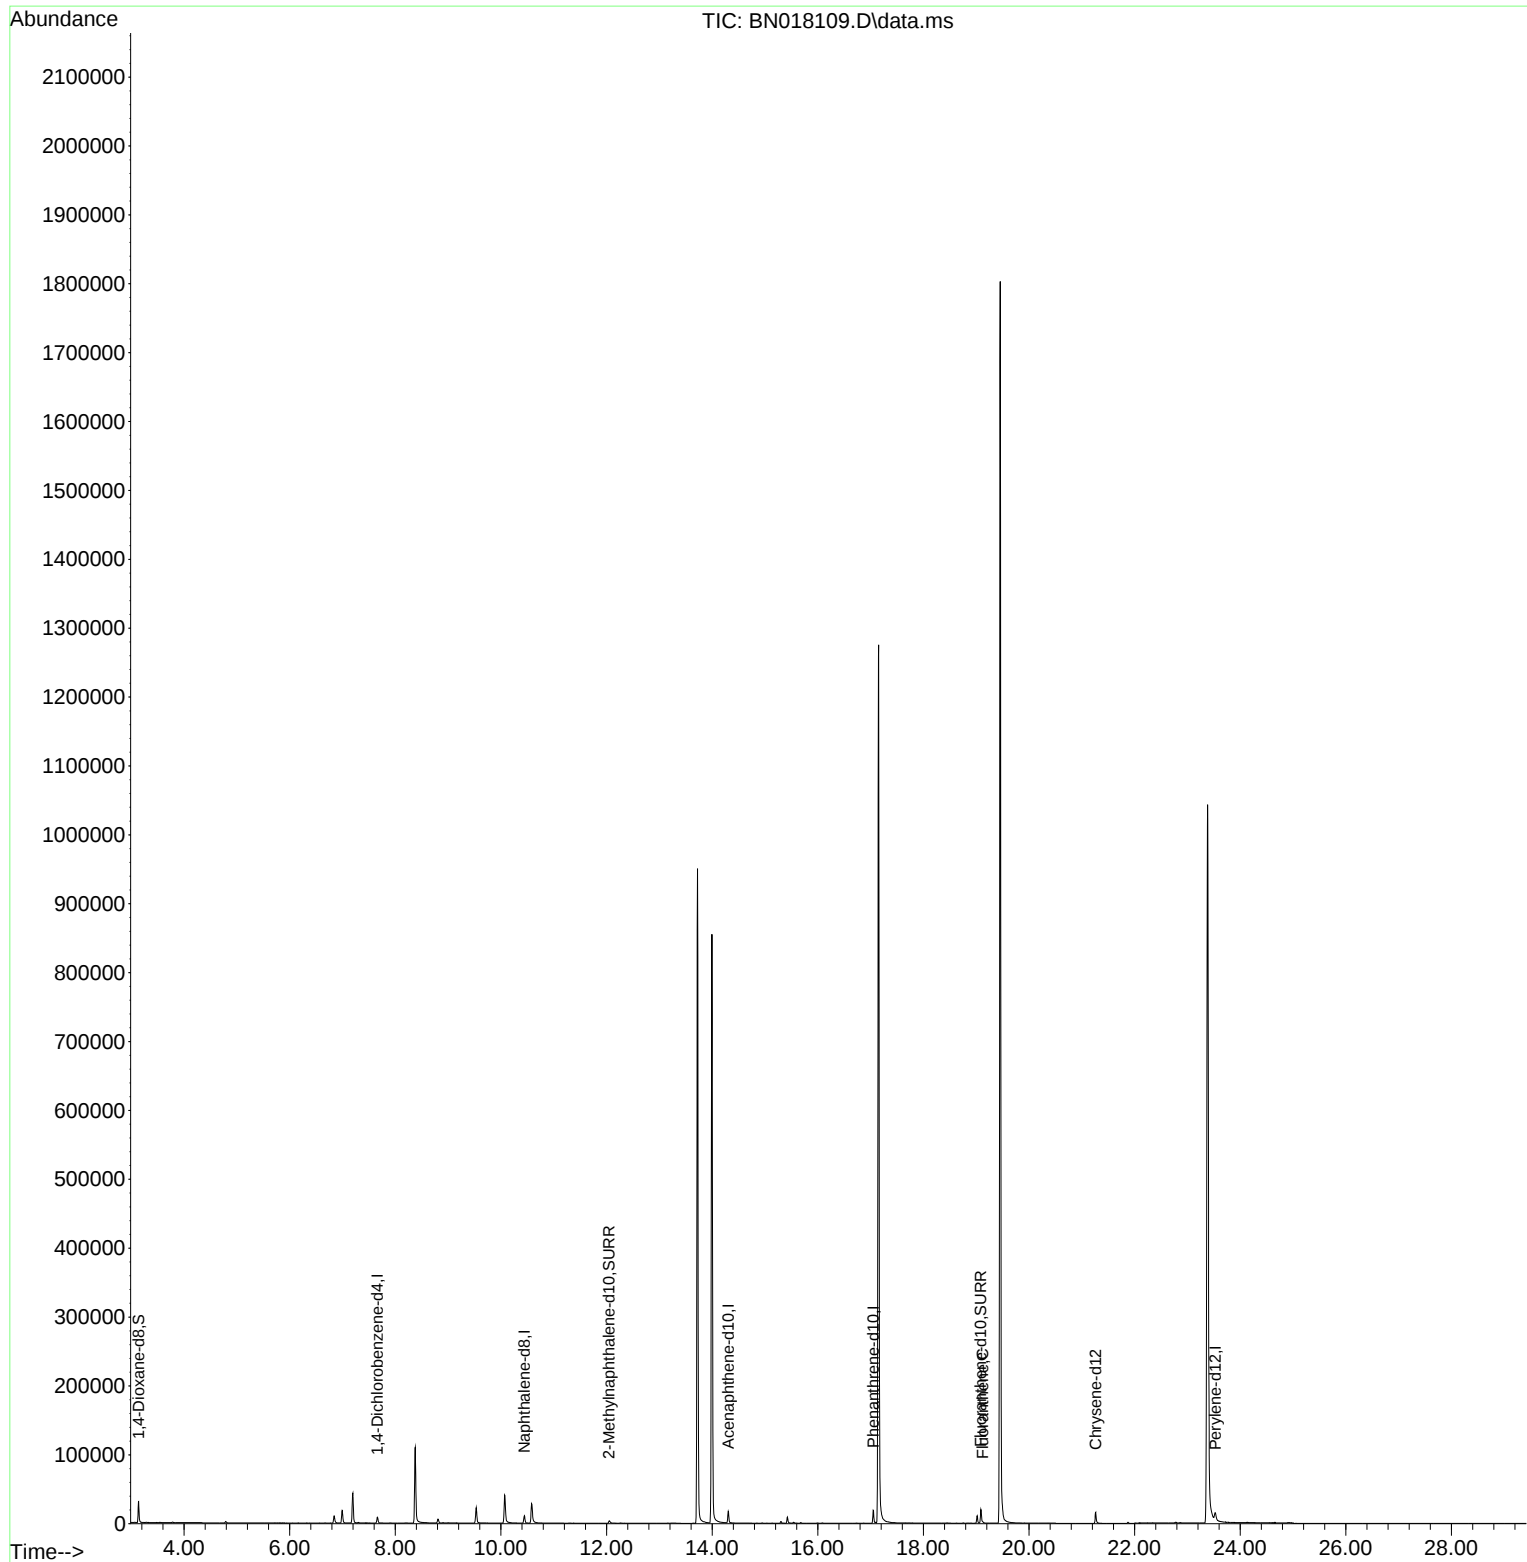

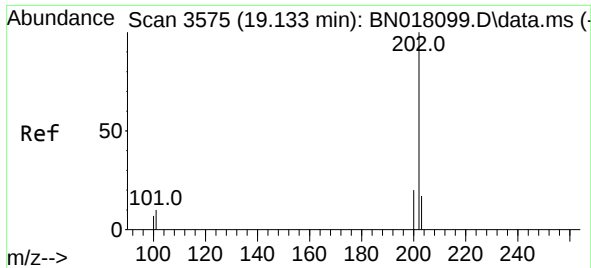

#19

Fluoranthene

Concen: 0.021 ng/ul

RT: 19.120 min Scan# 31

Delta R.T. -0.009 min

Lab File: BN018109.D


Acq: 17 Dec 2021 20:45

Instrument :

BNA_N

ClientSampleId :

C00Y8

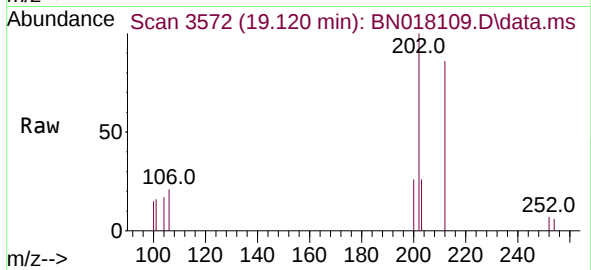

Tgt Ion:202 Resp: 1517

Ion Ratio Lower Upper

202 100

101 16.2 9.0 13.4#

100 14.7 6.8 10.2#

