

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
 Data File : BN018114.D
 Acq On : 17 Dec 2021 23:45
 Operator : CG/JU
 Sample : M5037-21
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C00Z0

Quant Time: Dec 18 02:30:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 17:47:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.662	152	4015	0.400	ng/ul	0.00
4) Naphthalene-d8	10.442	136	12608	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.303	164	7932	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.053	188	18398	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.263	240	16008	0.400	ng/ul	# 0.00
23) Perylene-d12	23.525	264	18695	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	16476	3.953	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.048	152	4719	0.321	ng/ul	-0.02
18) Fluoranthene-d10	19.091	212	18981	0.416	ng/ul	-0.01
Target Compounds						
15) Phenanthrene	17.091	178	1516	0.024	ng/ul#	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121621\
Data File : BN018114.D
Acq On : 17 Dec 2021 23:45
Operator : CG/JU
Sample : M5037-21
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C00Z0


Quant Time: Dec 18 02:30:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 17:47:27 2021
Response via : Initial Calibration

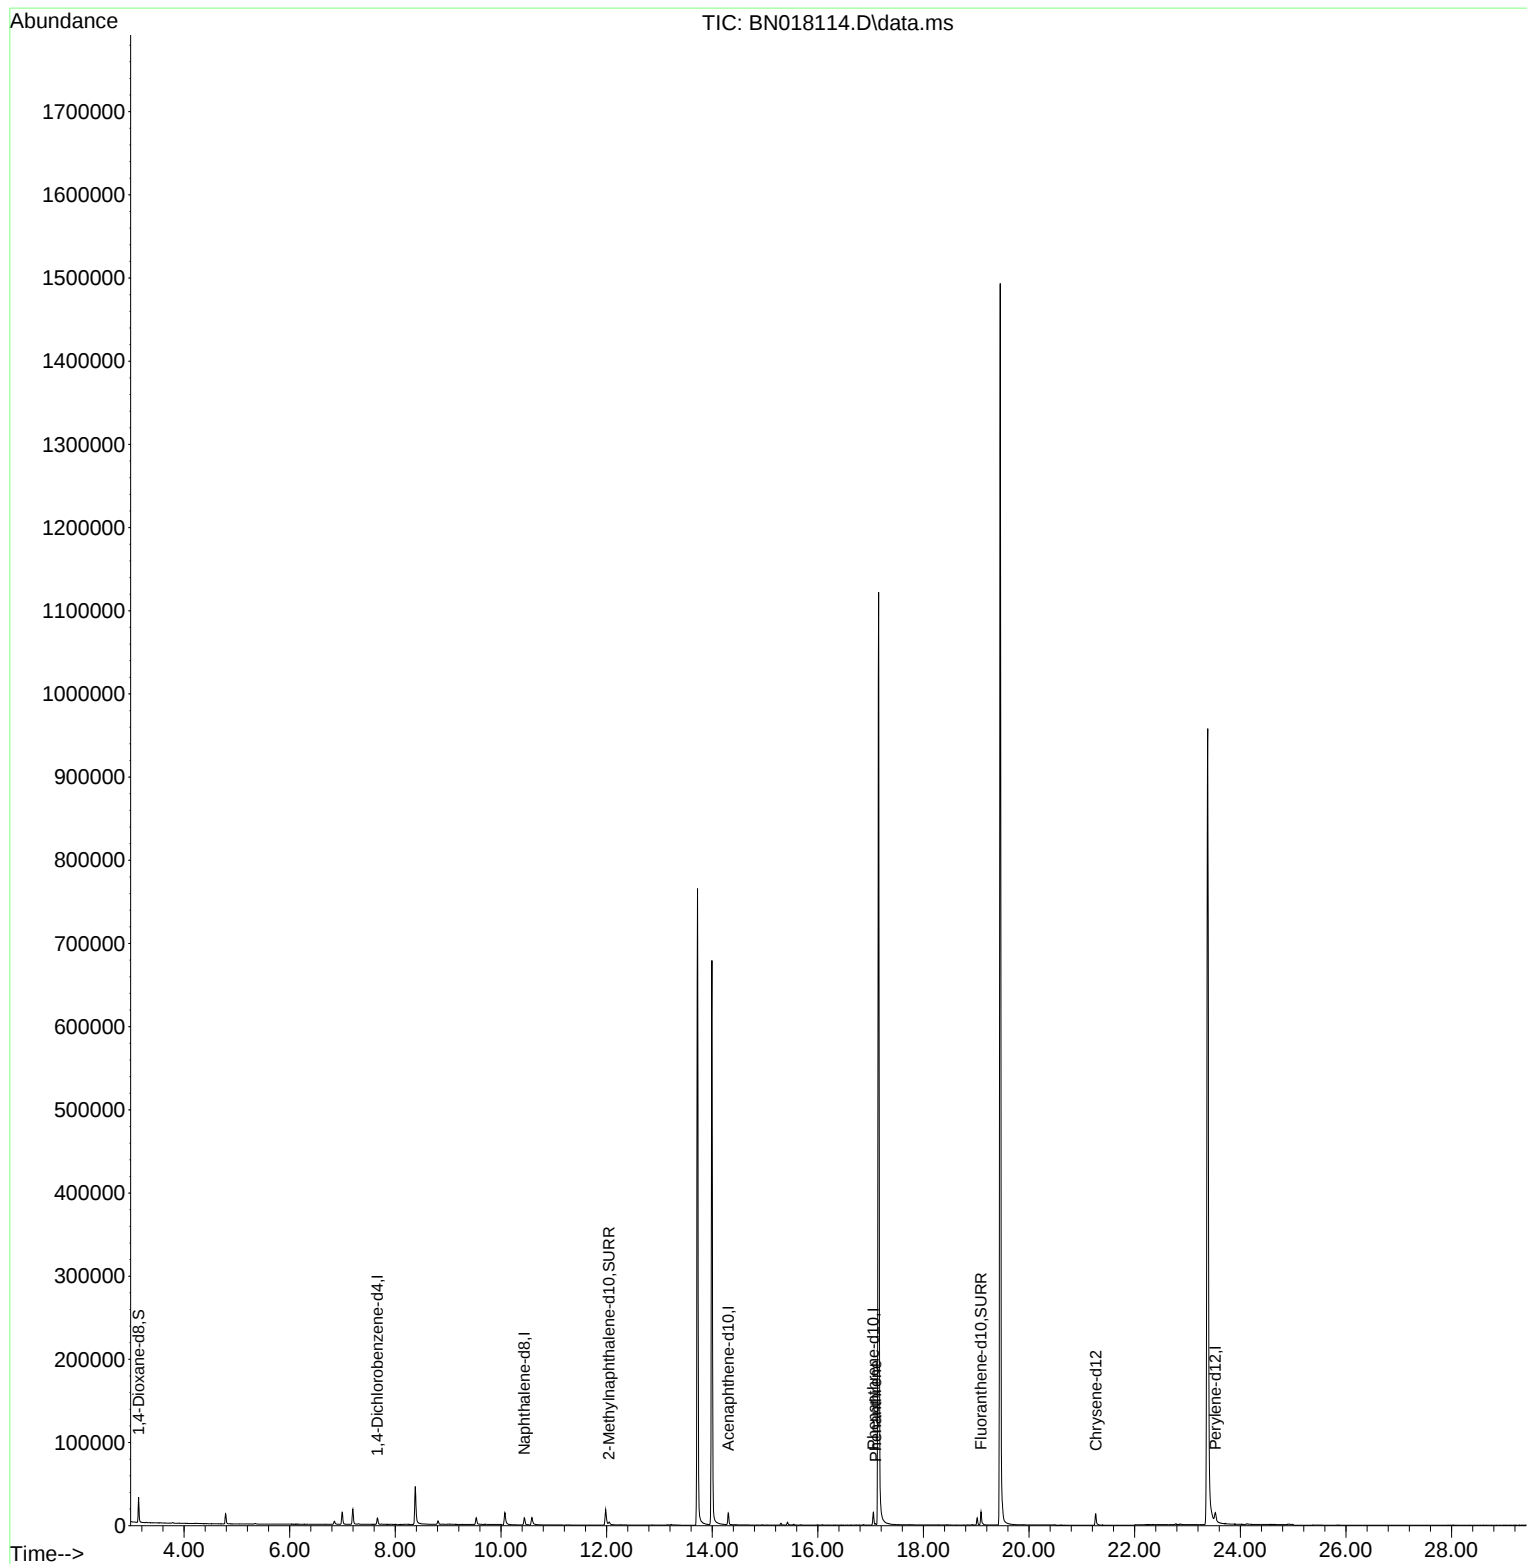

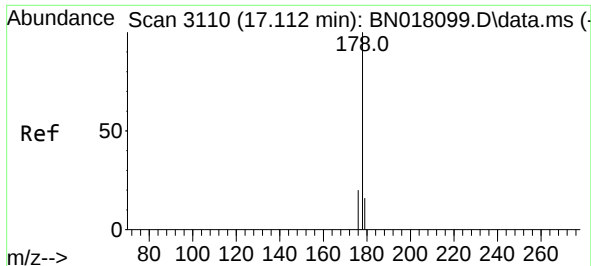

#15
 Phenanthrene
 Concen: 0.024 ng/ul
 RT: 17.091 min Scan# 31
 Delta R.T. -0.018 min
 Lab File: BN018114.D
 Acq: 17 Dec 2021 23:45

Instrument :
 BNA_N
 ClientSampleId :
 C00Z0

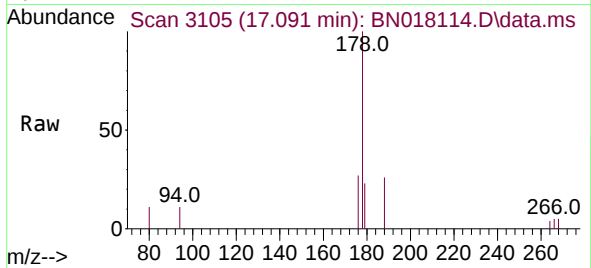

Tgt Ion	Ratio	Lower	Upper
178	100		
179	23.5	13.0	19.4#
176	26.9	15.6	23.4#

