

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030819\
 Data File : BN004675.D
 Acq On : 08 Mar 2019 16:23
 Operator : JU/SJ
 Sample : K1720-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF8A8

Quant Time: Mar 08 22:11:59 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 08 00:36:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	29189	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	133806	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	86275	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	204376	20.00	ng/ul	0.00
78) Chrysene-d12	21.31	240	189190	20.00	ng/ul	0.00
86) Perylene-d12	23.57	264	178456	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	3022	5.84	ng/uL	0.00
5) Phenol-d5	6.89	99	42079	17.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	21982	17.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	38183	18.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	38397	18.30	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	18954	18.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	20949	18.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	39427	17.86	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	54674	20.64	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	144419	19.36	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	160961	17.93	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	16651	12.03	ng/ul	0.00
58) Fluorene-d10	15.36	176	119224	18.80	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.48	200	14435	10.23	ng/ul	0.00
71) Anthracene-d10	17.21	188	189134	19.00	ng/ul	0.00
79) Pyrene-d10	19.51	212	192221	20.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.43	264	155962	16.27	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.82	163	33417	4.566	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030819\
Data File : BN004675.D
Acq On : 08 Mar 2019 16:23
Operator : JU/SJ
Sample : K1720-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF8A8

Quant Time: Mar 08 22:11:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 08 00:36:35 2019
Response via : Initial Calibration

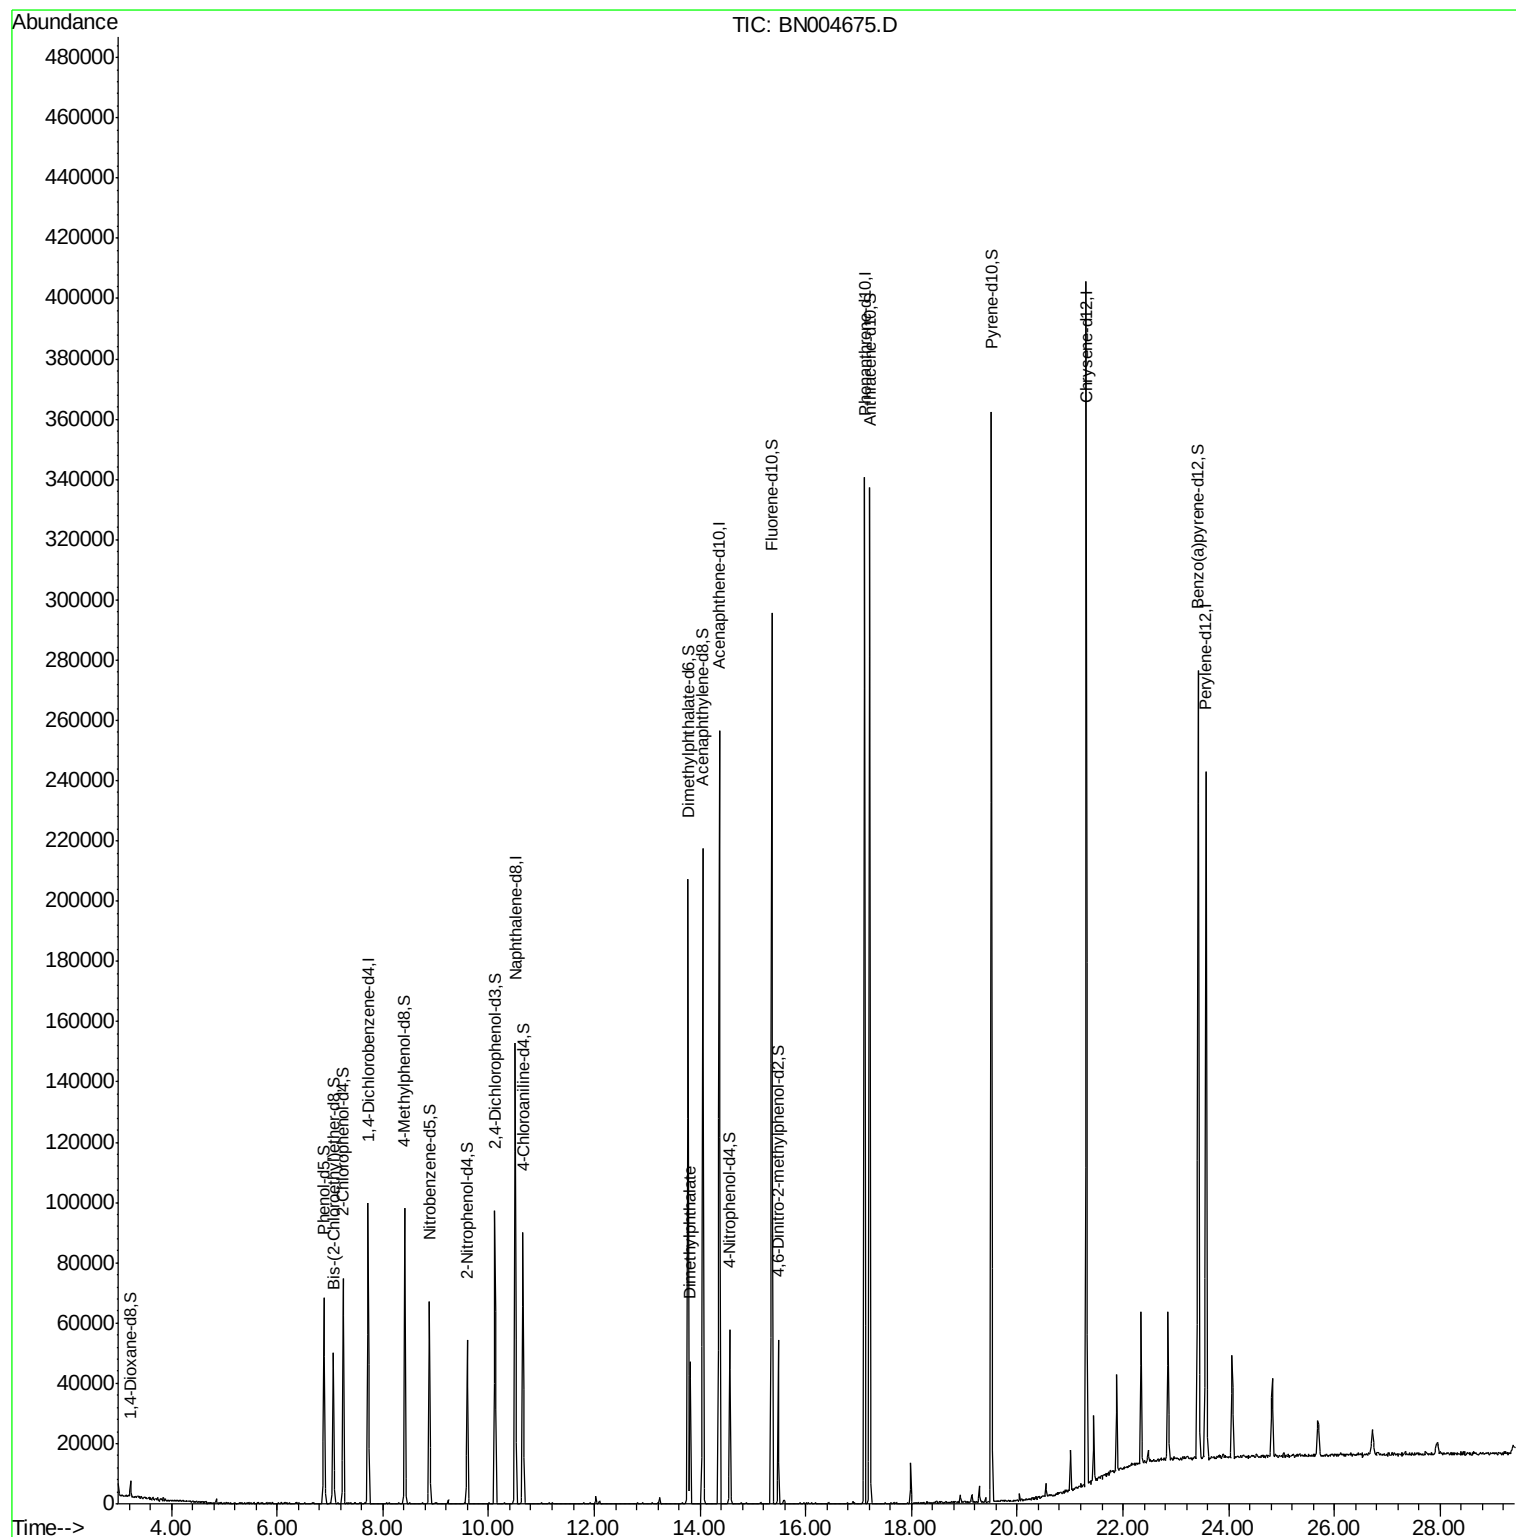

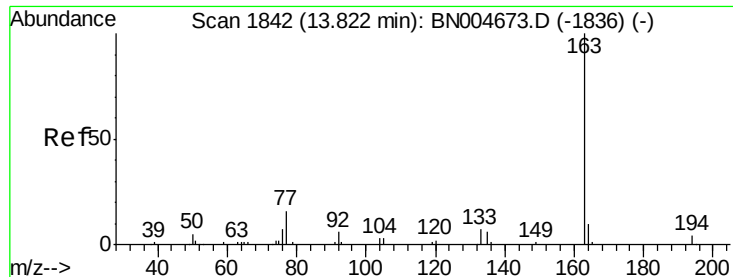

#45
 Dimethylphthalate
 Concen: 4.566 ng/ul
 RT: 13.82 min Scan# 1841
 Delta R.T. -0.01 min
 Lab File: BN004675.D
 Acq: 08 Mar 2019 16:23

Instrument :
 BNA_N
 ClientSampleId :
 BF8A8

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.4	3.4	5.2
164	10.6	7.9	11.9

