

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030819\
 Data File : BN004676.D
 Acq On : 08 Mar 2019 16:58
 Operator : JU/SJ
 Sample : K1720-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF8A9

Quant Time: Mar 08 22:12:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 08 00:36:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	27998	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	133429	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	86543	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	205895	20.00	ng/ul	0.00
78) Chrysene-d12	21.31	240	200899	20.00	ng/ul	0.00
86) Perylene-d12	23.57	264	177238	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	2965	5.97	ng/uL	0.00
5) Phenol-d5	6.88	99	32077	13.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	17353	14.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	29669	14.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	29051	14.44	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	15315	15.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	17924	15.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	32106	14.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	45532	17.24	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	121929	16.29	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	138737	15.40	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	14758	10.63	ng/ul	0.00
58) Fluorene-d10	15.36	176	104152	16.38	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.48	200	13131	9.24	ng/ul	0.00
71) Anthracene-d10	17.21	188	166410	16.59	ng/ul	0.00
79) Pyrene-d10	19.51	212	189473	19.30	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.43	264	149675	15.73	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.82	163	23823	3.245	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030819\
Data File : BN004676.D
Acq On : 08 Mar 2019 16:58
Operator : JU/SJ
Sample : K1720-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF8A9

Quant Time: Mar 08 22:12:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 08 00:36:35 2019
Response via : Initial Calibration

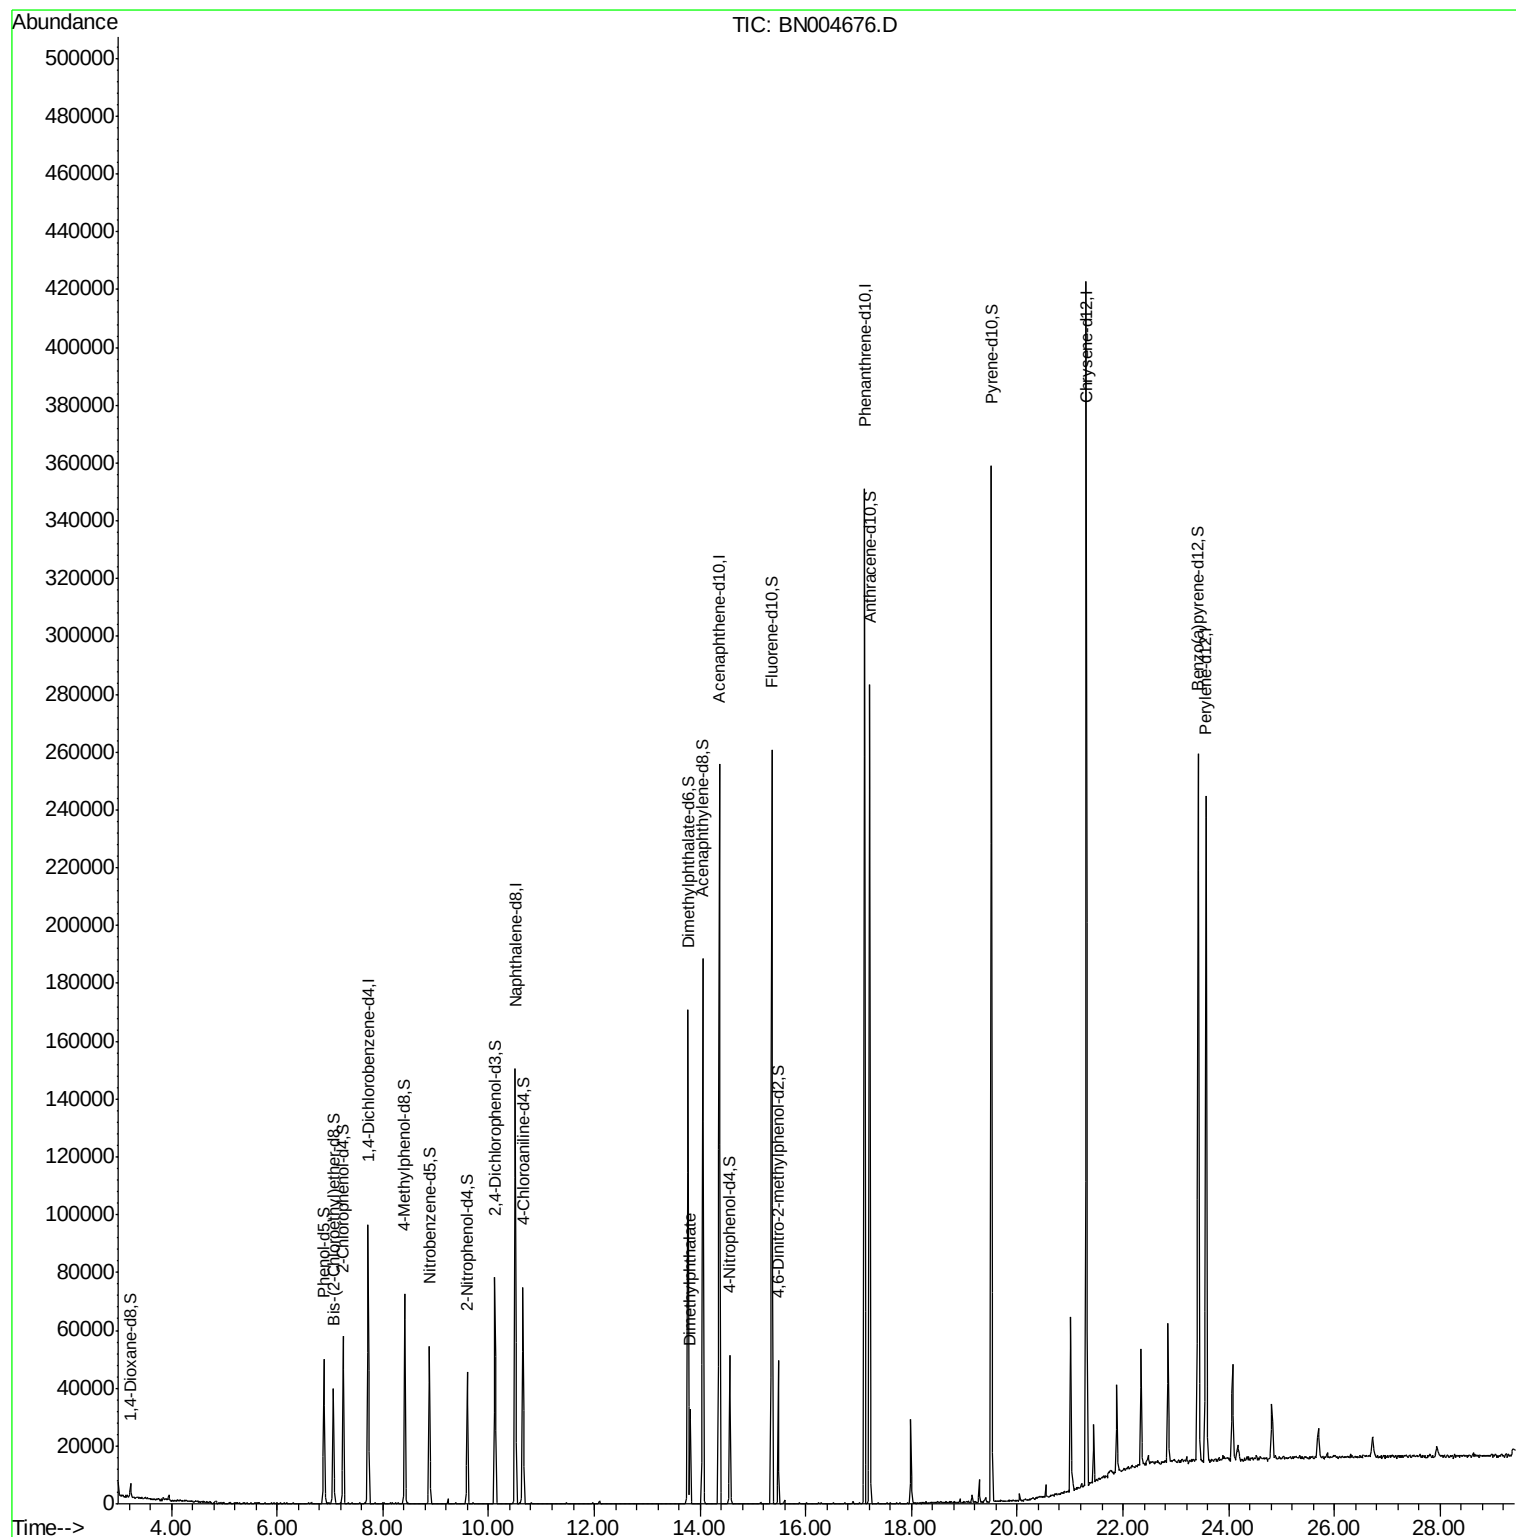

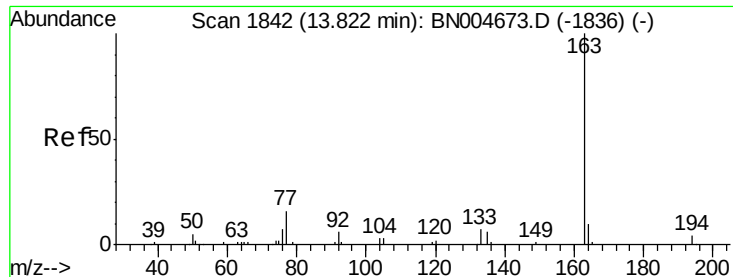

#45

Dimethylphthalate

Concen: 3.245 ng/ul

RT: 13.82 min Scan# 1841

Delta R.T. -0.01 min

Lab File: BN004676.D

Acq: 08 Mar 2019 16:58

Instrument :

BNA_N

ClientSampleId :

BF8A9


Tot Ion:163 Resp: 23823

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2

164 10.4 7.9 11.9

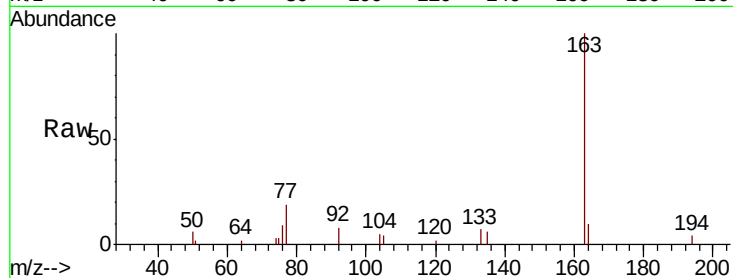

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

