

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030819\
 Data File : BN004677.D
 Acq On : 08 Mar 2019 17:33
 Operator : JU/SJ
 Sample : K1720-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF8B2

Quant Time: Mar 08 22:12:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 08 00:36:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	29539	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	138137	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	89978	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	216526	20.00	ng/ul	0.00
78) Chrysene-d12	21.31	240	205067	20.00	ng/ul	0.00
86) Perylene-d12	23.57	264	184659	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	2644	5.05	ng/uL	0.00
5) Phenol-d5	6.88	99	29507	12.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	16741	13.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	27176	12.83	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	27053	12.74	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	14051	13.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	15911	13.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	28934	12.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	41430	15.15	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	113818	14.63	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	120797	12.90	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	12527	8.68	ng/ul	0.00
58) Fluorene-d10	15.36	176	93405	14.13	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.48	200	10679	7.14	ng/ul	0.00
71) Anthracene-d10	17.21	188	146138	13.86	ng/ul	0.00
79) Pyrene-d10	19.51	212	151672	15.14	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	114824	11.58	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.91	94	3131	1.260 ng/ul#	91
45) Dimethylphthalate	13.82	163	25697	3.366 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030819\
Data File : BN004677.D
Acq On : 08 Mar 2019 17:33
Operator : JU/SJ
Sample : K1720-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF8B2

Quant Time: Mar 08 22:12:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 08 00:36:35 2019
Response via : Initial Calibration

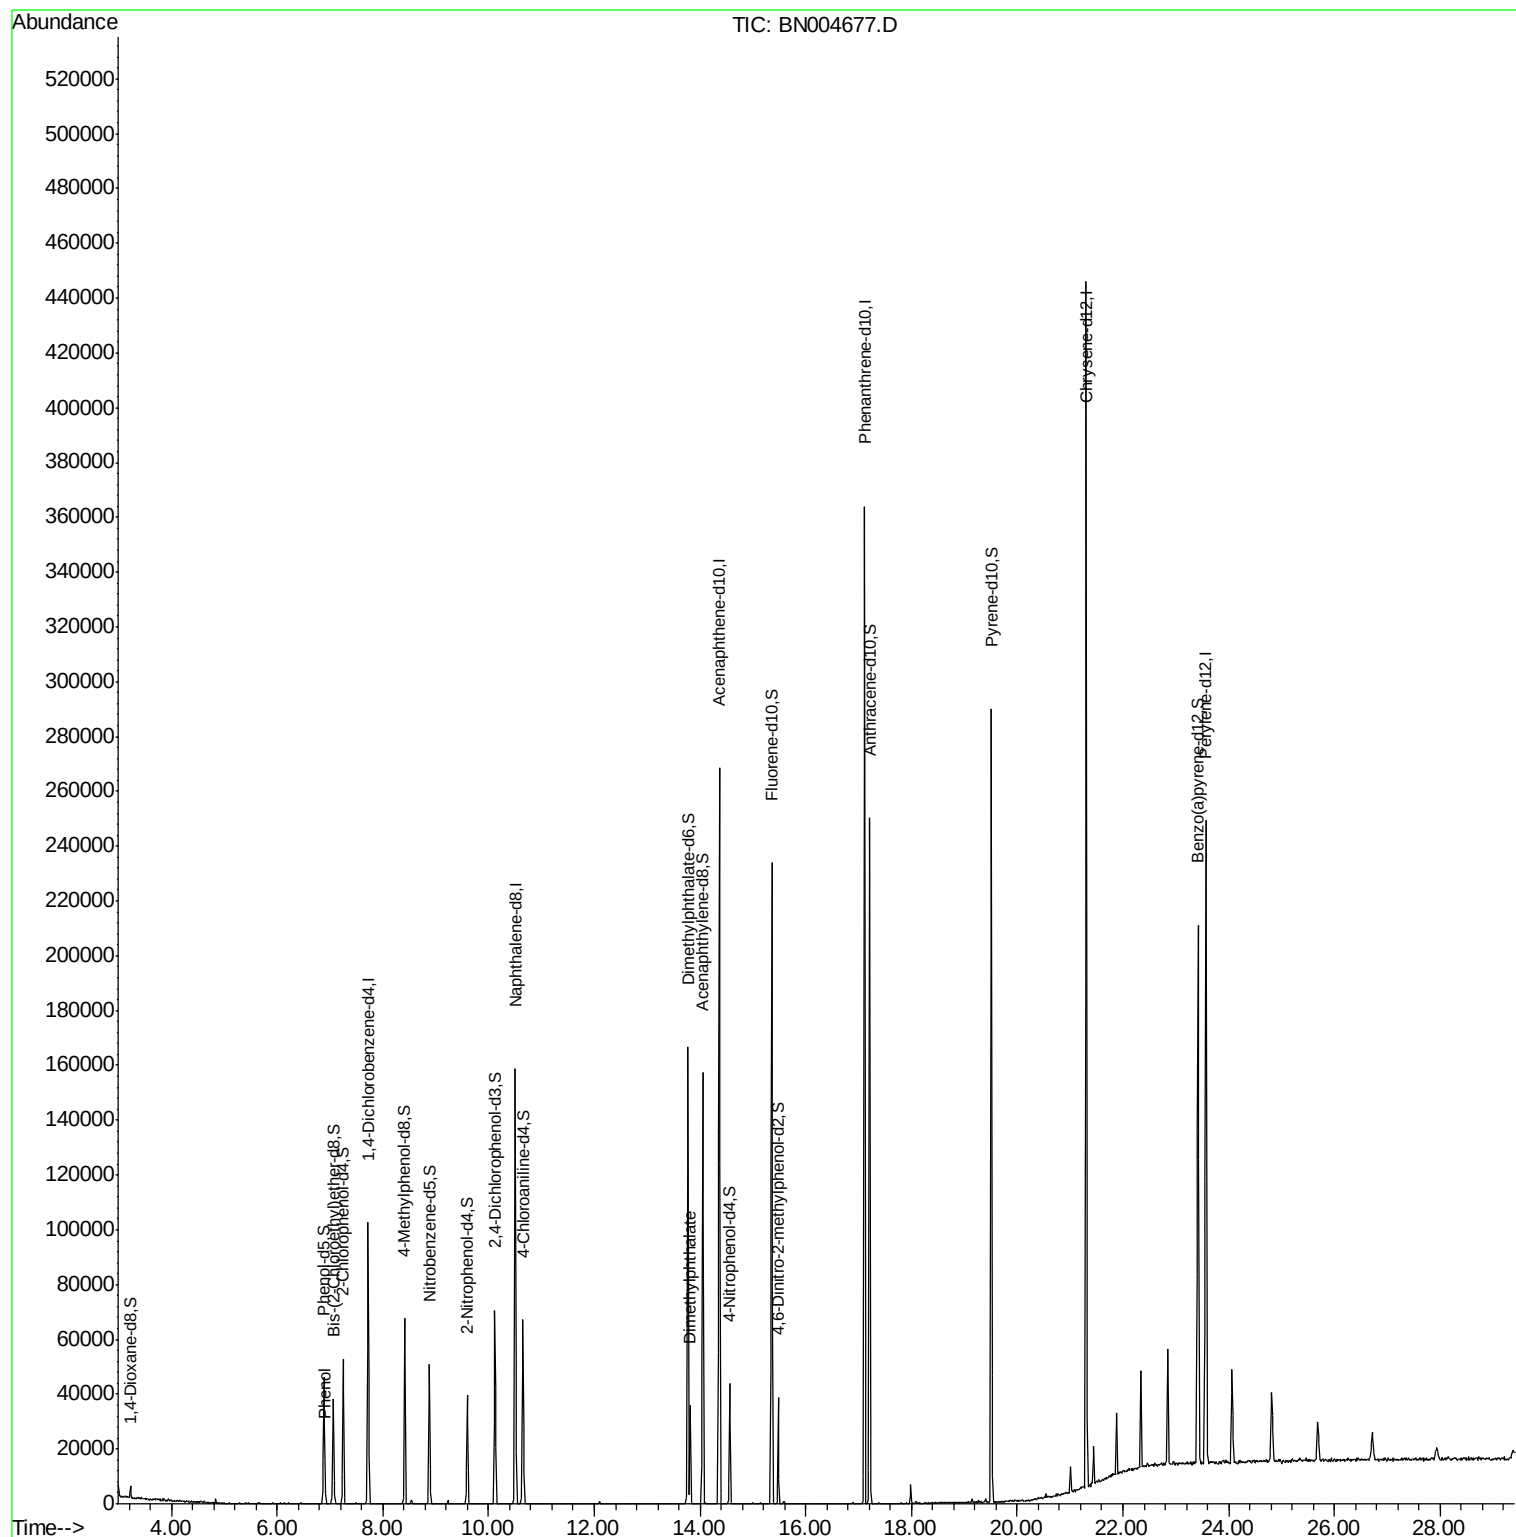

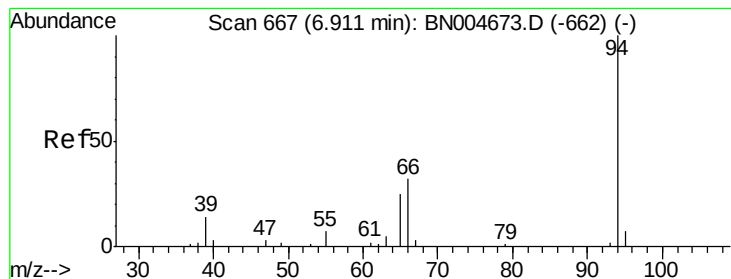

#6

Phenol

Concen: 1.260 ng/ul

RT: 6.91 min Scan# 667

Delta R.T. 0.00 min

Lab File: BN004677.D

Acq: 08 Mar 2019 17:33

Instrument :

BNA_N

ClientSampled :

BF8B2


Tot Ion: 94 Resp: 3131

Ion Ratio Lower Upper

94 100

65 27.2 20.2 30.4




66 42.4 28.2 42.2#

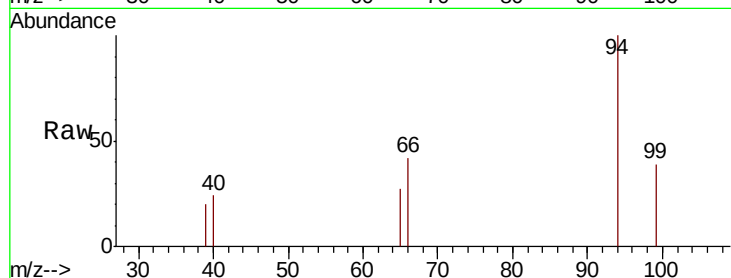

Abundance Ion 94.00 (93.70 to 94.70): BN004677.D (-633) (-)

Ion 65.00 (64.70 to 65.70): BN004677.D (-633) (-)

Ion 66.00 (65.70 to 66.70): BN004677.D (-633) (-)

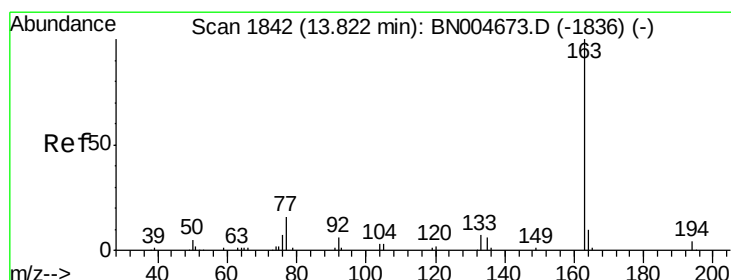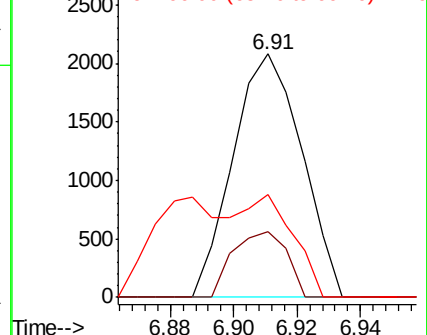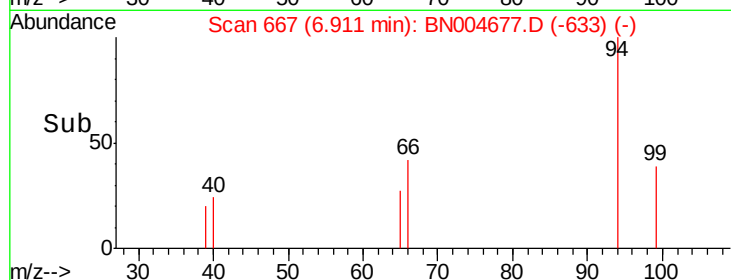

#45

Dimethylphthalate

Concen: 3.366 ng/ul

RT: 13.82 min Scan# 1841

Delta R.T. -0.01 min

Lab File: BN004677.D

Acq: 08 Mar 2019 17:33


Tgt Ion:163 Resp: 25697

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 9.9 7.9 11.9

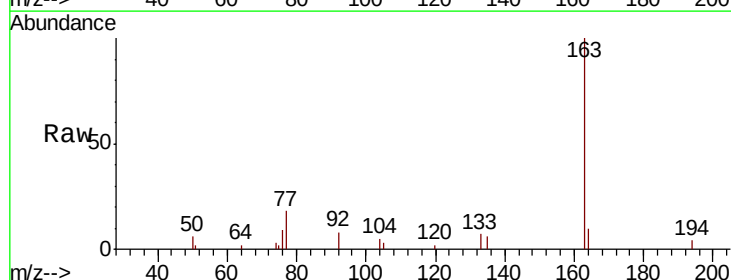

Abundance Ion 163.00 (162.70 to 163.70): BN004677.D (-1808) (-)

Ion 194.00 (193.70 to 194.70): BN004677.D (-1808) (-)

Ion 164.00 (163.70 to 164.70): BN004677.D (-1808) (-)

