

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030819\
 Data File : BN004709.D
 Acq On : 09 Mar 2019 13:17
 Operator : JU/SJ
 Sample : K1736-04
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF622

Quant Time: Mar 11 00:31:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 08 00:36:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	32394	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	142610	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	87266	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	206196	20.00	ng/ul	0.00
78) Chrysene-d12	21.31	240	231889	20.00	ng/ul	0.00
86) Perylene-d12	23.57	264	208979	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	3461	6.03	ng/uL	0.00
5) Phenol-d5	6.89	99	36864	13.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	21141	15.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	34798	14.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	32076	13.78	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	17170	15.79	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	19371	15.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	33648	14.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	43754	15.50	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	118429	15.70	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	139591	15.37	ng/ul	0.00
52) 4-Nitrophenol-d4	14.59	143	9811	7.01	ng/ul	0.02
58) Fluorene-d10	15.36	176	101191	15.78	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.48	200	6754	4.74	ng/ul	0.00
71) Anthracene-d10	17.21	188	160731	16.00	ng/ul	0.00
79) Pyrene-d10	19.51	212	187165	16.52	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	160265	14.28	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.82	163	13937	1.883	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030819\
Data File : BN004709.D
Acq On : 09 Mar 2019 13:17
Operator : JU/SJ
Sample : K1736-04
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF622

Quant Time: Mar 11 00:31:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 08 00:36:35 2019
Response via : Initial Calibration

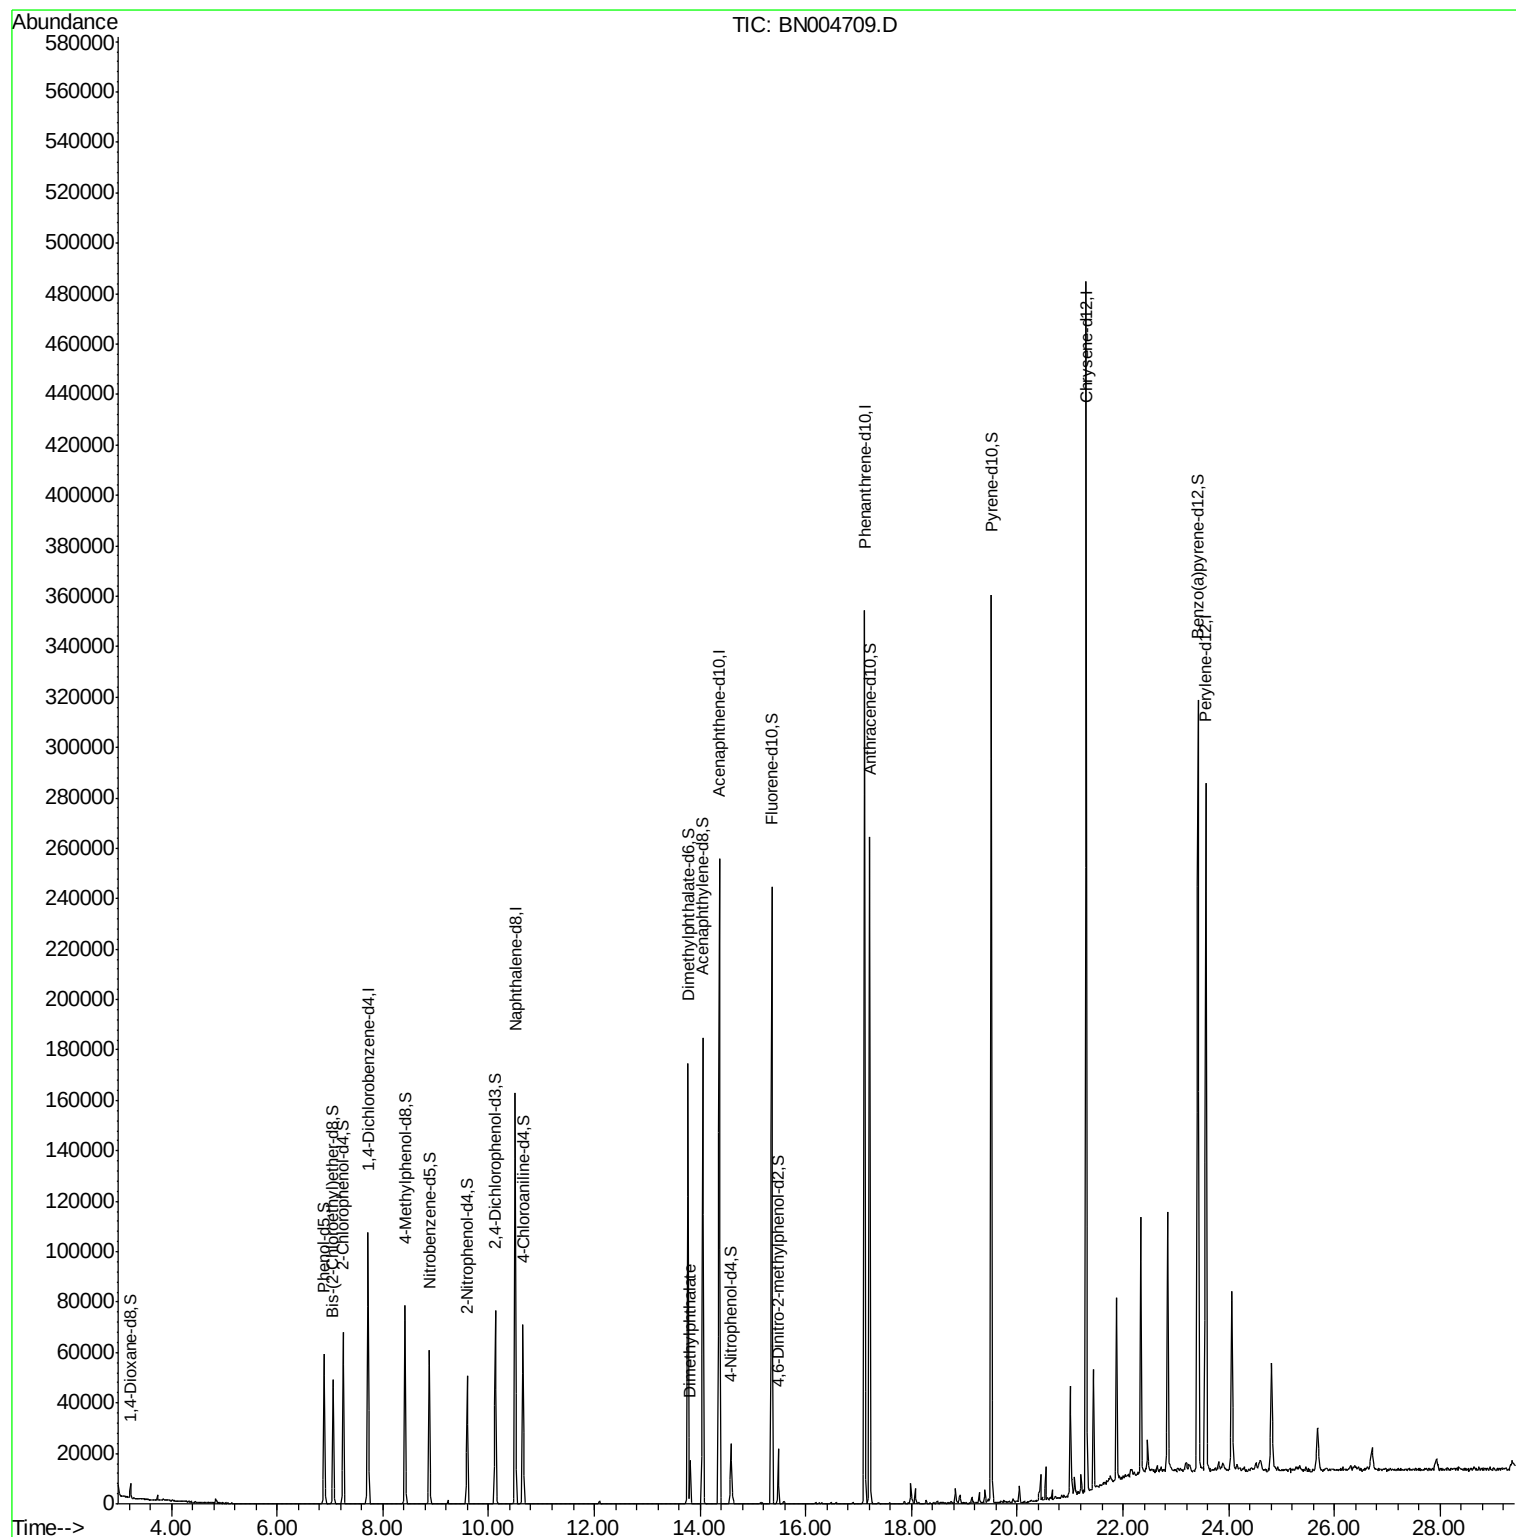

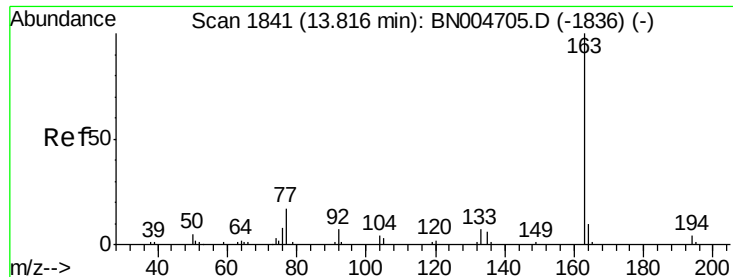

#45

Dimethylphthalate

Concen: 1.883 ng/ul

RT: 13.82 min Scan# 1841

Delta R.T. -0.01 min

Lab File: BN004709.D

Acq: 09 Mar 2019 13:17

Instrument :

BNA_N

ClientSampleId :

BF622


Tot Ion:163 Resp: 13937

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.2

164 10.4 7.9 11.9

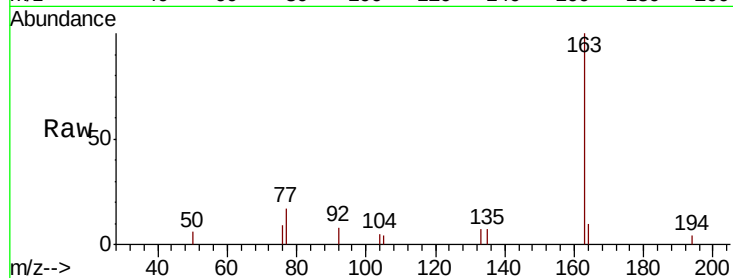

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

