
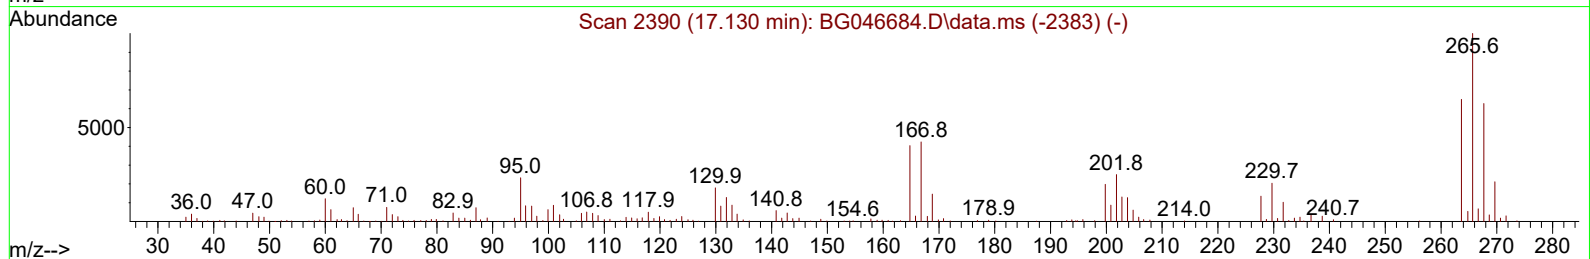
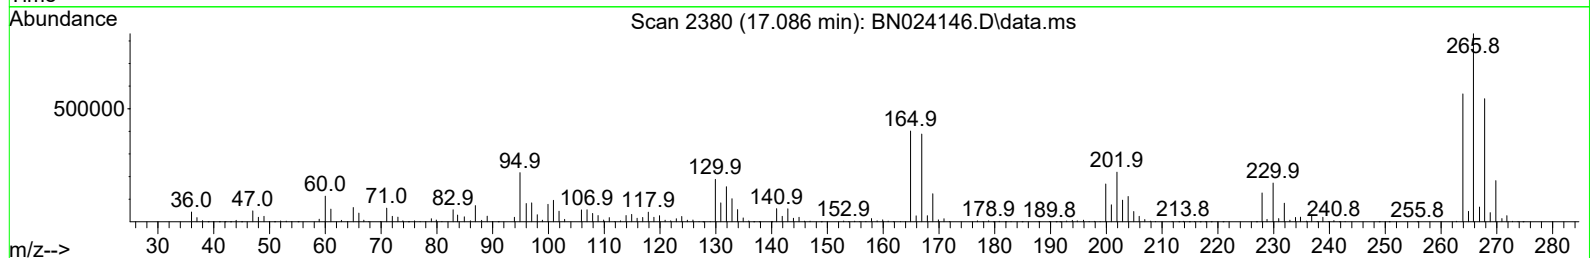


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030823\
Data File : BN024146.D
Acq On : 07 Mar 2023 15:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 06:57:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 08 06:57:10 2023
Response via : Initial Calibration

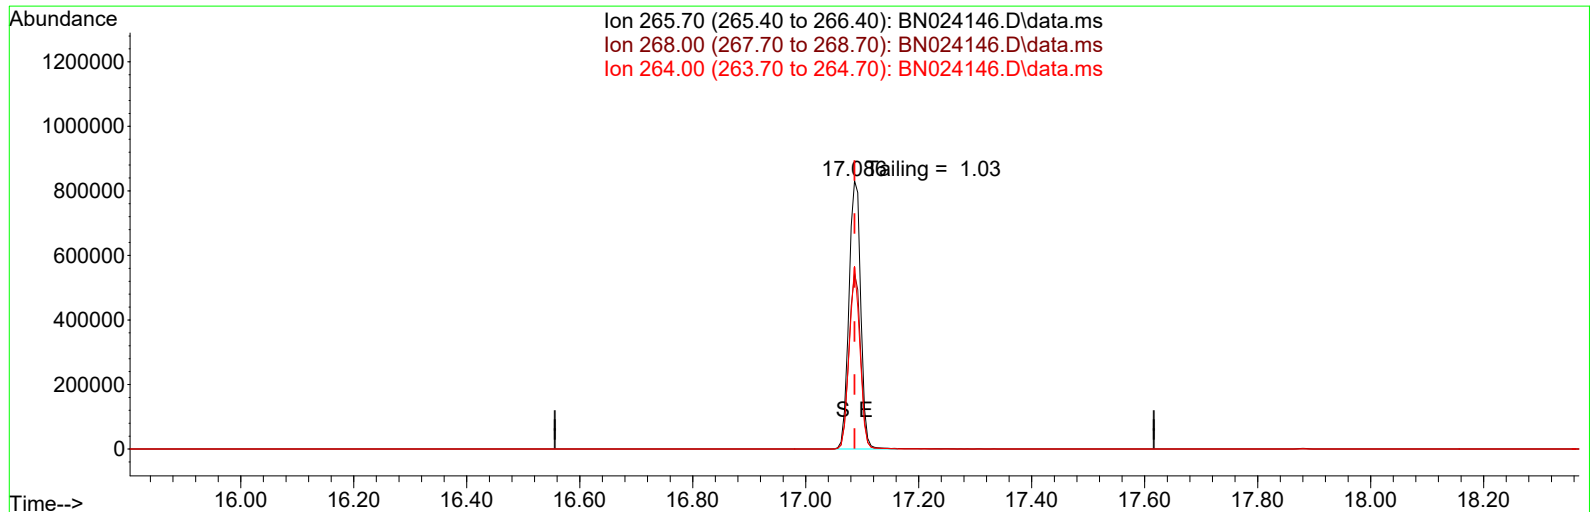

TIC: BN024146.D\data.ms

(70) Pentachlorophenol (C)




17.086min (0.000) 646825.80 ng

response 1208118

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.47
264.00	61.60	68.04
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030823\  
Data File : BN024146.D  
Acq On    : 07 Mar 2023   15:40  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Mar 08 06:57:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 08 06:57:10 2023
Response via : Initial Calibration

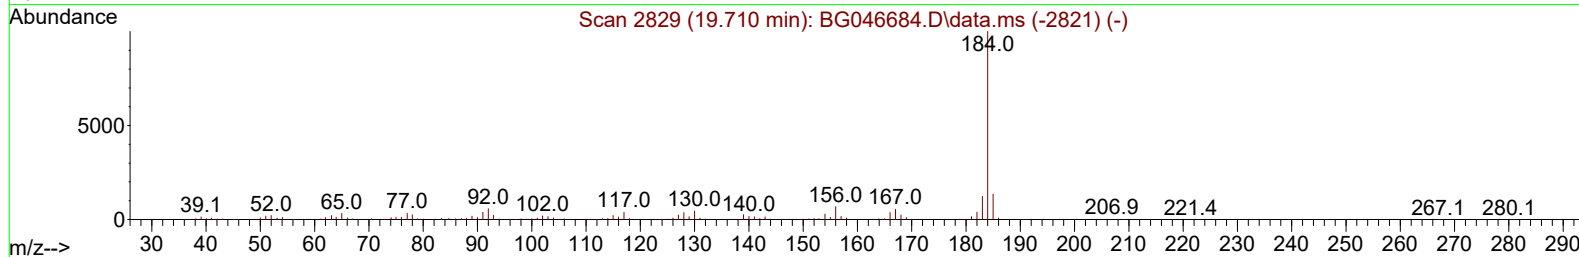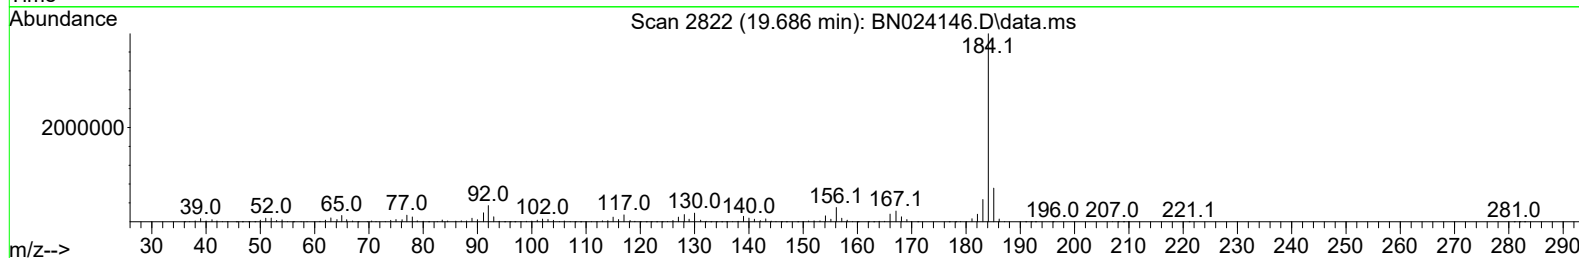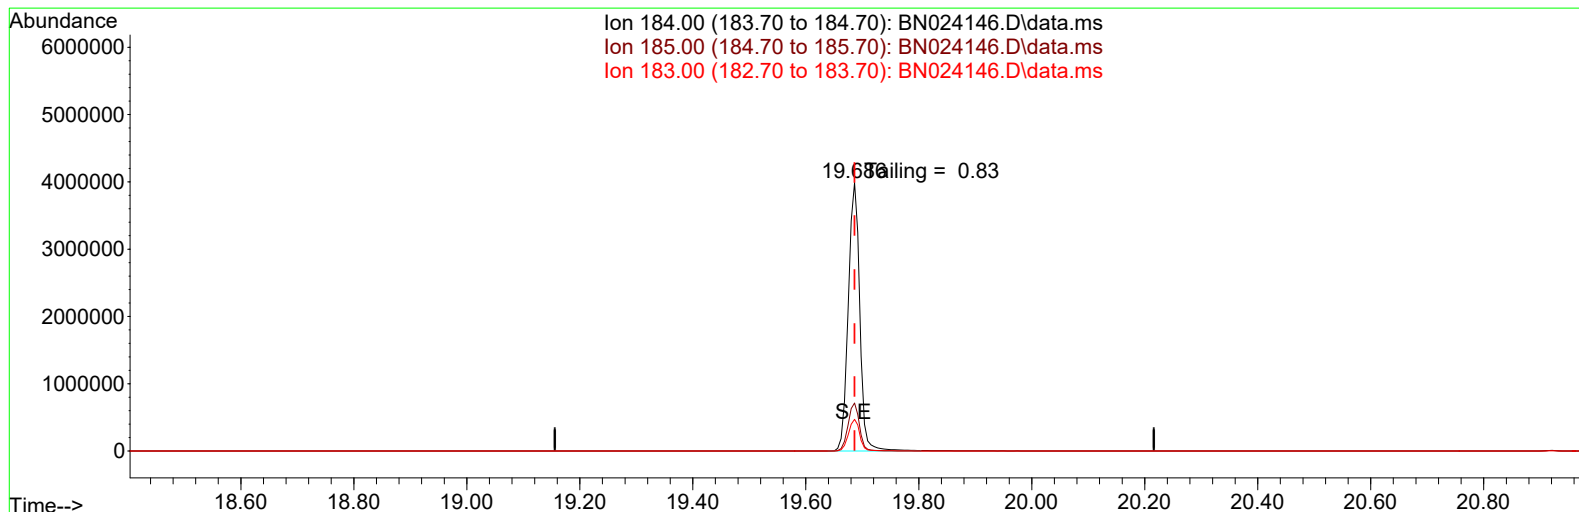

TIC: BN024146.D\data.ms

(77) Benzidine

19.686min (0.000) 912367.56 ng

response **5681062**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	17.88
183.00	13.20	11.80
0.00	0.00	0.00