


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030823\
Data File : BN024146.D
Acq On : 07 Mar 2023 15:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN030823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 08 03:54:47 2023

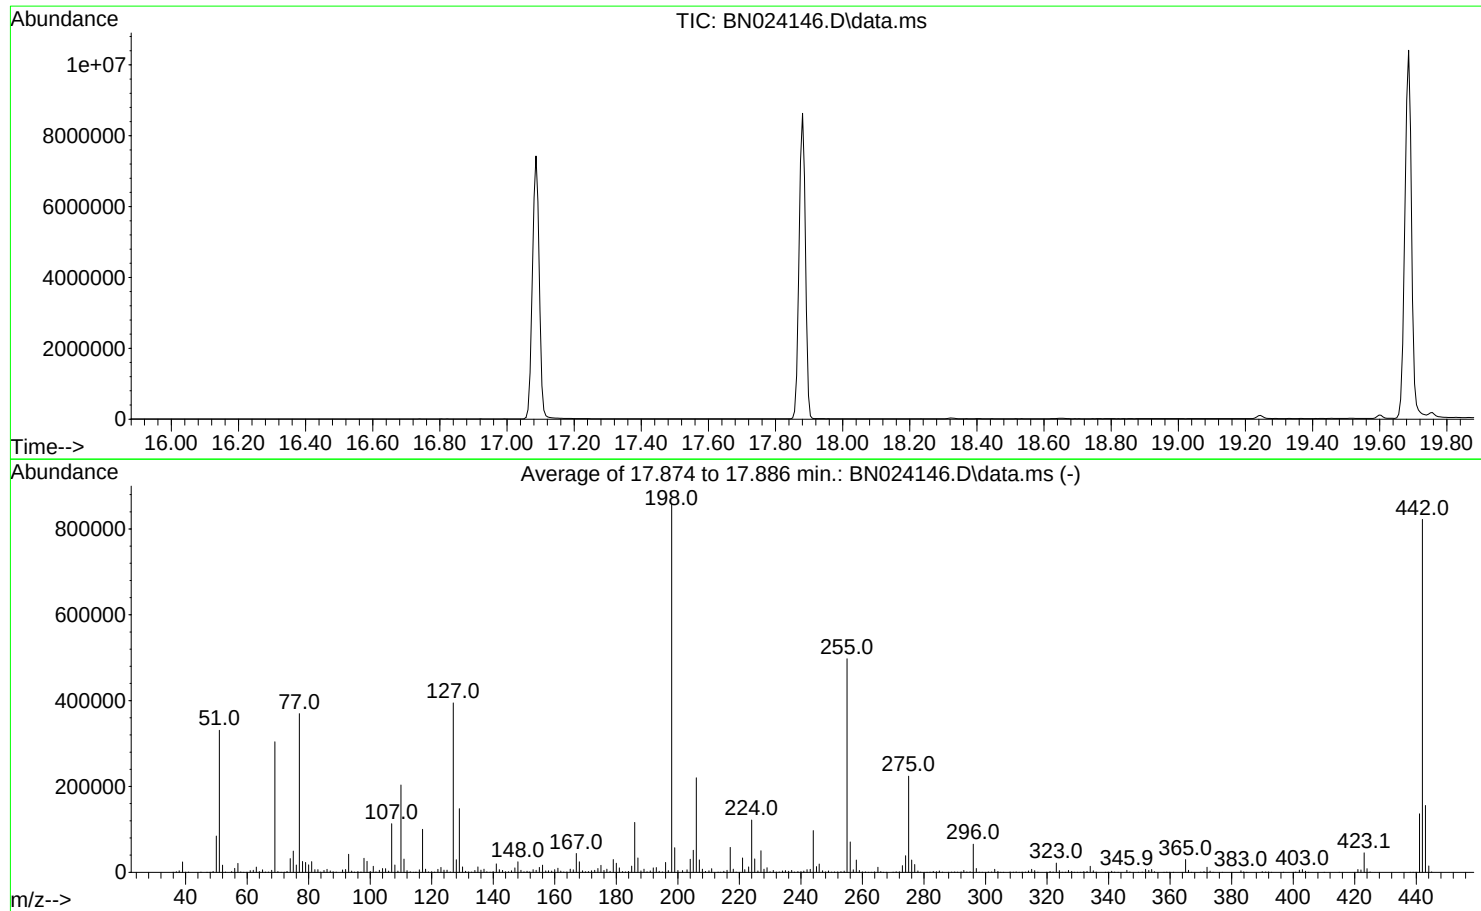




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	330731	PASS
68	69	0.00	2	1.6	4734	PASS
69	198	0.00	100	35.5	304192	PASS
70	69	0.00	2	0.5	1598	PASS
127	198	10	80	46.0	394667	PASS
197	198	0.00	2	0.5	4100	PASS
198	198	100	100	100.0	857195	PASS
199	198	5	9	6.7	57168	PASS
275	198	10	60	26.1	223808	PASS
365	198	1	100	3.4	29533	PASS
441	198	0.01	100	15.9	136323	PASS
442	442	50	100	100.0	822336	PASS
443	442	15	24	18.9	155712	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030823\
Data File : BN024146.D
Acq On : 07 Mar 2023 15:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 08 06:57:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 08 06:57:10 2023
Response via : Initial Calibration

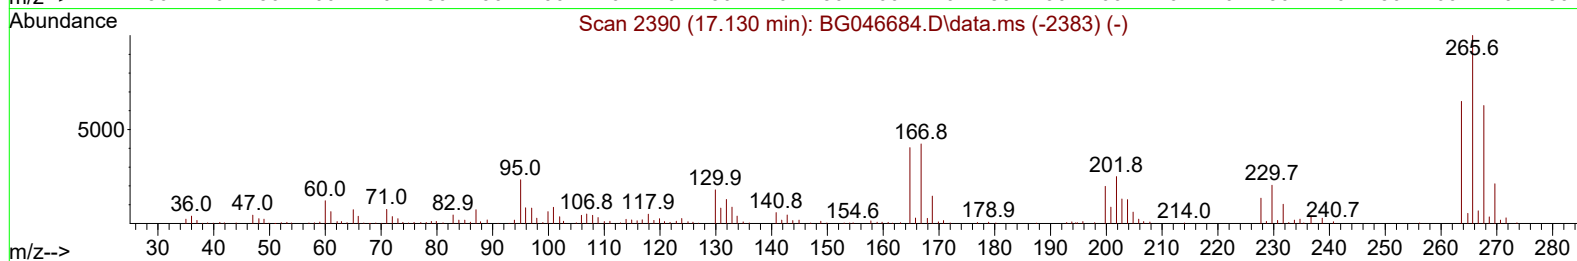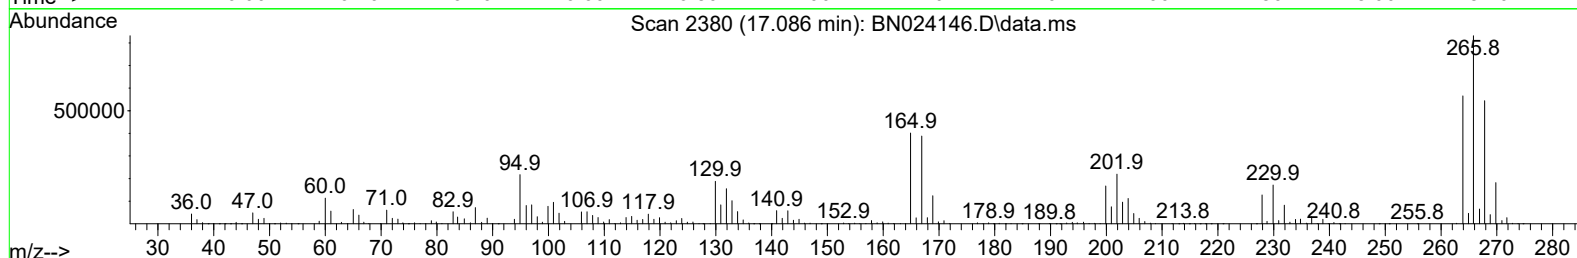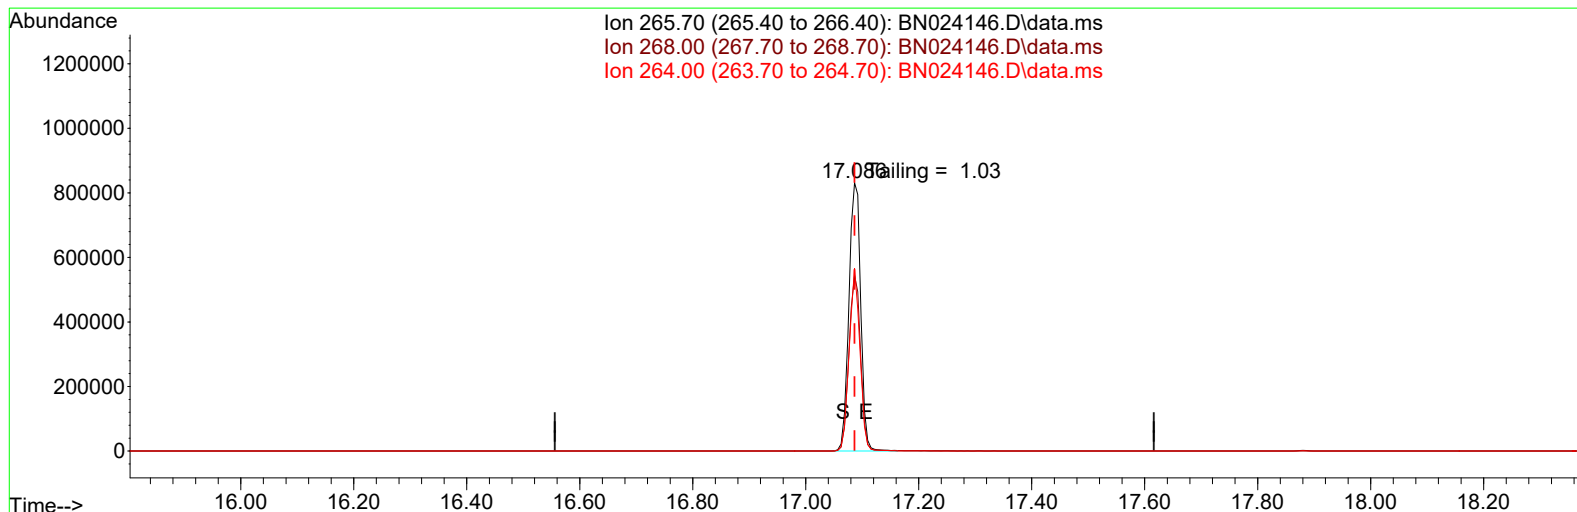

TIC: BN024146.D\data.ms

(70) Pentachlorophenol (C)

17.086min (0.000) 646825.80 ng




response 1208118

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.47
264.00	61.60	68.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030823\
Data File : BN024146.D
Acq On : 07 Mar 2023 15:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 08 06:57:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 08 06:57:10 2023
Response via : Initial Calibration

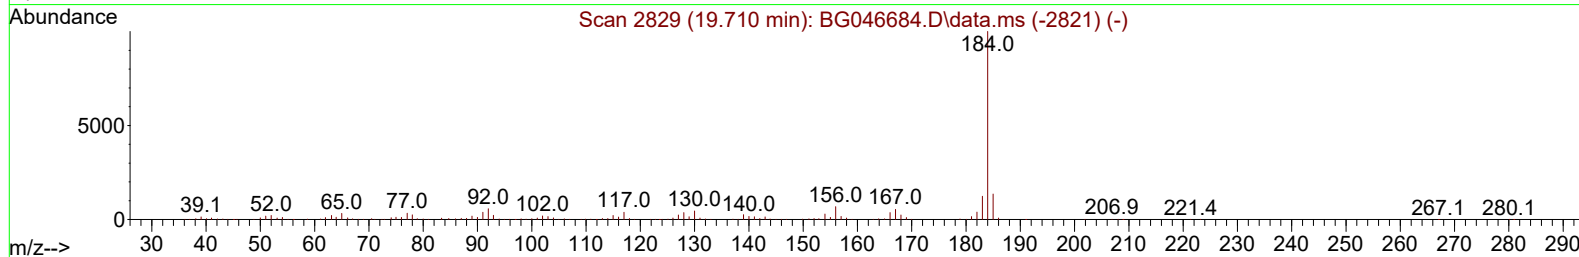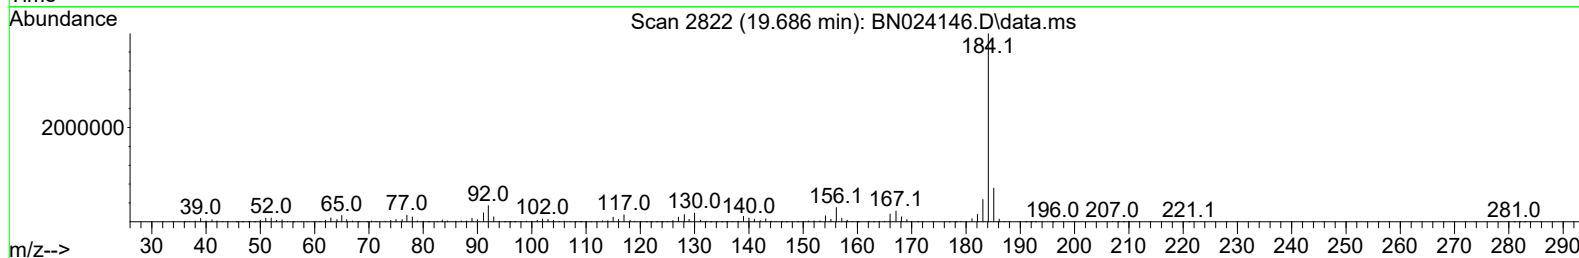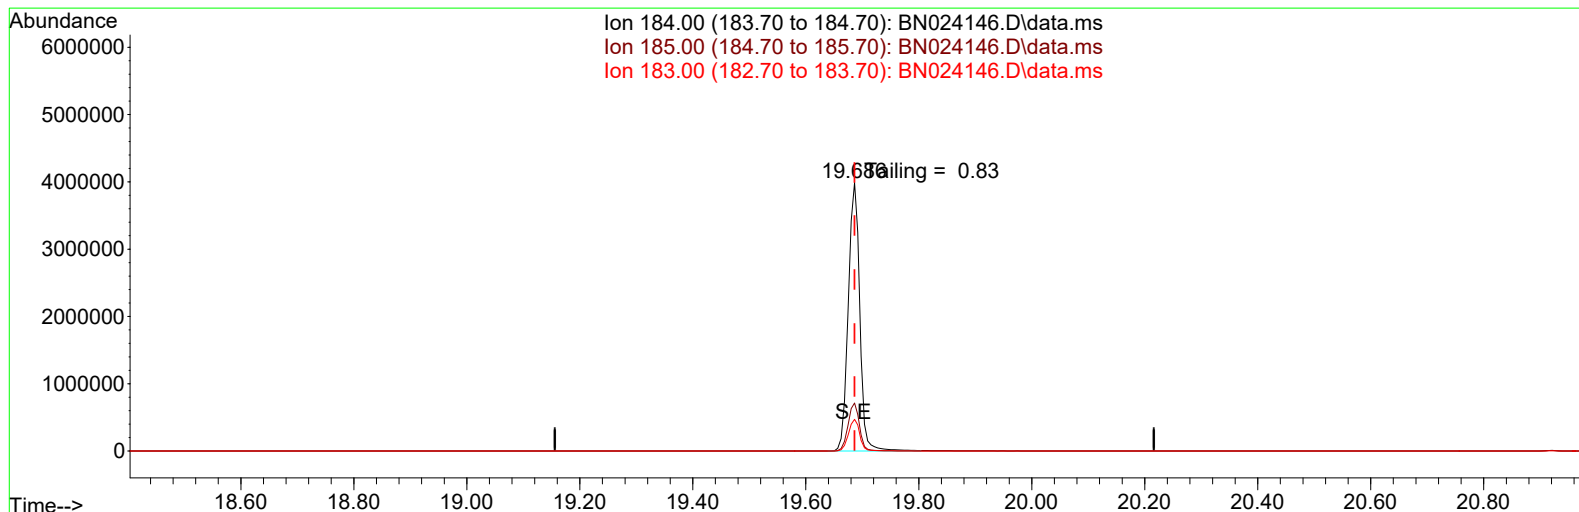

TIC: BN024146.D\data.ms

(77) Benzidine

19.686min (0.000) 912367.56 ng

response 5681062

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	17.88
183.00	13.20	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/8/2023	BNA_N	<u>BN024146.D</u>
Compound Name	Response	Retention Time
DDT	2599229	20.921
DDD	38097	20.474
DDE	560	19.963
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38657	2637886	1.47

Instrument :
BNA_N
ClientSampleId :
DFTPP