


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040622\
 Data File : BN019365.D
 Acq On : 06 Apr 2022 11:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 04 17:40:00 2022

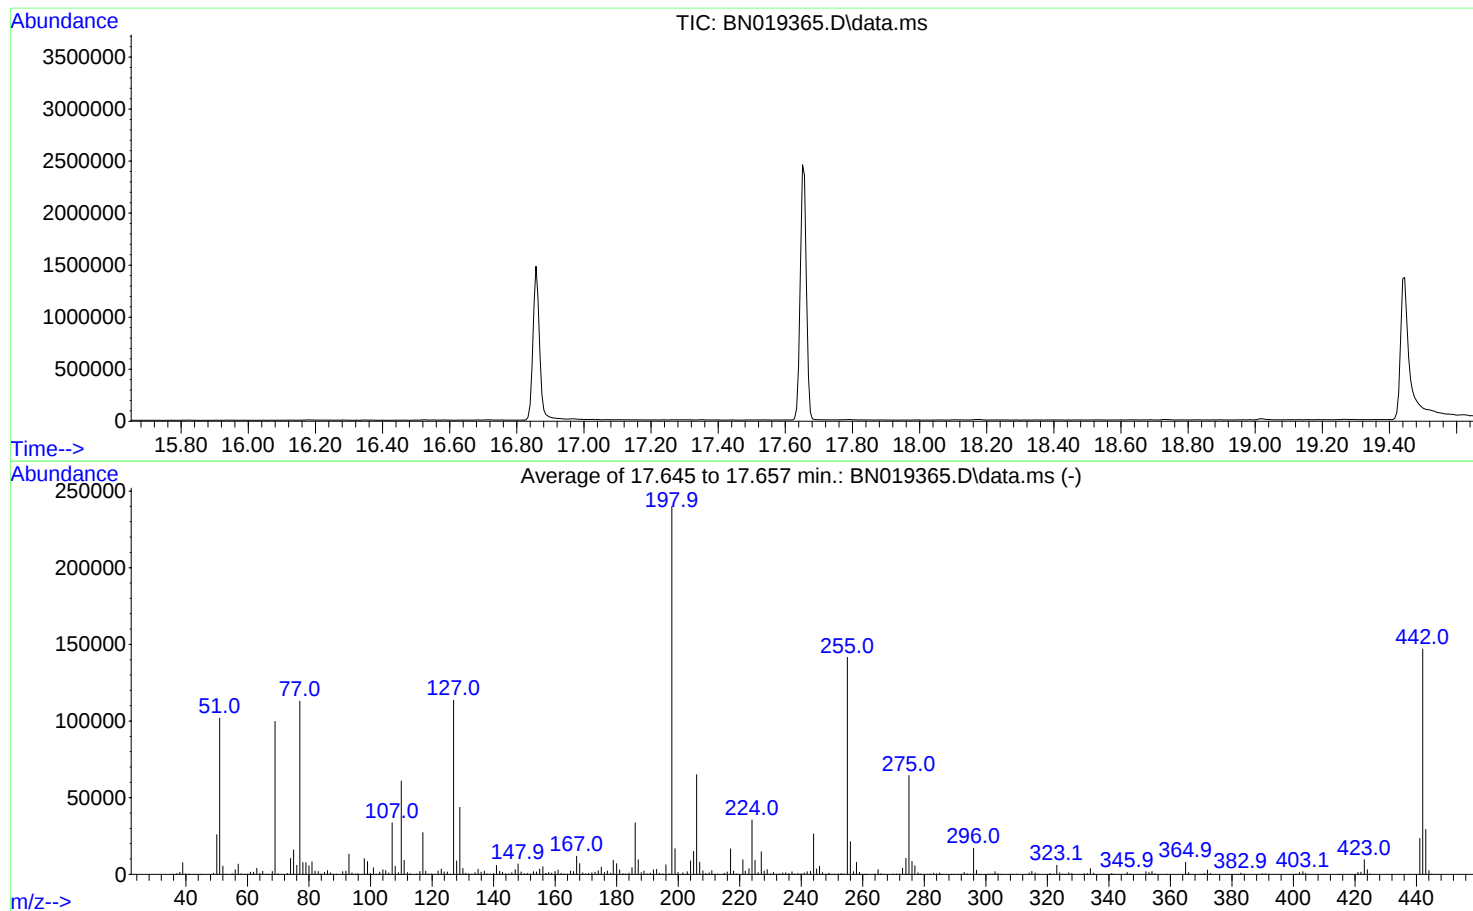




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	101888	PASS
68	69	0.00	2	1.9	1908	PASS
69	198	0.00	100	41.6	99780	PASS
70	69	0.00	2	0.4	416	PASS
127	198	10	80	47.3	113536	PASS
197	198	0.00	2	0.1	339	PASS
198	198	100	100	100.0	239936	PASS
199	198	5	9	7.0	16683	PASS
275	198	10	60	26.9	64544	PASS
365	198	1	100	3.3	7843	PASS
441	198	0.01	100	9.8	23485	PASS
442	442	50	100	100.0	146896	PASS
443	442	15	24	20.0	29364	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040622\
 Data File : BN019365.D
 Acq On : 06 Apr 2022 11:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 07 06:12:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

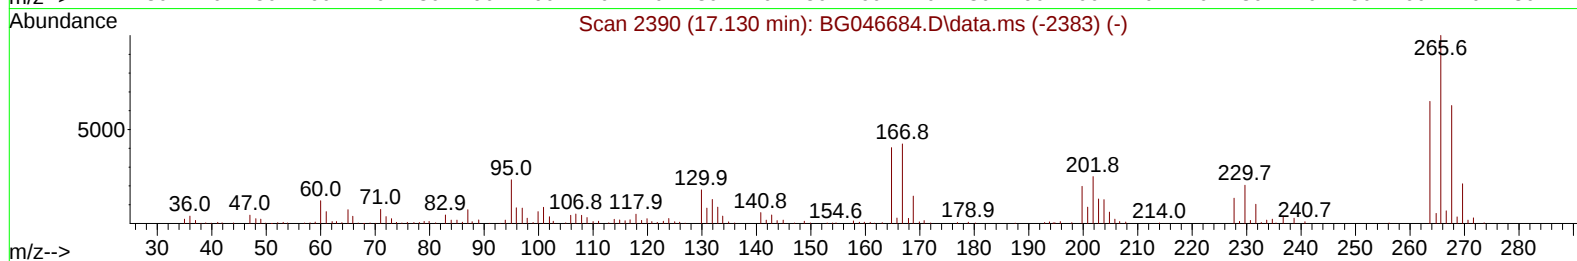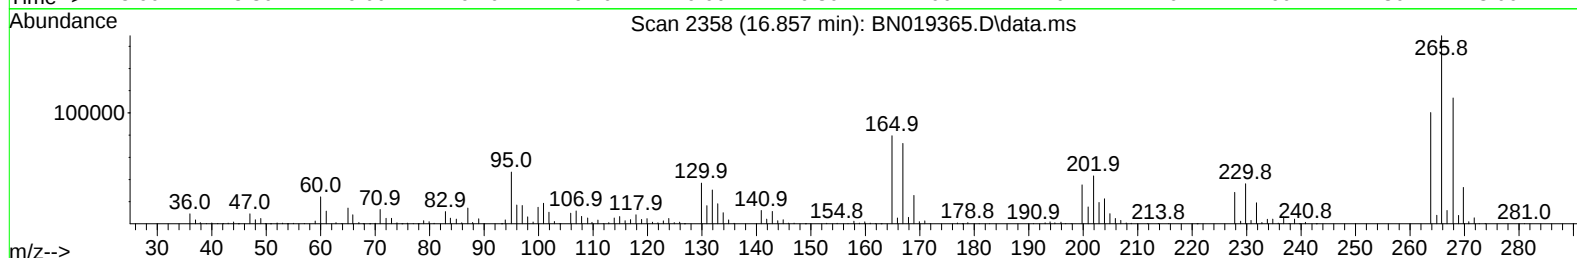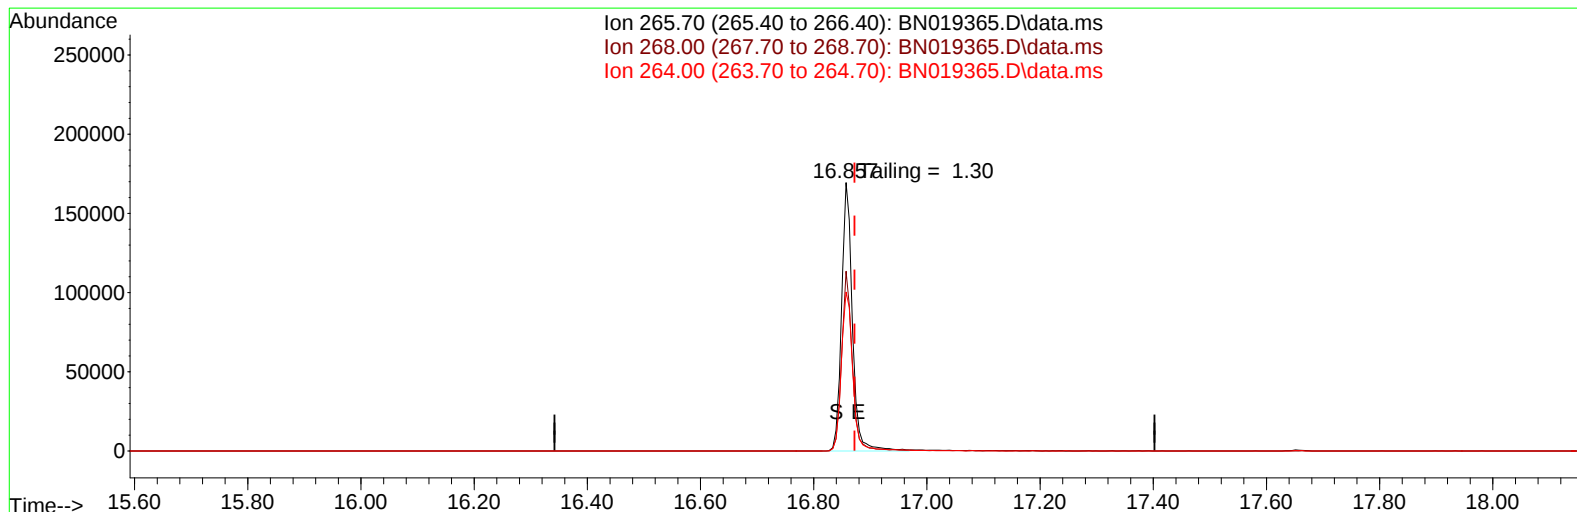

TIC: BN019365.D\data.ms

(70) Pentachlorophenol (C)

16.857min (-0.015) 17413.33 ng




response 227668

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.95
264.00	61.60	59.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040622\
Data File : BN019365.D
Acq On : 06 Apr 2022 11:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 07 06:12:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

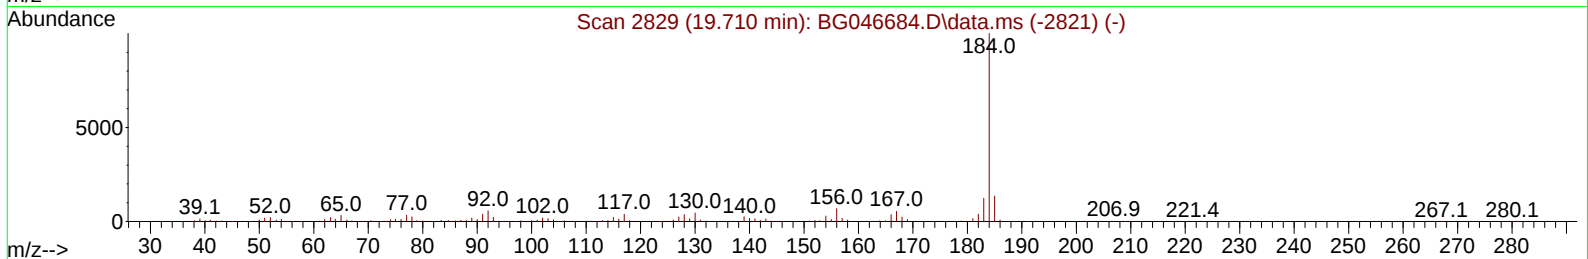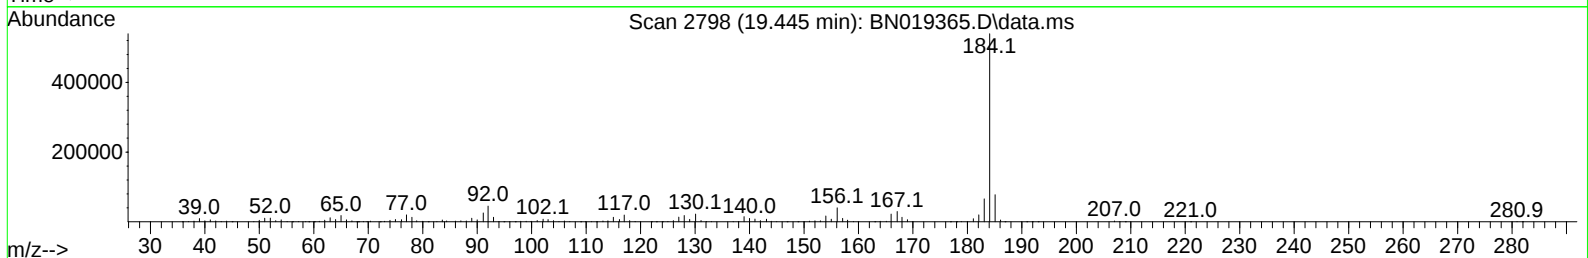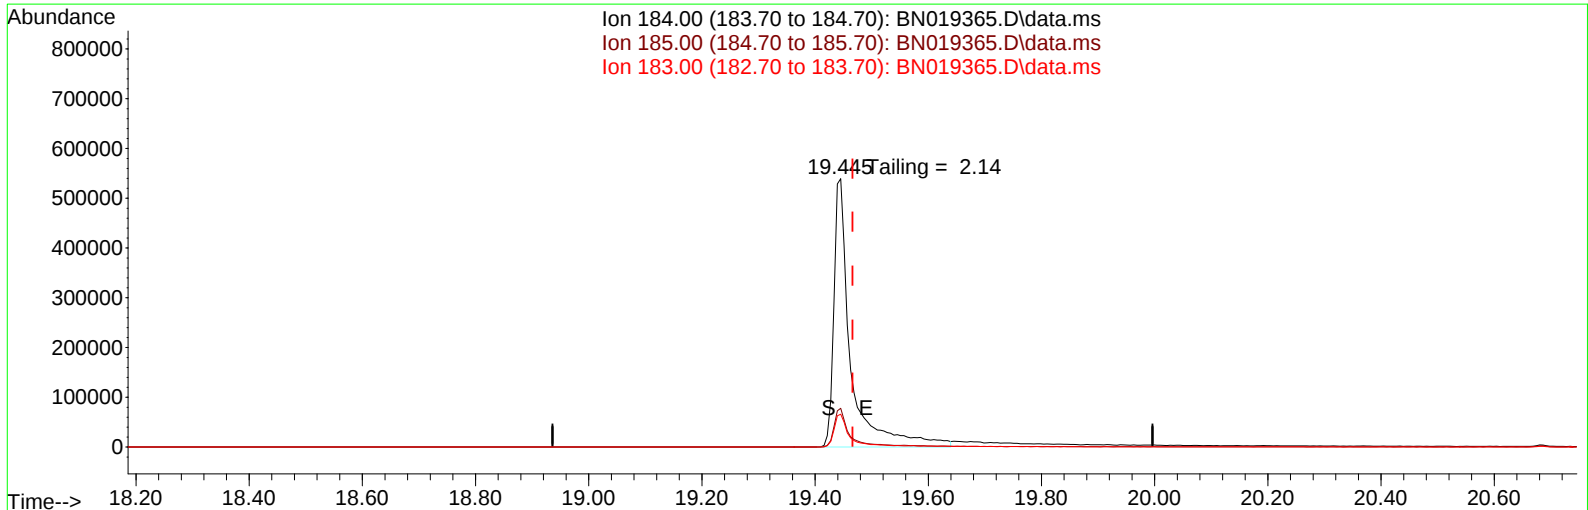

TIC: BN019365.D\data.ms

(77) Benzidine

19.445min (-0.021) 0.00 ng

response 1151481

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.42
183.00	13.20	12.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/6/2022	BNA_N	<u>BN019365.D</u>
Compound Name	Response	Retention Time
DDT	849030	20.686
DDD	12978	20.245
DDE	907	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13885	862915	1.61

Instrument :
BNA_N
ClientSampleId :
DFTPP