




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030827.D
Acq On : 10 Apr 2024 22:28
Operator : MA/JU
Sample : P2006-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0RH4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/12/2024
Supervised By :mohammad ahmed 04/12/2024

Quant Time: Apr 10 23:11:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 12:10:11 2024
Response via : Initial Calibration

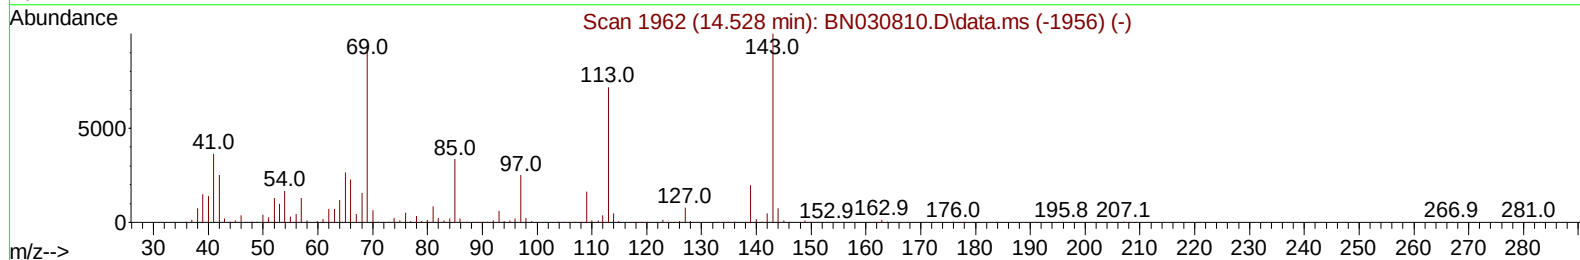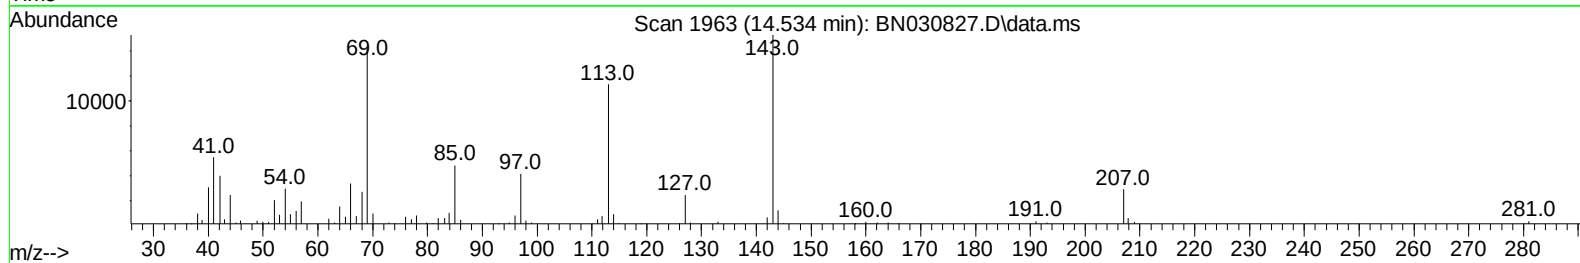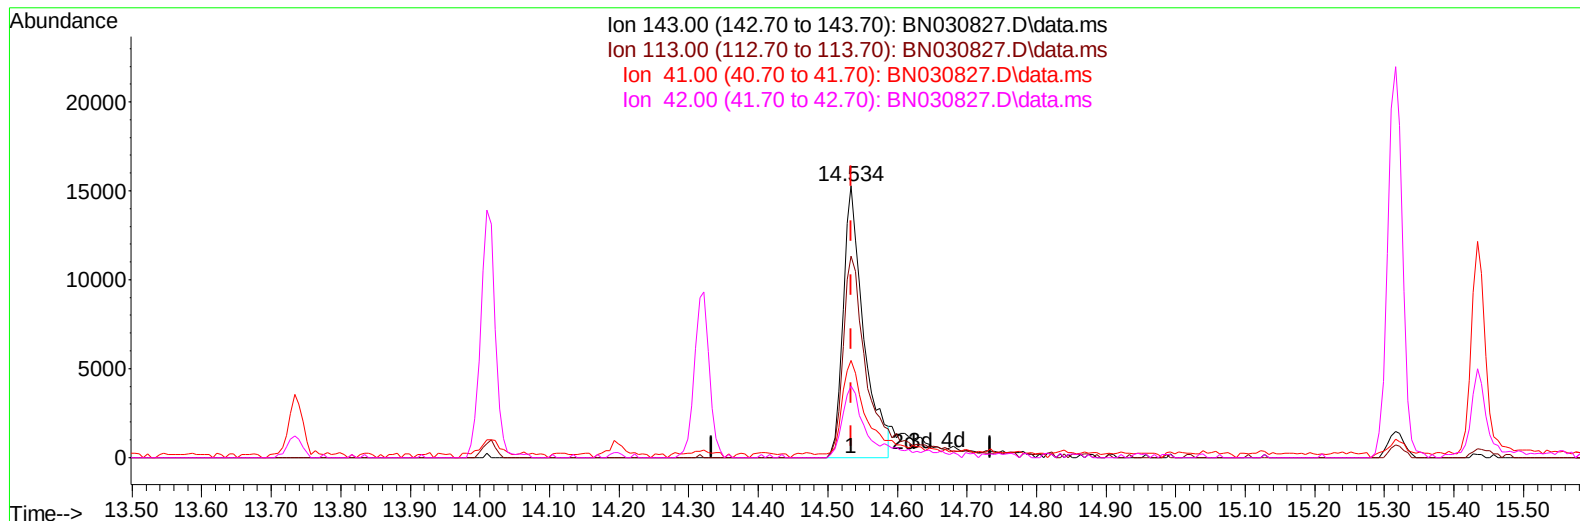

TIC: BN030827.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.534min (+ 0.000) 4.98 ng/ul****response 31130**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	72.10	74.09
41.00	38.20	35.80
42.00	26.70	26.21




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030827.D
Acq On : 10 Apr 2024 22:28
Operator : MA/JU
Sample : P2006-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0RH4

Manual IntegrationsAPPROVED

Quant Time: Apr 10 23:11:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 12:10:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/12/2024
Supervised By :mohammad ahmed 04/12/2024

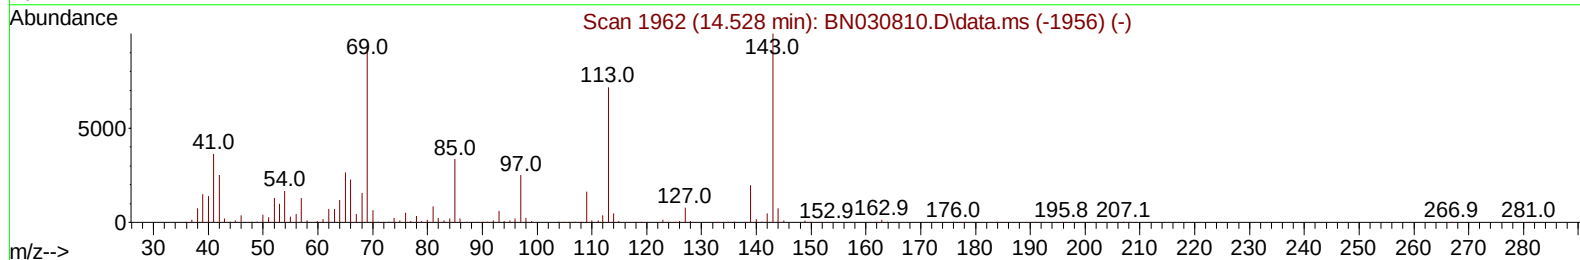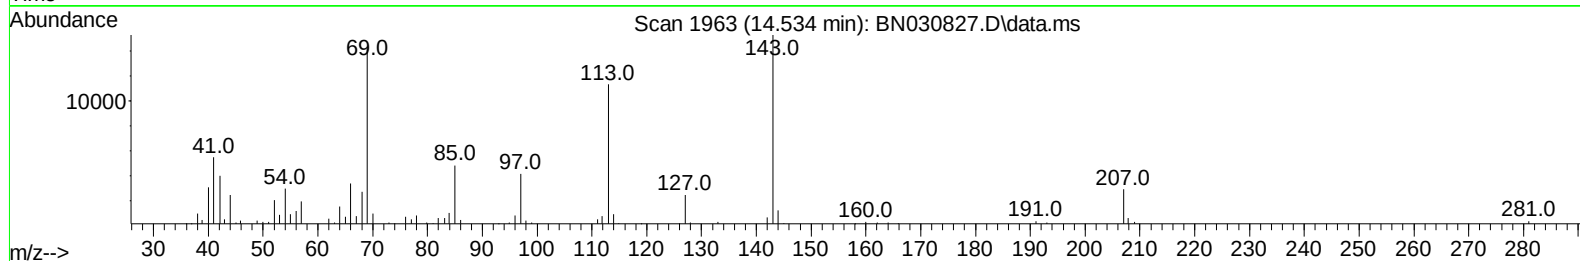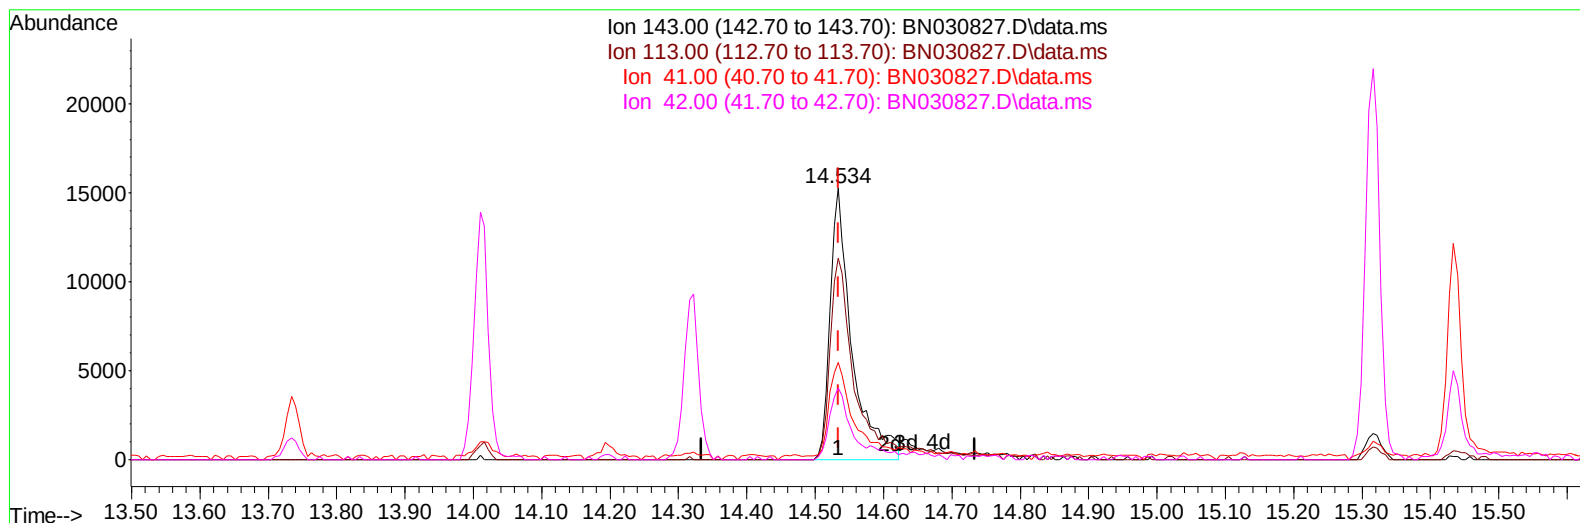

TIC: BN030827.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.534min (+ 0.000) 5.42 ng/ul m

response 33860

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	72.10	74.09
41.00	38.20	35.80
42.00	26.70	26.21

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030827.D
 Acq On : 10 Apr 2024 22:28
 Operator : MA/JU
 Sample : P2006-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MCORH4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/12/2024
 Supervised By :mohammad ahmed 04/12/2024

Quant Time: Apr 10 23:12:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 09 12:10:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.675	152	145600	20.000	ng/ul	0.00
20) Naphthalene-d8	10.457	136	683878	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.322	164	489383	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.069	188	1080224	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	1058736	20.000	ng/ul	0.00
88) Perylene-d12	24.239	264	1094502	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	17424	5.611	ng/uL	0.00
4) Pyridine-d5	3.593	84	142522	15.307	ng/ul	0.00
7) Phenol-d5	6.852	99	103758	8.809	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.016	67	321719	44.223	ng/ul	0.00
11) 2-Chlorophenol-d4	7.210	132	323198	36.172	ng/ul	0.00
15) 4-Methylphenol-d8	8.381	113	214112	21.690	ng/ul	0.00
21) Nitrobenzene-d5	8.834	128	228915	48.253	ng/ul	0.00
24) 2-Nitrophenol-d4	9.552	143	225627	51.989	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.081	165	404366	42.560	ng/ul	0.00
31) 4-Chloroaniline-d4	10.599	131	521166	33.319	ng/ul	0.00
46) Dimethylphthalate-d6	13.740	166	1566451	47.942	ng/ul	0.00
49) Acenaphthylene-d8	14.010	160	1766351	47.018	ng/ul	0.00
54) 4-Nitrophenol-d4	14.534	143	33860m	5.418	ng/ul	0.00
60) Fluorene-d10	15.316	176	1381071	48.302	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.434	200	190924	40.042	ng/ul	0.00
73) Anthracene-d10	17.169	188	2311267	49.659	ng/ul	0.00
81) Pyrene-d10	19.469	212	2858380	50.216	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.039	264	2719987	53.934	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030827.D
Acq On : 10 Apr 2024 22:28
Operator : MA/JU
Sample : P2006-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0RH4

Manual IntegrationsAPPROVED

Quant Time: Apr 10 23:12:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 12:10:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/12/2024
Supervised By :mohammad ahmed 04/12/2024

