

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030822.D
 Acq On : 10 Apr 2024 18:31
 Operator : MA/JU
 Sample : P2006-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MCORF3

Quant Time: Apr 10 19:16:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 09 12:10:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.681	152	174498	20.000	ng/u1	0.00
20) Naphthalene-d8	10.463	136	813421	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.322	164	556918	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.069	188	1219044	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	1203746	20.000	ng/u1	0.00
88) Perylene-d12	24.239	264	1259550	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	15785	4.241	ng/uL	0.00
4) Pyridine-d5	3.599	84	101107	9.061	ng/u1	0.00
7) Phenol-d5	6.852	99	91088	6.453	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.016	67	276579	31.722	ng/u1	0.00
11) 2-Chlorophenol-d4	7.210	132	277908	25.952	ng/u1	0.00
15) 4-Methylphenol-d8	8.381	113	190787	16.126	ng/u1	0.00
21) Nitrobenzene-d5	8.834	128	192688	34.149	ng/u1	0.00
24) 2-Nitrophenol-d4	9.552	143	194600	37.699	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.081	165	366883	32.465	ng/u1	0.00
31) 4-Chloroaniline-d4	10.604	131	457184	24.574	ng/u1	0.00
46) Dimethylphthalate-d6	13.740	166	1512513	40.678	ng/u1	0.00
49) Acenaphthylene-d8	14.010	160	1668840	39.036	ng/u1	0.00
54) 4-Nitrophenol-d4	14.534	143	36839	5.180	ng/u1	0.00
60) Fluorene-d10	15.316	176	1345398	41.348	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.434	200	189358	35.192	ng/u1	0.00
73) Anthracene-d10	17.169	188	2245043	42.743	ng/u1	0.00
81) Pyrene-d10	19.469	212	2694013	41.627	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.045	264	2618302	45.114	ng/u1	0.00
Target Compounds						
					Qvalue	
75) 1,2,3,4-Tetrachloroben...	13.110	216	26001	1.736	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030822.D
Acq On : 10 Apr 2024 18:31
Operator : MA/JU
Sample : P2006-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0RF3


Quant Time: Apr 10 19:16:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 12:10:11 2024
Response via : Initial Calibration

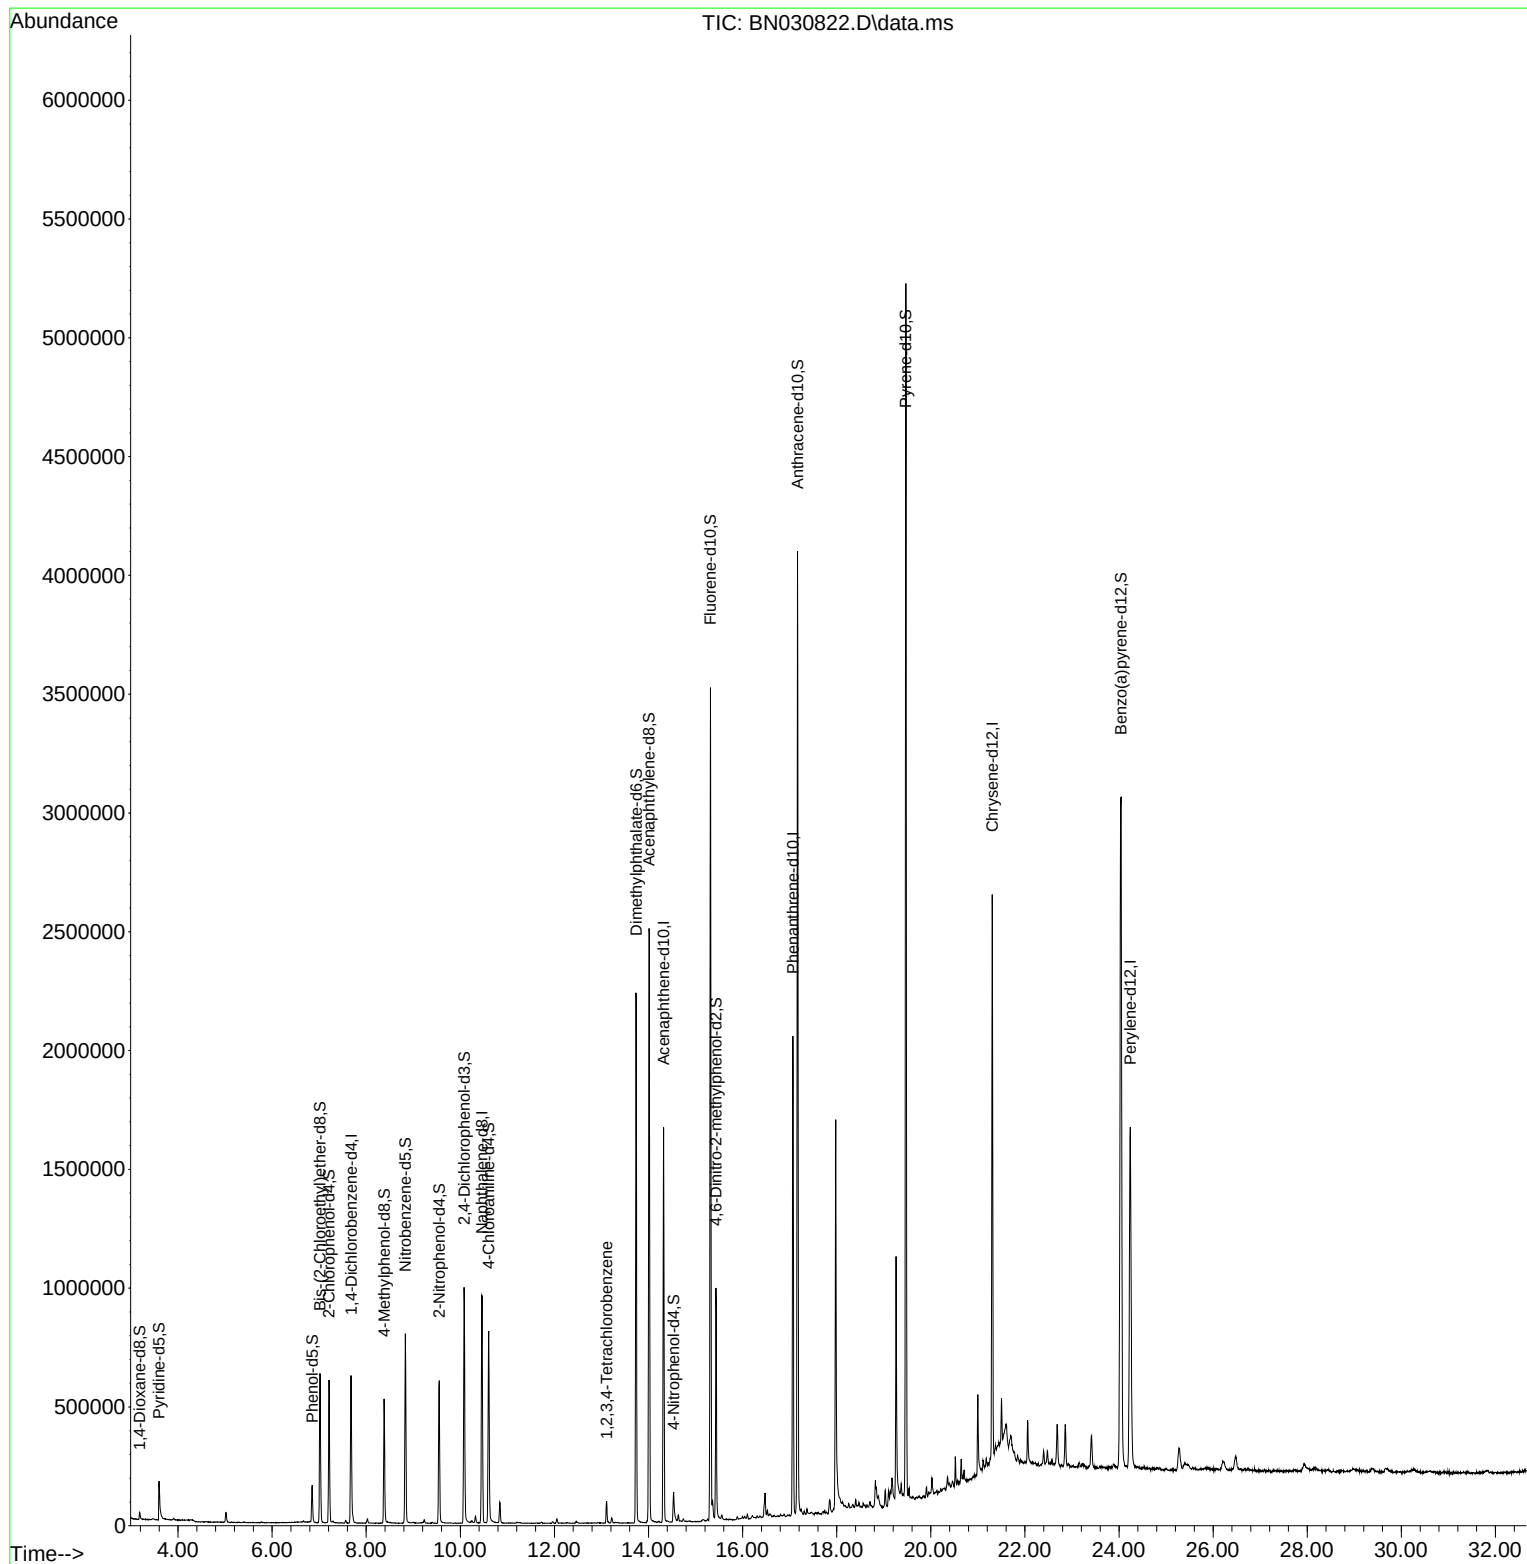

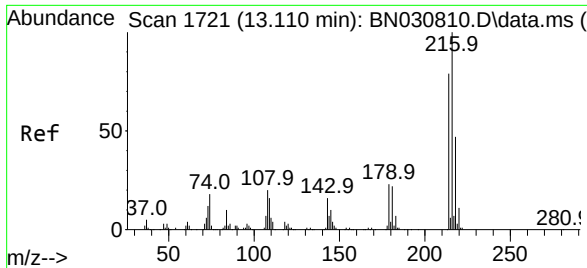

#75
 1,2,3,4-Tetrachlorobenzene
 Concen: 1.736 ng/uL
 RT: 13.110 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN030822.D
 Acq: 10 Apr 2024 18:31

Instrument :
 BNA_N
 ClientSampleId :
 MC0RF3

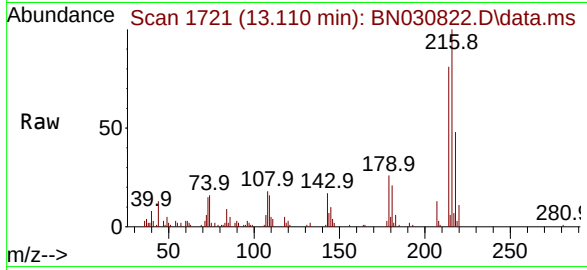

Tgt Ion:	216	Resp:	26001
Ion Ratio	Lower	Upper	
216	100		
214	81.3	63.1	94.7
218	47.7	39.5	59.3

