

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030829.D
 Acq On : 10 Apr 2024 23:47
 Operator : MA/JU
 Sample : P1970-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAK0

Quant Time: Apr 11 00:20:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 09 12:10:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.675	152	221947	20.000	ng/u1	0.00
20) Naphthalene-d8	10.458	136	1009672	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.322	164	704801	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.069	188	1555701	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	1424707	20.000	ng/u1	0.00
88) Perylene-d12	24.233	264	1341446	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	18674	3.945	ng/uL	0.00
4) Pyridine-d5	3.599	84	109898	7.743	ng/u1	0.00
7) Phenol-d5	6.846	99	109021	6.072	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.017	67	338773	30.549	ng/u1	0.00
11) 2-Chlorophenol-d4	7.211	132	338874	24.880	ng/u1	0.00
15) 4-Methylphenol-d8	8.381	113	229936	15.281	ng/u1	0.00
21) Nitrobenzene-d5	8.834	128	241009	34.410	ng/u1	0.00
24) 2-Nitrophenol-d4	9.546	143	233235	36.401	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.081	165	434936	31.006	ng/u1	0.00
31) 4-Chloroaniline-d4	10.605	131	315165	13.648	ng/u1	0.00
46) Dimethylphthalate-d6	13.734	166	1777113	37.766	ng/u1	0.00
49) Acenaphthylene-d8	14.010	160	1950542	36.052	ng/u1	0.00
54) 4-Nitrophenol-d4	14.534	143	38304	4.256	ng/u1	0.00
60) Fluorene-d10	15.316	176	1562795	37.952	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.434	200	221385	32.240	ng/u1	0.00
73) Anthracene-d10	17.169	188	2556638	38.142	ng/u1	0.00
81) Pyrene-d10	19.469	212	2989589	39.030	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.039	264	2493095	40.334	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.223	88	9828	1.938 ng/uL	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030829.D
Acq On : 10 Apr 2024 23:47
Operator : MA/JU
Sample : P1970-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK0


Quant Time: Apr 11 00:20:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 12:10:11 2024
Response via : Initial Calibration

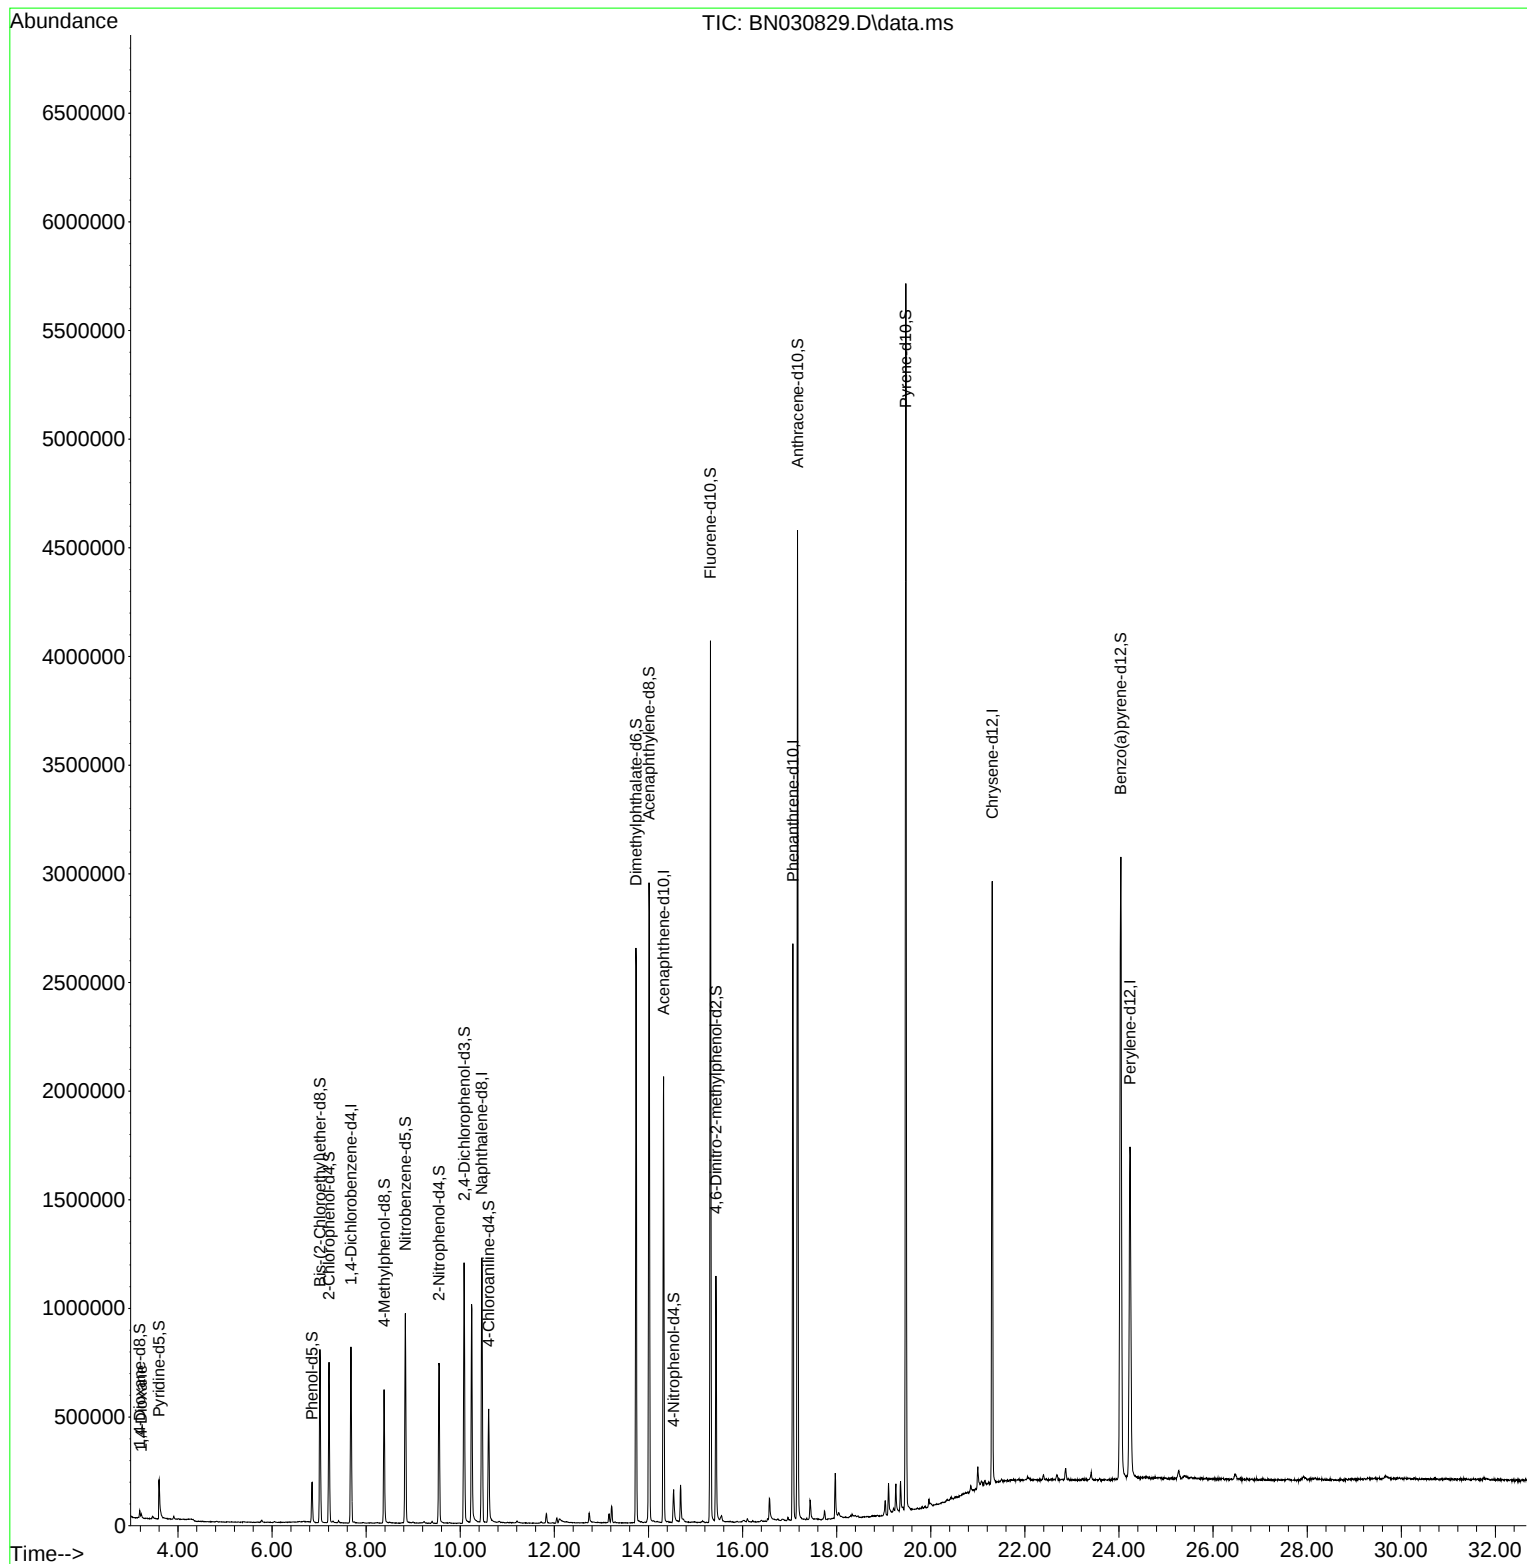

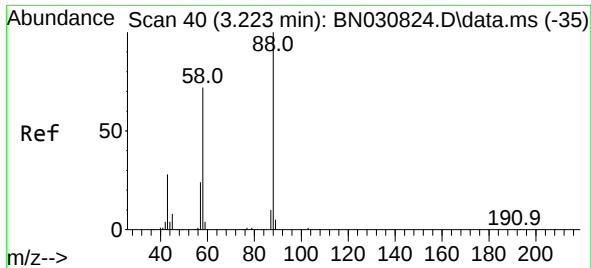

#2
 1,4-Dioxane
 Concen: 1.938 ng/uL
 RT: 3.223 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: BN030829.D
 Acq: 10 Apr 2024 23:47

Instrument :
 BNA_N
 ClientSampleId :
 C0AK0

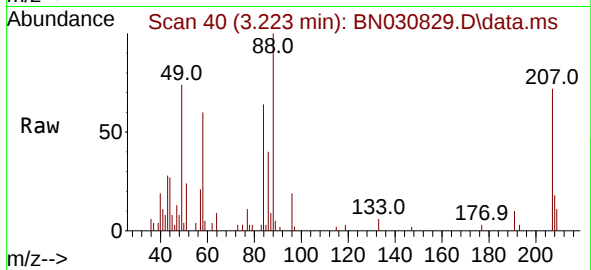

Tgt Ion:	88	Resp:	9828
Ion	Ratio	Lower	Upper
88	100		
43	27.5	23.8	35.8
58	59.9	56.6	84.8

