

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030812.D
 Acq On : 10 Apr 2024 11:09
 Operator : MA/JU
 Sample : PB160122BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK122

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030812.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	31	34	45	rVB	41477	64360	1.13%	0.119%
2	3.593	99	103	126	rBV	549404	961491	16.95%	1.772%
3	3.917	154	158	160	rVB3	6107	7442	0.13%	0.014%
4	6.852	650	657	671	rBV	709942	1144668	20.17%	2.109%
5	7.022	679	686	695	rVB	601853	950702	16.76%	1.752%
6	7.211	711	718	730	rBV	741663	1147132	20.22%	2.114%
7	7.675	790	797	806	rBV	606122	989042	17.43%	1.823%
8	8.381	911	917	931	rBV	959367	1515916	26.72%	2.793%
9	8.834	984	994	1006	rBV	732216	1179145	20.78%	2.173%
10	9.552	1108	1116	1128	rBV	577783	930715	16.40%	1.715%
11	10.081	1199	1206	1220	rBV	970655	1611660	28.41%	2.970%
12	10.457	1263	1270	1281	rBV	923508	1580698	27.86%	2.913%
13	10.604	1287	1295	1315	rBV	1052584	1858440	32.75%	3.425%
14	12.057	1536	1542	1548	rBV	15002	26797	0.47%	0.049%
15	13.216	1734	1739	1744	rVB3	9131	14261	0.25%	0.026%
16	13.734	1820	1827	1839	rBV	1885101	2645941	46.63%	4.876%
17	14.016	1867	1875	1888	rBV	2173495	3243245	57.16%	5.977%
18	14.322	1920	1927	1939	rBV	1668791	2392453	42.17%	4.409%
19	14.528	1955	1962	1986	rBV	649852	1229207	21.66%	2.265%
20	15.316	2089	2096	2106	rBV	2921591	4108248	72.41%	7.570%
21	15.434	2110	2116	2131	rVV	714527	1035256	18.25%	1.908%
22	15.557	2133	2137	2141	rVB2	15277	21372	0.38%	0.039%
23	16.104	2225	2230	2235	rBV3	9204	12807	0.23%	0.024%
24	17.069	2388	2394	2404	rBV	2177023	3015080	53.14%	5.556%
25	17.169	2404	2411	2429	rVB	3336265	4820810	84.97%	8.884%
26	19.033	2724	2728	2732	rVB	39690	49753	0.88%	0.092%
27	19.104	2736	2740	2744	rBV	33527	46125	0.81%	0.085%
28	19.469	2796	2802	2813	rBV	4220886	5673823	100.00%	10.455%
29	21.304	3109	3114	3125	rBV2	2357002	3312833	58.39%	6.105%
30	24.039	3570	3579	3596	rVB	2318289	5281412	93.08%	9.732%
31	24.239	3604	3613	3637	rVB	1324867	3395763	59.85%	6.258%




Sum of corrected areas: 54266597

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030812.D
Acq On : 10 Apr 2024 11:09
Operator : MA/JU
Sample : PB160122BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

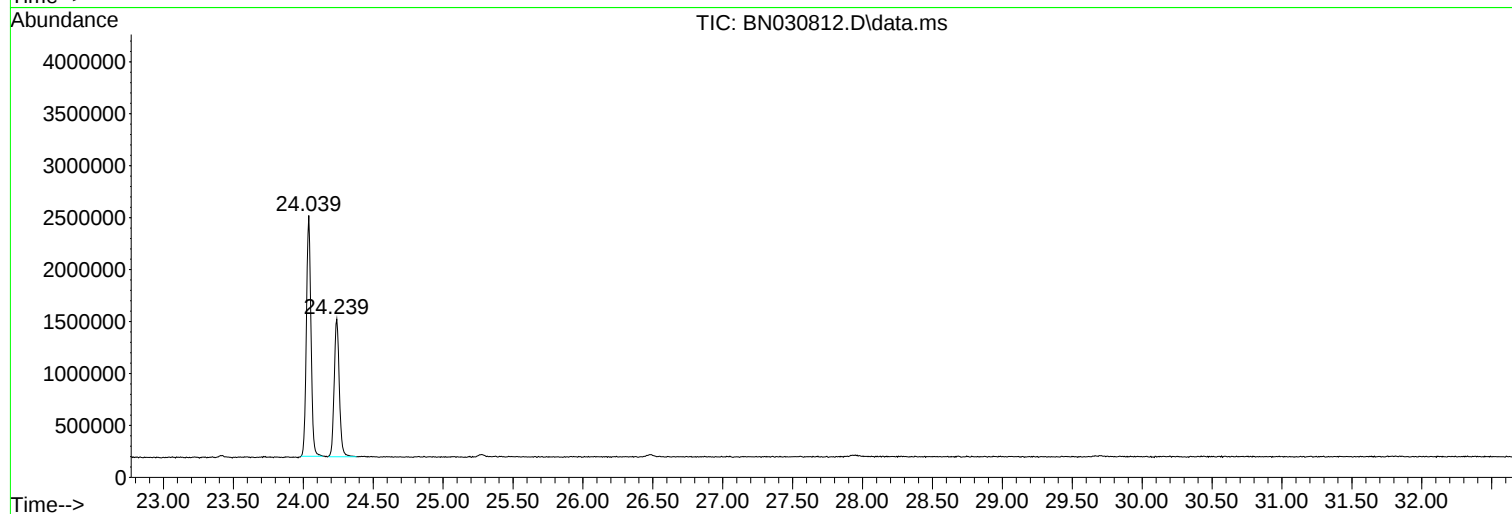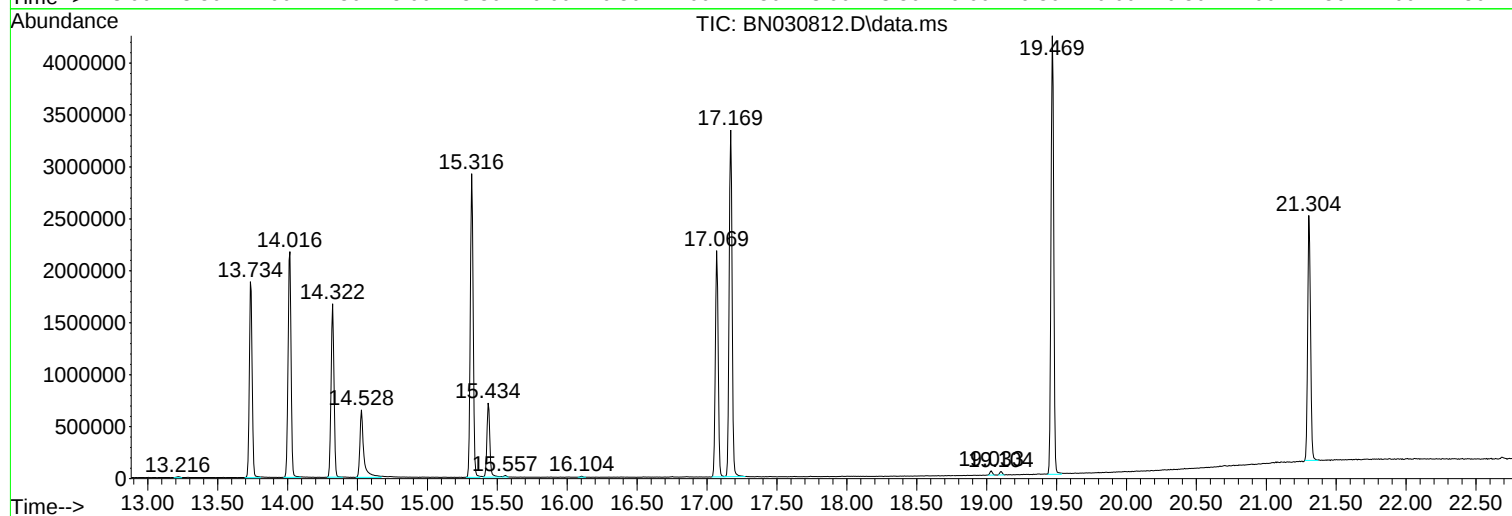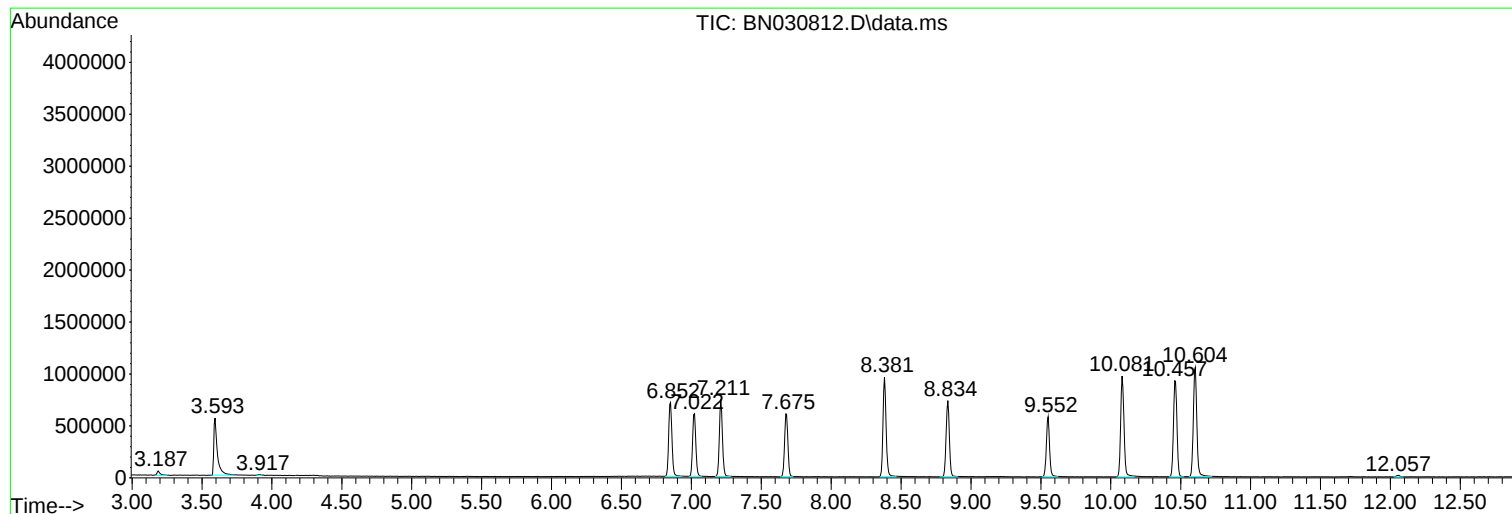

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030812.D
Acq On : 10 Apr 2024 11:09
Operator : MA/JU
Sample : PB160122BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030812.D
Acq On : 10 Apr 2024 11:09
Operator : MA/JU
Sample : PB160122BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc