

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030813.D
 Acq On : 10 Apr 2024 12:27
 Operator : MA/JU
 Sample : P1948-16DL 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AK5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	25	29	36	rBV	22588	35456	1.10%	0.204%
2	3.222	36	40	48	rVB	48374	69309	2.16%	0.399%
3	3.452	76	79	81	rBV4	3847	5860	0.18%	0.034%
4	3.911	154	157	160	rBV2	5925	7146	0.22%	0.041%
5	4.434	242	246	248	rBV5	2935	3680	0.11%	0.021%
6	6.728	633	636	640	rBV6	2335	4150	0.13%	0.024%
7	6.852	653	657	664	rBV5	7057	13637	0.42%	0.079%
8	7.022	681	686	695	rVB	42648	68245	2.12%	0.393%
9	7.210	713	718	725	rBV	27928	49789	1.55%	0.287%
10	7.681	791	798	810	rBV	575761	933963	29.06%	5.378%
11	7.793	813	817	825	rVB6	10296	15768	0.49%	0.091%
12	8.381	911	917	924	rBV3	20184	36840	1.15%	0.212%
13	8.834	989	994	1001	rBV	42834	72498	2.26%	0.417%
14	9.551	1111	1116	1122	rBV2	22218	39188	1.22%	0.226%
15	10.087	1200	1207	1220	rBV	37503	73612	2.29%	0.424%
16	10.463	1262	1271	1281	rBV	871215	1498211	46.62%	8.626%
17	10.604	1289	1295	1302	rBV2	40665	75289	2.34%	0.433%
18	11.222	1392	1400	1406	rBV9	3341	7891	0.25%	0.045%
19	11.716	1482	1484	1489	rVB5	3046	4069	0.13%	0.023%
20	13.216	1735	1739	1743	rVB5	3975	7376	0.23%	0.042%
21	13.734	1821	1827	1835	rBV	153146	223390	6.95%	1.286%
22	14.010	1869	1874	1881	rBV	154874	233912	7.28%	1.347%
23	14.322	1920	1927	1942	rBV	1485107	2282224	71.02%	13.141%
24	14.545	1958	1965	1972	rBV2	71537	165338	5.15%	0.952%
25	15.316	2089	2096	2107	rBV	256119	376763	11.72%	2.169%
26	15.434	2112	2116	2128	rVB3	21987	38755	1.21%	0.223%
27	15.986	2207	2210	2215	rBV6	2094	4742	0.15%	0.027%
28	16.098	2227	2229	2234	rVB6	2454	3366	0.10%	0.019%
29	16.475	2289	2293	2297	rBV6	7533	10251	0.32%	0.059%
30	16.551	2301	2306	2308	rBV4	3860	5446	0.17%	0.031%
31	16.863	2356	2359	2364	rVB6	3069	5714	0.18%	0.033%
32	16.998	2379	2382	2386	rVB3	12721	13783	0.43%	0.079%
33	17.069	2387	2394	2405	rBV	2029406	2939768	91.48%	16.927%
34	17.169	2405	2411	2421	rVB	285221	435451	13.55%	2.507%
35	17.316	2434	2436	2440	rBV5	3322	4187	0.13%	0.024%
36	17.439	2452	2457	2459	rBV4	9523	14904	0.46%	0.086%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030813.D
Acq On : 10 Apr 2024 12:27
Operator : MA/JU
Sample : P1948-16DL 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	17.745	2506	2509	2512	rBV4	7826	10565	0.33%	0.061%
38	17.839	2522	2525	2531	rBV8	9978	18797	0.58%	0.108%
39	17.969	2542	2547	2554	rBV	58679	91776	2.86%	0.528%
40	18.404	2619	2621	2624	rVB3	9465	8026	0.25%	0.046%
41	19.469	2797	2802	2809	rBV	423943	578848	18.01%	3.333%
42	21.304	3109	3114	3124	rBV2	2329551	3213559	100.00%	18.503%
43	22.857	3374	3378	3385	rVB	96210	164673	5.12%	0.948%
44	24.033	3573	3578	3588	rVB2	162945	378053	11.76%	2.177%
45	24.239	3604	3613	3626	rBV	1259384	3123441	97.20%	17.984%




Sum of corrected areas: 17367709

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030813.D
Acq On : 10 Apr 2024 12:27
Operator : MA/JU
Sample : P1948-16DL 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

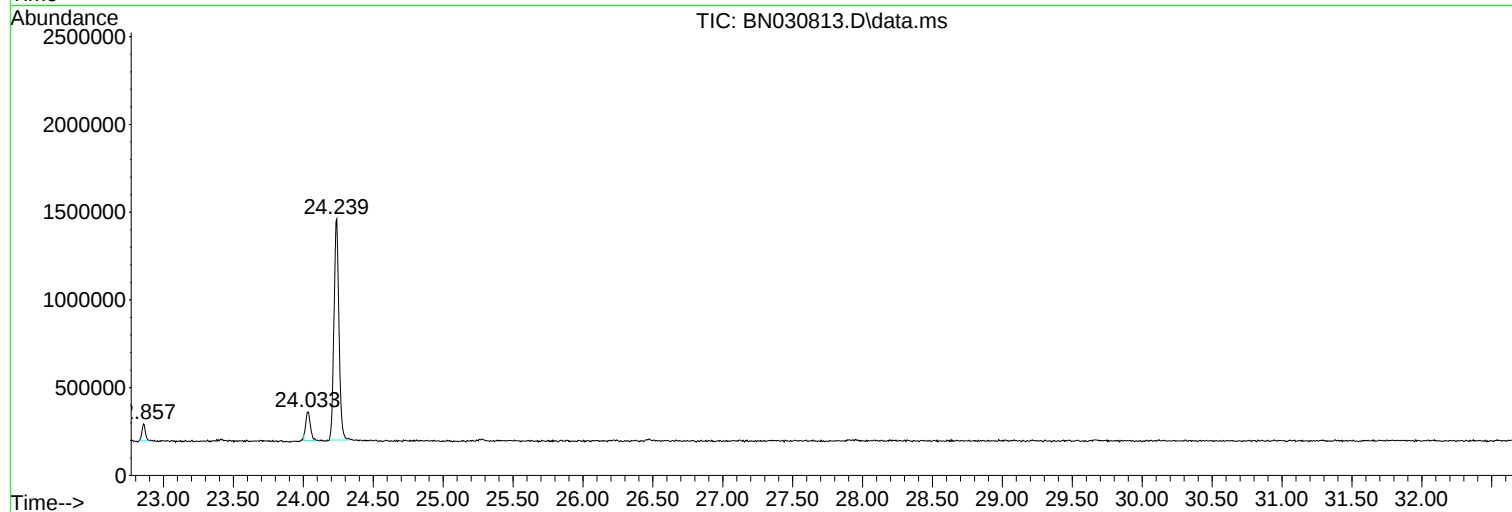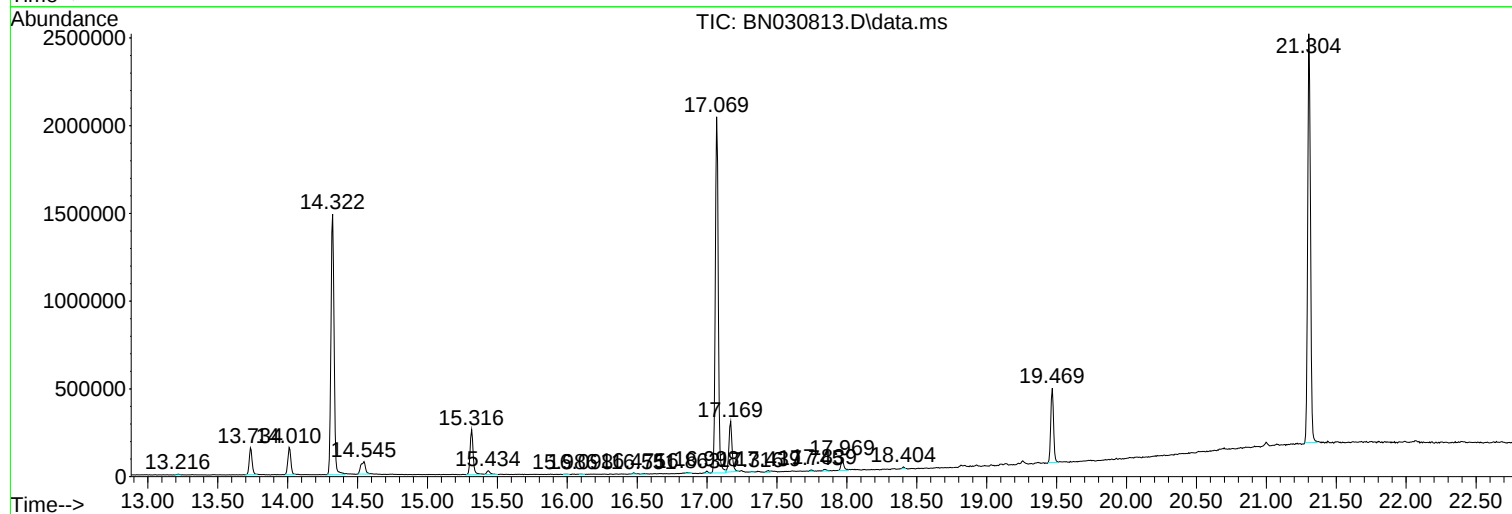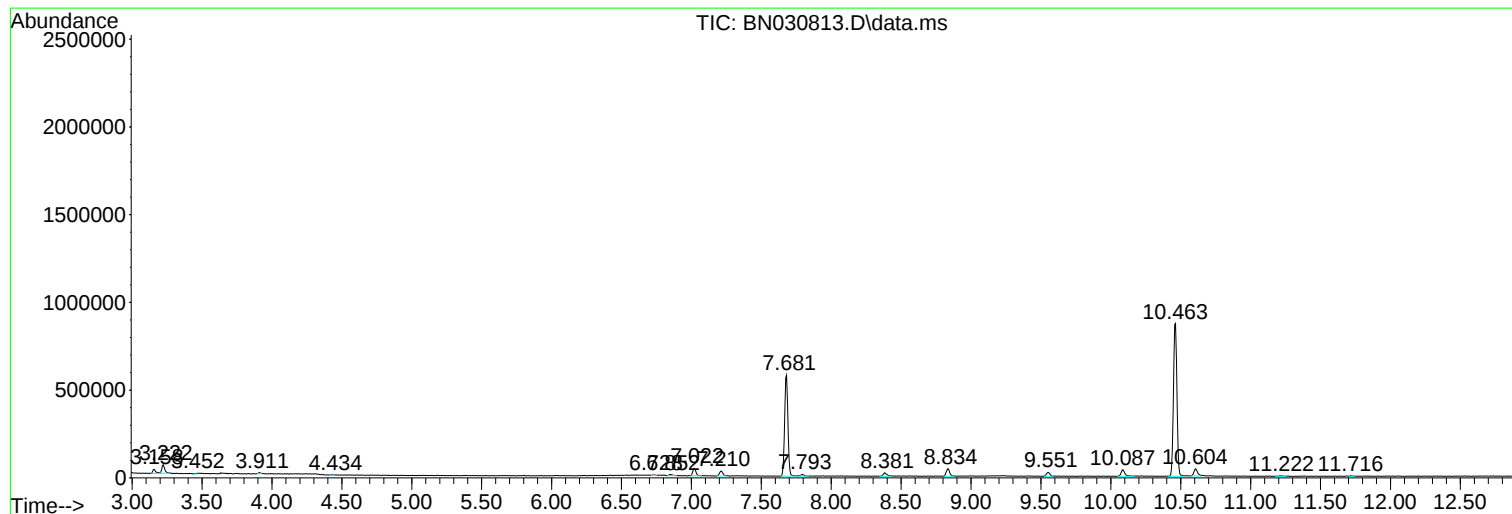

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030813.D
Acq On : 10 Apr 2024 12:27
Operator : MA/JU
Sample : P1948-16DL 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030813.D
Acq On : 10 Apr 2024 12:27
Operator : MA/JU
Sample : P1948-16DL 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc