

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030814.D
 Acq On : 10 Apr 2024 13:07
 Operator : MA/JU
 Sample : P1948-15DL 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030814.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	25	29	36	rBV3	26199	46054	1.46%	0.259%
2	3.222	36	40	48	rVB	59817	85850	2.71%	0.483%
3	3.622	106	108	110	rBV	12331	12957	0.41%	0.073%
4	3.911	153	157	162	rBV4	8331	13093	0.41%	0.074%
5	6.852	653	657	662	rVB3	7950	11922	0.38%	0.067%
6	7.022	679	686	693	rBV	50948	83603	2.64%	0.471%
7	7.210	711	718	726	rBV3	37119	65978	2.09%	0.371%
8	7.675	790	797	807	rBV	594377	963780	30.47%	5.427%
9	7.793	814	817	821	rVB5	4408	5670	0.18%	0.032%
10	8.381	910	917	926	rBV2	26878	49147	1.55%	0.277%
11	8.834	987	994	1003	rBV	50062	91058	2.88%	0.513%
12	9.551	1110	1116	1122	rBV	31254	53267	1.68%	0.300%
13	10.087	1201	1207	1216	rBV	51051	95690	3.03%	0.539%
14	10.457	1263	1270	1283	rBV	902053	1546173	48.89%	8.706%
15	10.604	1289	1295	1303	rBV	53760	105104	3.32%	0.592%
16	11.722	1482	1485	1489	rVB4	2389	3716	0.12%	0.021%
17	13.216	1735	1739	1745	rBV4	8324	11822	0.37%	0.067%
18	13.734	1821	1827	1836	rBV	176622	252082	7.97%	1.419%
19	14.010	1869	1874	1882	rBV	174808	263829	8.34%	1.486%
20	14.322	1920	1927	1944	rBV	1559983	2336031	73.87%	13.153%
21	15.316	2090	2096	2107	rVV	280273	422142	13.35%	2.377%
22	15.386	2107	2108	2112	rVV3	5163	5250	0.17%	0.030%
23	15.433	2112	2116	2124	rVB4	30510	50067	1.58%	0.282%
24	15.557	2134	2137	2140	rBV5	2407	3717	0.12%	0.021%
25	15.733	2161	2167	2172	rVB9	2496	5401	0.17%	0.030%
26	16.857	2351	2358	2362	rVB5	4940	10097	0.32%	0.057%
27	17.069	2388	2394	2405	rBV	2041096	2938736	92.92%	16.547%
28	17.169	2405	2411	2425	rVB	315382	491475	15.54%	2.767%
29	17.433	2451	2456	2471	rBV	92141	161249	5.10%	0.908%
30	17.563	2473	2478	2485	rVB9	4086	9976	0.32%	0.056%
31	17.704	2499	2502	2503	rBV2	4612	3623	0.11%	0.020%
32	17.739	2505	2508	2513	rVB6	7289	8979	0.28%	0.051%
33	17.851	2525	2527	2530	rBV4	3665	3926	0.12%	0.022%
34	17.963	2542	2546	2553	rBV3	22916	35224	1.11%	0.198%
35	18.051	2557	2561	2566	rBV7	6855	11735	0.37%	0.066%
36	18.722	2670	2675	2681	rBV6	11581	22996	0.73%	0.129%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030814.D
Acq On : 10 Apr 2024 13:07
Operator : MA/JU
Sample : P1948-15DL 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ4DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	19.257	2762	2766	2771	rBV7	20175	28144	0.89%	0.158%
38	19.351	2777	2782	2791	rBV	91477	160143	5.06%	0.902%
39	19.469	2796	2802	2813	rVV	468427	630136	19.92%	3.548%
40	20.845	3034	3036	3042	rBV4	31754	50164	1.59%	0.282%
41	21.304	3109	3114	3126	rBV2	2223499	3162558	100.00%	17.807%
42	24.033	3572	3578	3587	rVB2	182859	417715	13.21%	2.352%
43	24.239	3604	3613	3627	rBV2	1189725	3029723	95.80%	17.059%




Sum of corrected areas: 17760002

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030814.D
Acq On : 10 Apr 2024 13:07
Operator : MA/JU
Sample : P1948-15DL 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

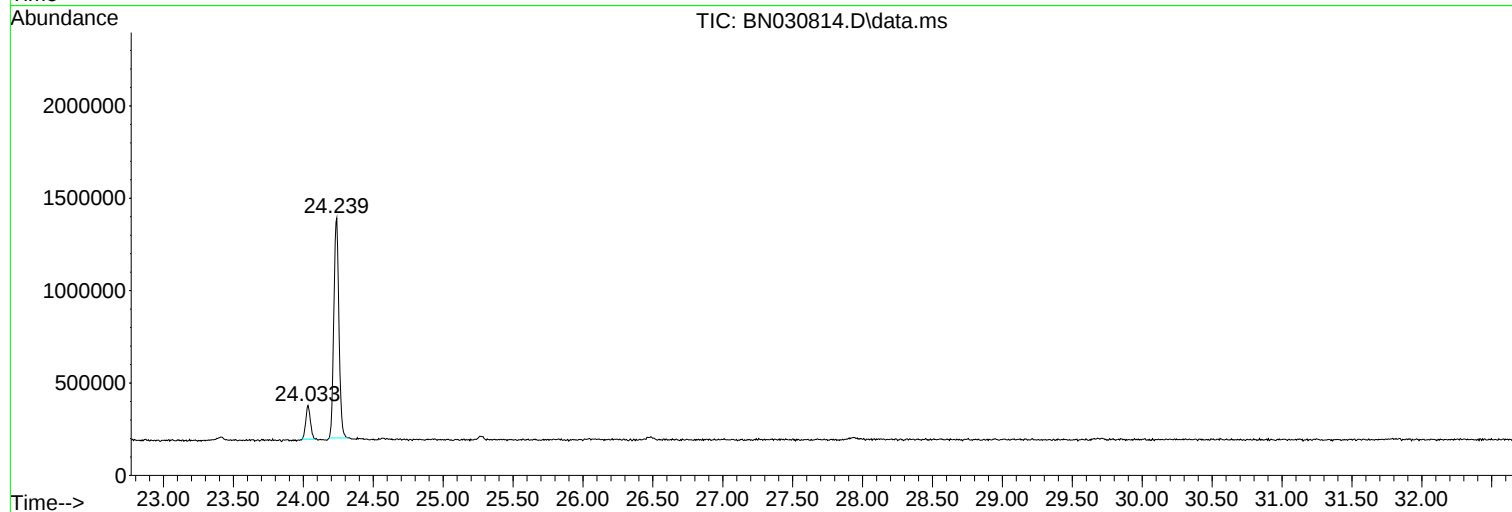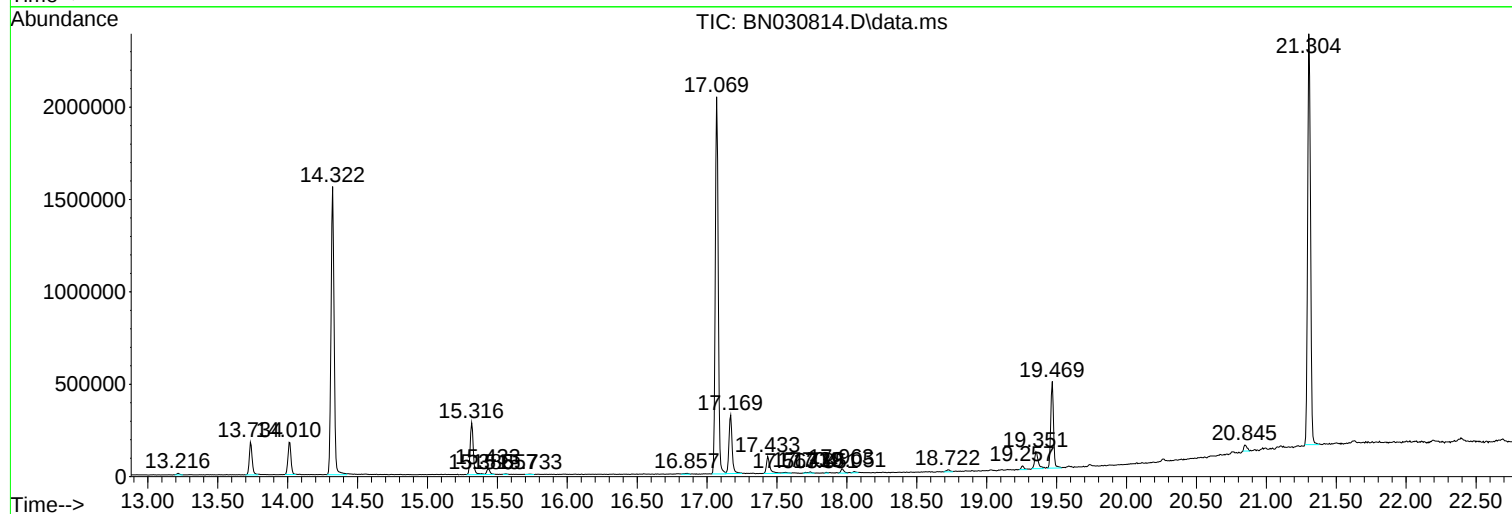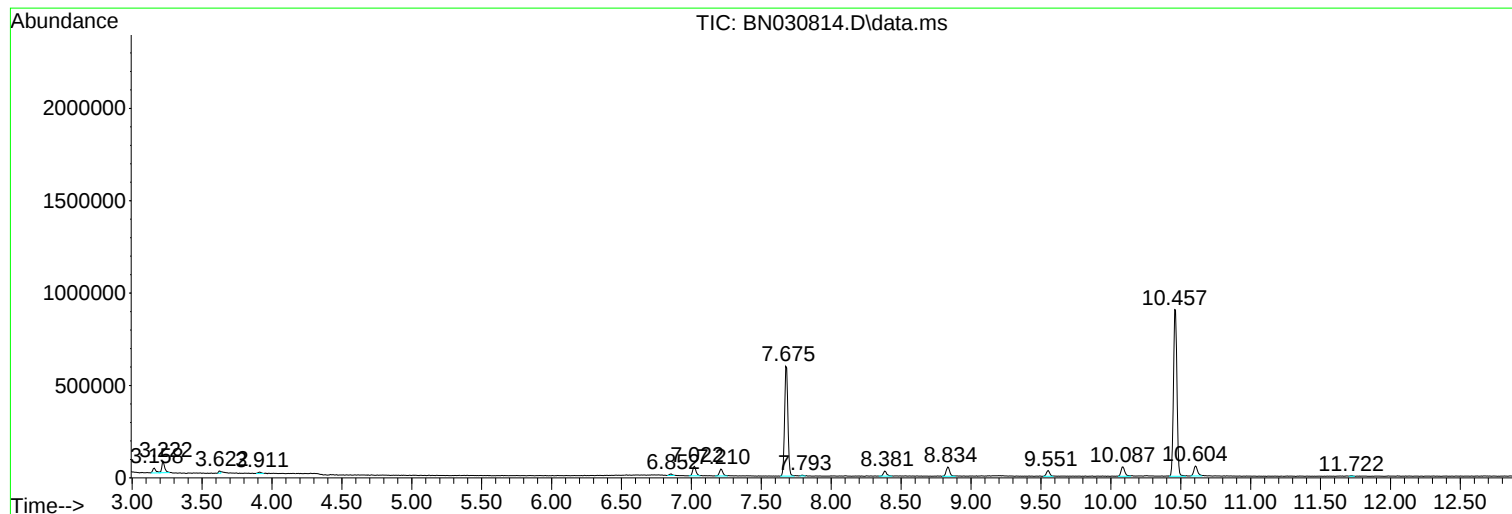

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030814.D
Acq On : 10 Apr 2024 13:07
Operator : MA/JU
Sample : P1948-15DL 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030814.D
Acq On : 10 Apr 2024 13:07
Operator : MA/JU
Sample : P1948-15DL 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc