

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030827.D
 Acq On : 10 Apr 2024 22:28
 Operator : MA/JU
 Sample : P2006-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MCORH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030827.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	48	rVB	31120	49134	0.66%	0.082%
2	3.593	100	103	119	rBV	225904	402077	5.37%	0.675%
3	3.911	153	157	162	rBV2	6903	9554	0.13%	0.016%
4	5.017	338	345	355	rBV	242860	392874	5.25%	0.660%
5	6.852	651	657	665	rVB	175084	277642	3.71%	0.466%
6	7.016	678	685	696	rBV	747638	1175021	15.70%	1.972%
7	7.211	711	718	729	rBV	692520	1090053	14.56%	1.830%
8	7.563	773	778	785	rVB2	22134	36931	0.49%	0.062%
9	7.675	789	797	801	rBV	535832	869537	11.62%	1.460%
10	7.710	801	803	813	rVB	155844	216327	2.89%	0.363%
11	8.022	849	856	864	rBV	127431	211177	2.82%	0.354%
12	8.381	910	917	926	rBV	592332	930473	12.43%	1.562%
13	8.834	986	994	1007	rBV	918434	1485444	19.85%	2.494%
14	9.057	1028	1032	1038	rVB3	7957	12218	0.16%	0.021%
15	9.240	1058	1063	1068	rVB8	5326	8688	0.12%	0.015%
16	9.552	1108	1116	1132	rBV	696497	1164372	15.56%	1.955%
17	10.081	1199	1206	1222	rBV	1115257	1863982	24.91%	3.129%
18	10.322	1241	1247	1254	rVB	47031	75771	1.01%	0.127%
19	10.457	1263	1270	1280	rBV	819253	1379990	18.44%	2.317%
20	10.599	1287	1294	1307	rBV	931916	1619613	21.64%	2.719%
21	10.840	1330	1335	1339	rVB3	13130	19768	0.26%	0.033%
22	11.722	1477	1485	1490	rVB6	5001	10397	0.14%	0.017%
23	12.051	1536	1541	1548	rVB2	21448	33400	0.45%	0.056%
24	13.216	1733	1739	1744	rBV2	21474	33737	0.45%	0.057%
25	13.734	1821	1827	1839	rBV	2303032	3304752	44.16%	5.548%
26	14.010	1868	1874	1891	rBV	2717670	4015003	53.65%	6.740%
27	14.198	1900	1906	1910	rBV	25425	36971	0.49%	0.062%
28	14.322	1919	1927	1937	rBV	1421819	2104134	28.11%	3.532%
29	14.534	1956	1963	1977	rBV	98928	237998	3.18%	0.400%
30	14.634	1977	1980	1983	rVB3	12770	16410	0.22%	0.028%
31	15.316	2089	2096	2110	rBV	3532601	5143845	68.73%	8.635%
32	15.434	2110	2116	2131	rVV	984868	1384936	18.50%	2.325%
33	15.557	2132	2137	2142	rVB3	18559	30095	0.40%	0.051%
34	16.104	2225	2230	2234	rBV3	13104	18037	0.24%	0.030%
35	16.751	2336	2340	2344	rVB4	5416	8020	0.11%	0.013%
36	16.851	2355	2357	2365	rVB4	4383	7497	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030827.D
Acq On : 10 Apr 2024 22:28
Operator : MA/JU
Sample : P2006-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MCORH4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	17.069	2387	2394	2404	rBV	1901110	2652650	35.44%	4.453%
38	17.169	2404	2411	2425	rVV	4204971	6027744	80.54%	10.119%
39	17.745	2506	2509	2514	rVB6	8801	9980	0.13%	0.017%
40	17.969	2543	2547	2552	rBV5	17806	23964	0.32%	0.040%
41	19.028	2722	2727	2734	rBV	58759	85819	1.15%	0.144%
42	19.104	2735	2740	2744	rBV	48928	69223	0.92%	0.116%
43	19.257	2762	2766	2770	rBV5	18373	26344	0.35%	0.044%
44	19.469	2796	2802	2812	rBV	5395489	7439434	99.40%	12.488%
45	21.304	3108	3114	3122	rBV	2129385	3035626	40.56%	5.096%
46	24.039	3569	3579	3596	rBV2	3073282	7484342	100.00%	12.564%
47	24.239	3604	3613	3624	rVB	1229492	3039790	40.62%	5.103%




Sum of corrected areas: 59570794

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030827.D
Acq On : 10 Apr 2024 22:28
Operator : MA/JU
Sample : P2006-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MCORH4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

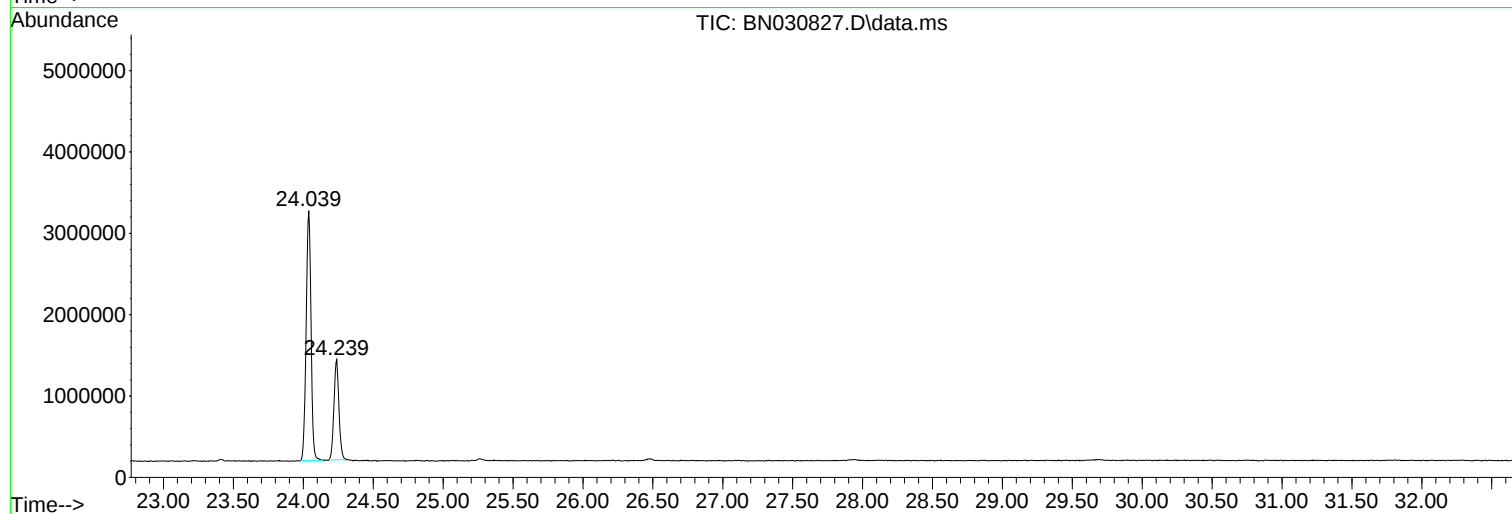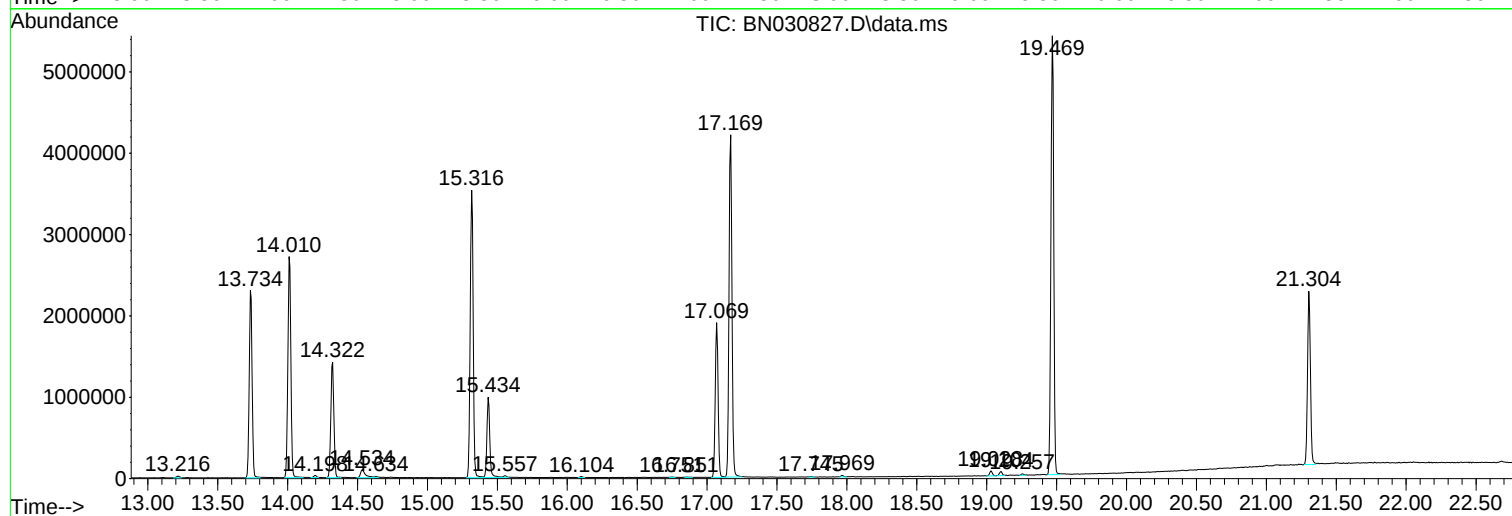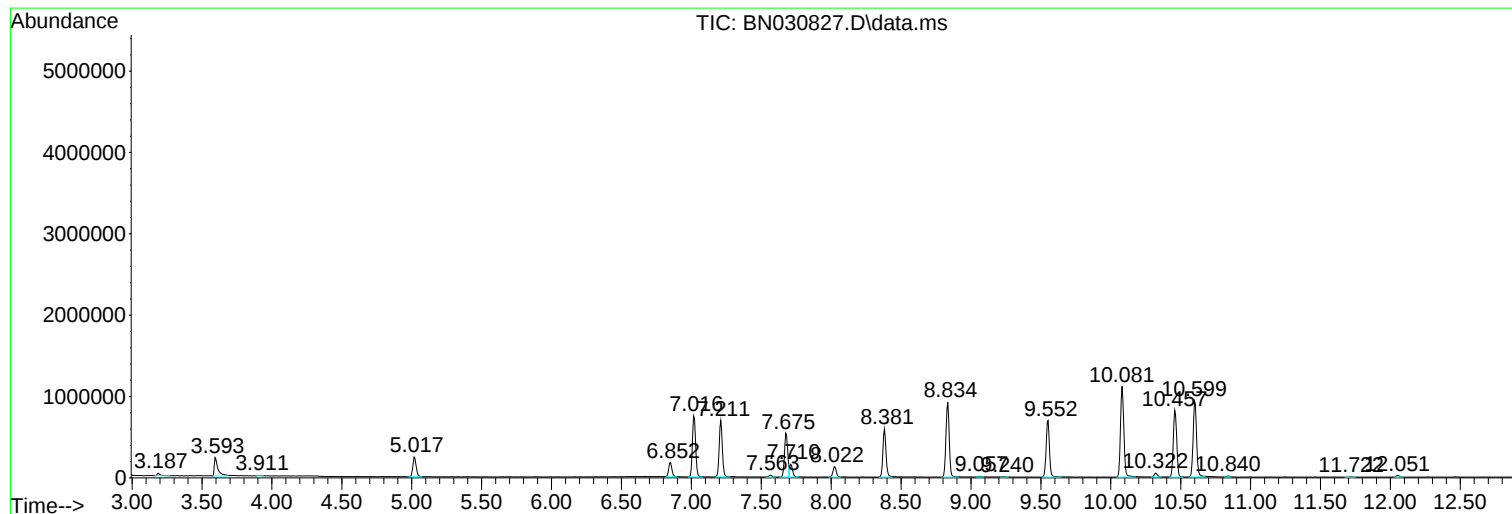

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030827.D
Acq On : 10 Apr 2024 22:28
Operator : MA/JU
Sample : P2006-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0RH4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030827.D
Acq On : 10 Apr 2024 22:28
Operator : MA/JU
Sample : P2006-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0RH4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc