

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030830.D
 Acq On : 11 Apr 2024 00:26
 Operator : MA/JU
 Sample : P2014-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0MC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030830.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	42	rVB	27845	41340	0.55%	0.069%
2	3.593	101	103	127	rBV	178223	327111	4.36%	0.545%
3	3.911	154	157	162	rVB2	7890	11962	0.16%	0.020%
4	6.852	651	657	667	rBV	175440	289169	3.85%	0.482%
5	7.016	679	685	695	rBV	687835	1073974	14.31%	1.790%
6	7.210	711	718	729	rBV	655303	1013006	13.49%	1.689%
7	7.675	790	797	805	rBV	619148	996381	13.27%	1.661%
8	8.381	909	917	931	rBV	572052	912916	12.16%	1.522%
9	8.834	987	994	1006	rBV	832864	1372764	18.29%	2.288%
10	9.234	1057	1062	1068	rVB2	17139	27196	0.36%	0.045%
11	9.398	1086	1090	1094	rBV2	11234	15500	0.21%	0.026%
12	9.546	1107	1115	1130	rBV	619151	1052541	14.02%	1.755%
13	10.081	1199	1206	1222	rBV	1034509	1716816	22.87%	2.862%
14	10.246	1229	1234	1241	rVB3	15180	25484	0.34%	0.042%
15	10.457	1263	1270	1279	rBV	934285	1611608	21.47%	2.686%
16	10.598	1286	1294	1309	rBV	975376	1707642	22.75%	2.847%
17	11.204	1391	1397	1404	rBV3	7680	18817	0.25%	0.031%
18	11.728	1482	1486	1490	rVB5	4484	7508	0.10%	0.013%
19	12.051	1536	1541	1546	rVB2	19337	28912	0.39%	0.048%
20	13.145	1722	1727	1733	rVB5	9160	14600	0.19%	0.024%
21	13.216	1733	1739	1746	rBV2	17965	29447	0.39%	0.049%
22	13.734	1820	1827	1840	rBV	2288531	3162091	42.12%	5.271%
23	14.010	1865	1874	1894	rBV	2483534	3764883	50.15%	6.276%
24	14.228	1907	1911	1918	rVB7	4691	8169	0.11%	0.014%
25	14.316	1918	1926	1942	rBV	1599542	2416628	32.19%	4.028%
26	14.534	1957	1963	1976	rBV	126925	276312	3.68%	0.461%
27	14.739	1995	1998	2003	rVB7	5944	10593	0.14%	0.018%
28	14.986	2034	2040	2042	rBV6	4678	7862	0.10%	0.013%
29	15.122	2059	2063	2066	rBV4	4793	8069	0.11%	0.013%
30	15.316	2088	2096	2109	rBV	3404807	4936430	65.76%	8.229%
31	15.433	2109	2116	2131	rVV	979590	1357185	18.08%	2.262%
32	15.557	2133	2137	2141	rVB2	15757	26037	0.35%	0.043%
33	16.104	2225	2230	2236	rVB5	13912	20540	0.27%	0.034%
34	16.545	2301	2305	2308	rBV5	4568	8956	0.12%	0.015%
35	16.745	2336	2339	2344	rVB6	6647	9970	0.13%	0.017%
36	16.839	2351	2355	2356	rBV3	6691	7537	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030830.D
 Acq On : 11 Apr 2024 00:26
 Operator : MA/JU
 Sample : P2014-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0MC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	16.998	2377	2382	2385	rBV4	19053	23040	0.31%	0.038%
38	17.069	2385	2394	2404	rBV	2108141	3046399	40.58%	5.078%
39	17.169	2404	2411	2431	rVB2	4020265	5860388	78.06%	9.769%
40	17.363	2440	2444	2447	rBV	6555	7863	0.10%	0.013%
41	17.745	2505	2509	2514	rVB5	13819	17436	0.23%	0.029%
42	17.839	2521	2525	2529	rBV7	5923	9138	0.12%	0.015%
43	17.969	2542	2547	2555	rBV	84532	131065	1.75%	0.218%
44	18.298	2600	2603	2610	rVB8	9087	19053	0.25%	0.032%
45	18.404	2617	2621	2623	rBV5	9090	10898	0.15%	0.018%
46	18.451	2626	2629	2632	rBV4	6424	9044	0.12%	0.015%
47	18.845	2692	2696	2703	rVB8	9432	16710	0.22%	0.028%
48	19.027	2723	2727	2733	rBV2	61845	87824	1.17%	0.146%
49	19.098	2735	2739	2743	rBV	52410	74724	1.00%	0.125%
50	19.257	2762	2766	2771	rBV2	56693	81310	1.08%	0.136%
51	19.469	2796	2802	2810	rBV	5350303	7179844	95.64%	11.969%
52	20.998	3058	3062	3070	rBV5	71788	127148	1.69%	0.212%
53	21.304	3108	3114	3127	rBV	2408728	3545022	47.22%	5.909%
54	22.857	3375	3378	3384	rVB	82497	123379	1.64%	0.206%
55	24.039	3569	3579	3595	rBV	3044009	7507268	100.00%	12.514%
56	24.233	3604	3612	3626	rVB2	1507371	3795861	50.56%	6.328%




Sum of corrected areas: 59989370

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030830.D
Acq On : 11 Apr 2024 00:26
Operator : MA/JU
Sample : P2014-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

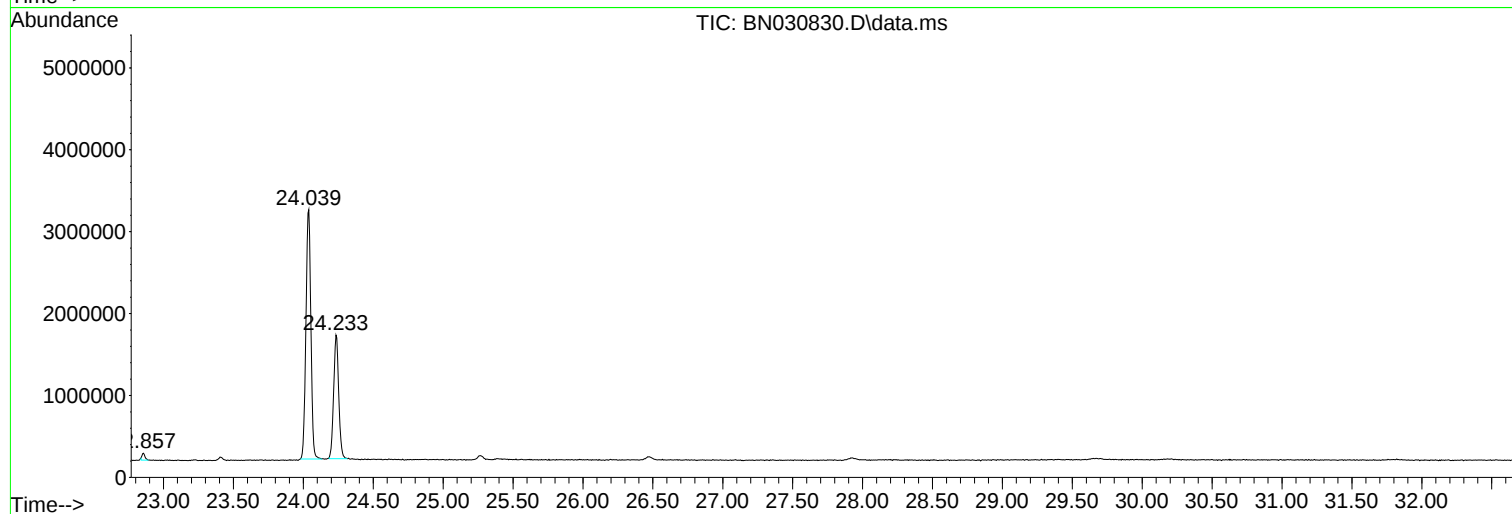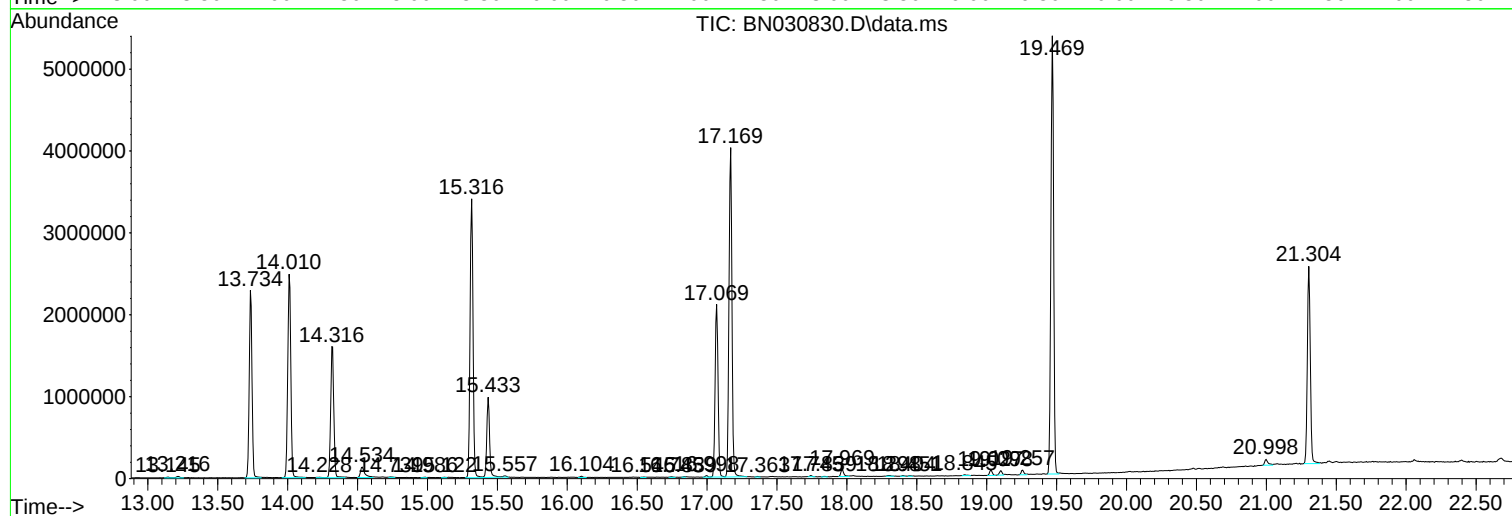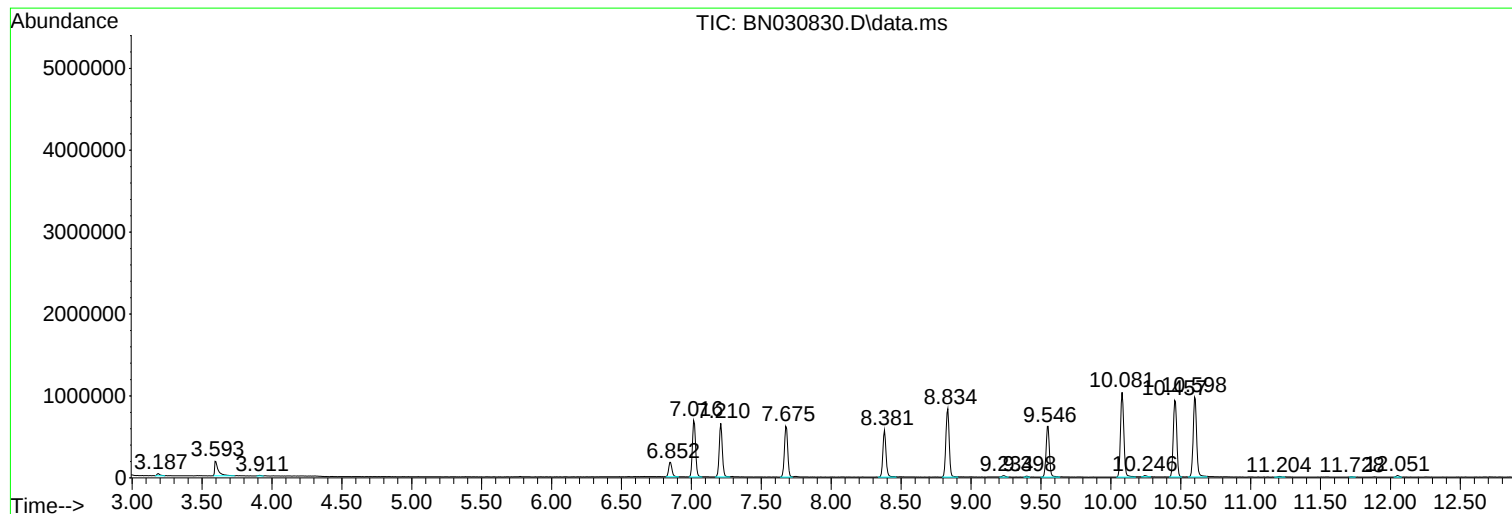

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030830.D
Acq On : 11 Apr 2024 00:26
Operator : MA/JU
Sample : P2014-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030830.D
Acq On : 11 Apr 2024 00:26
Operator : MA/JU
Sample : P2014-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc