

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030832.D
 Acq On : 11 Apr 2024 01:45
 Operator : MA/JU
 Sample : P2014-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EOMD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	25	29	31	rBV4	9739	14418	0.21%	0.026%
2	3.187	31	34	38	rVB	24986	31311	0.45%	0.055%
3	3.593	100	103	120	rBV	213913	385110	5.52%	0.681%
4	3.911	153	157	160	rBV3	6540	8490	0.12%	0.015%
5	4.428	239	245	259	rVB	60469	106896	1.53%	0.189%
6	6.846	651	656	668	rVB	175078	286010	4.10%	0.506%
7	7.016	678	685	694	rBV	673648	1051994	15.08%	1.861%
8	7.210	711	718	729	rBV	631352	999257	14.32%	1.768%
9	7.675	788	797	806	rBV	591934	929468	13.32%	1.644%
10	8.381	910	917	928	rBV	557320	881358	12.63%	1.559%
11	8.834	984	994	1005	rBV	812393	1337035	19.16%	2.366%
12	9.234	1057	1062	1066	rBV3	7787	11541	0.17%	0.020%
13	9.546	1109	1115	1127	rBV	620163	1015125	14.55%	1.796%
14	10.081	1199	1206	1220	rBV	991701	1656516	23.74%	2.931%
15	10.457	1263	1270	1280	rBV	899697	1487950	21.32%	2.633%
16	10.599	1285	1294	1310	rBV	958104	1682903	24.12%	2.978%
17	12.051	1536	1541	1547	rVB3	19250	31134	0.45%	0.055%
18	13.216	1734	1739	1745	rVV2	21060	30754	0.44%	0.054%
19	13.734	1820	1827	1838	rBV	2082339	2967144	42.52%	5.250%
20	14.010	1867	1874	1892	rBV2	2493661	3658662	52.43%	6.473%
21	14.316	1920	1926	1935	rBV	1445150	2192828	31.42%	3.880%
22	14.416	1940	1943	1949	rVB7	5226	7755	0.11%	0.014%
23	14.534	1956	1963	1975	rBV	105670	244046	3.50%	0.432%
24	14.681	1986	1988	1994	rVB6	4507	7168	0.10%	0.013%
25	14.751	1994	2000	2005	rBV9	8374	15416	0.22%	0.027%
26	15.122	2058	2063	2067	rBV5	4634	10412	0.15%	0.018%
27	15.316	2089	2096	2109	rBV	3228439	4794483	68.71%	8.483%
28	15.434	2110	2116	2131	rVV	890600	1240082	17.77%	2.194%
29	15.551	2133	2136	2144	rVB4	16874	30296	0.43%	0.054%
30	16.104	2225	2230	2234	rBV5	12160	16213	0.23%	0.029%
31	16.269	2254	2258	2263	rBV8	4049	7342	0.11%	0.013%
32	16.745	2337	2339	2343	rVB5	5902	7218	0.10%	0.013%
33	16.998	2379	2382	2385	rVB3	11155	12075	0.17%	0.021%
34	17.069	2388	2394	2404	rVV	2016479	2829275	40.54%	5.006%
35	17.169	2404	2411	2431	rVB	3927903	5638860	80.81%	9.977%
36	17.357	2441	2443	2448	rBV3	6355	8929	0.13%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030832.D
Acq On : 11 Apr 2024 01:45
Operator : MA/JU
Sample : P2014-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	17.457	2456	2460	2468	rBV8	5337	11887	0.17%	0.021%
38	17.739	2506	2508	2513	rVB4	6592	7017	0.10%	0.012%
39	17.963	2539	2546	2552	rBV3	49805	82613	1.18%	0.146%
40	18.045	2557	2560	2563	rVB	6319	8834	0.13%	0.016%
41	18.404	2618	2621	2625	rVB5	11403	12393	0.18%	0.022%
42	19.033	2722	2728	2734	rBV	52724	73472	1.05%	0.130%
43	19.098	2735	2739	2744	rBV	46353	64350	0.92%	0.114%
44	19.257	2762	2766	2771	rBV3	28867	44342	0.64%	0.078%
45	19.469	2796	2802	2812	rBV2	4920802	6895702	98.82%	12.200%
46	21.304	3108	3114	3125	rBV	2212925	3271139	46.88%	5.788%
47	24.033	3569	3578	3593	rBV	2864366	6978322	100.00%	12.347%
48	24.233	3604	3612	3624	rVB	1389163	3434789	49.22%	6.077%




Sum of corrected areas: 56520334

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030832.D
Acq On : 11 Apr 2024 01:45
Operator : MA/JU
Sample : P2014-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

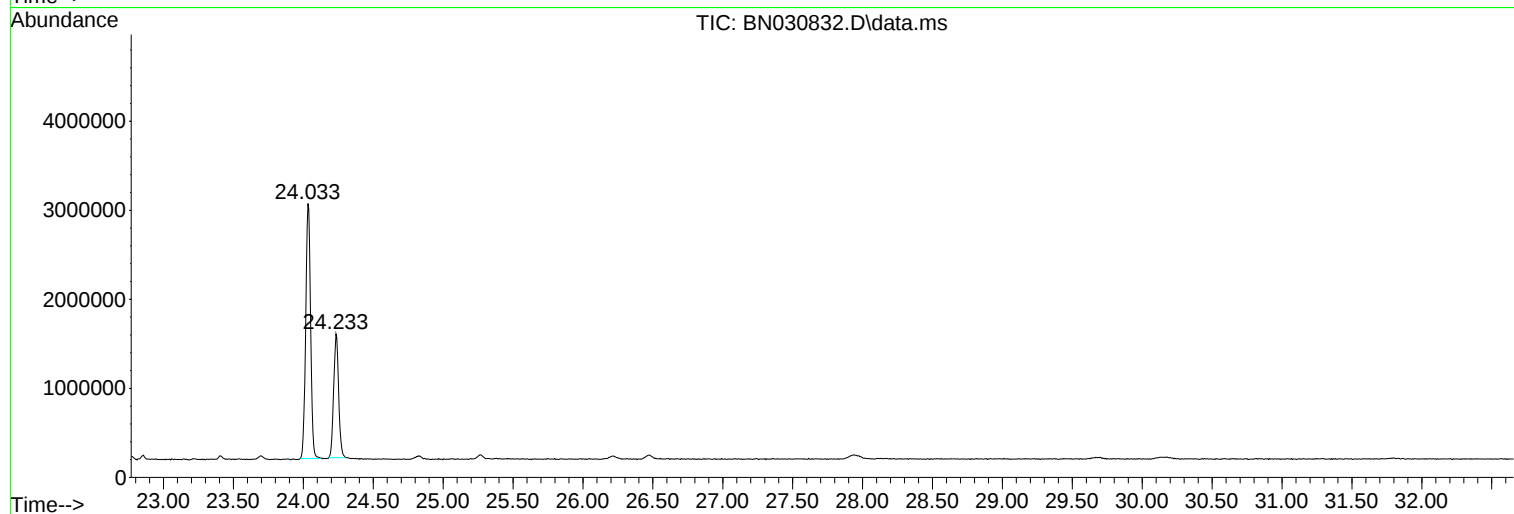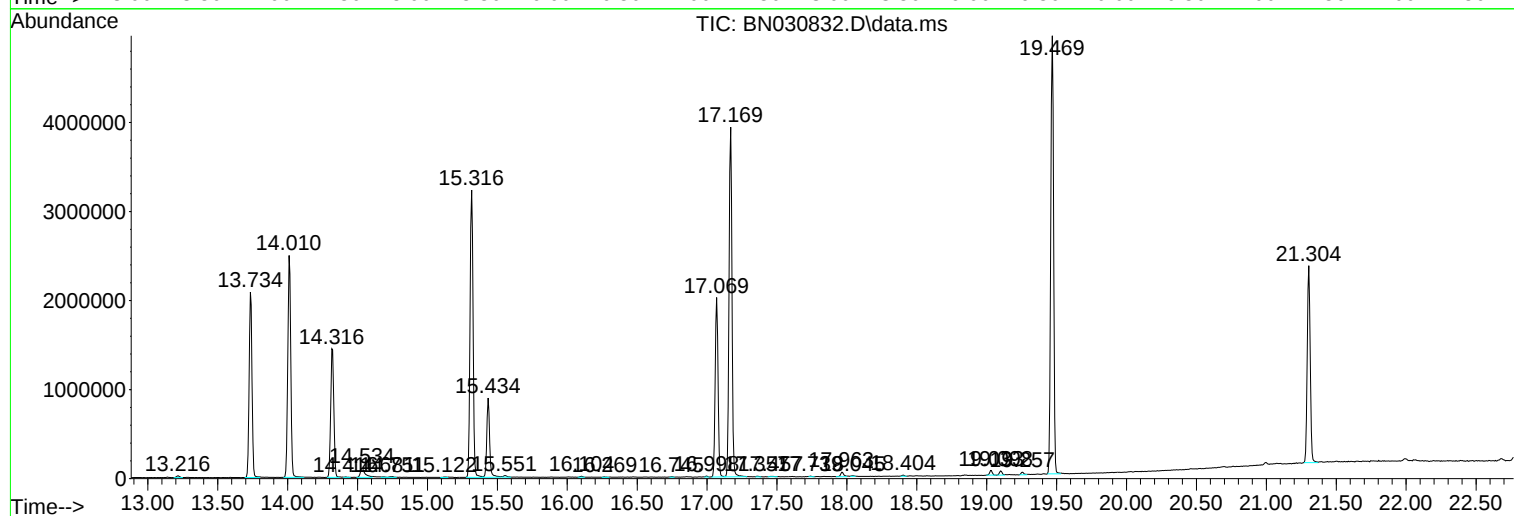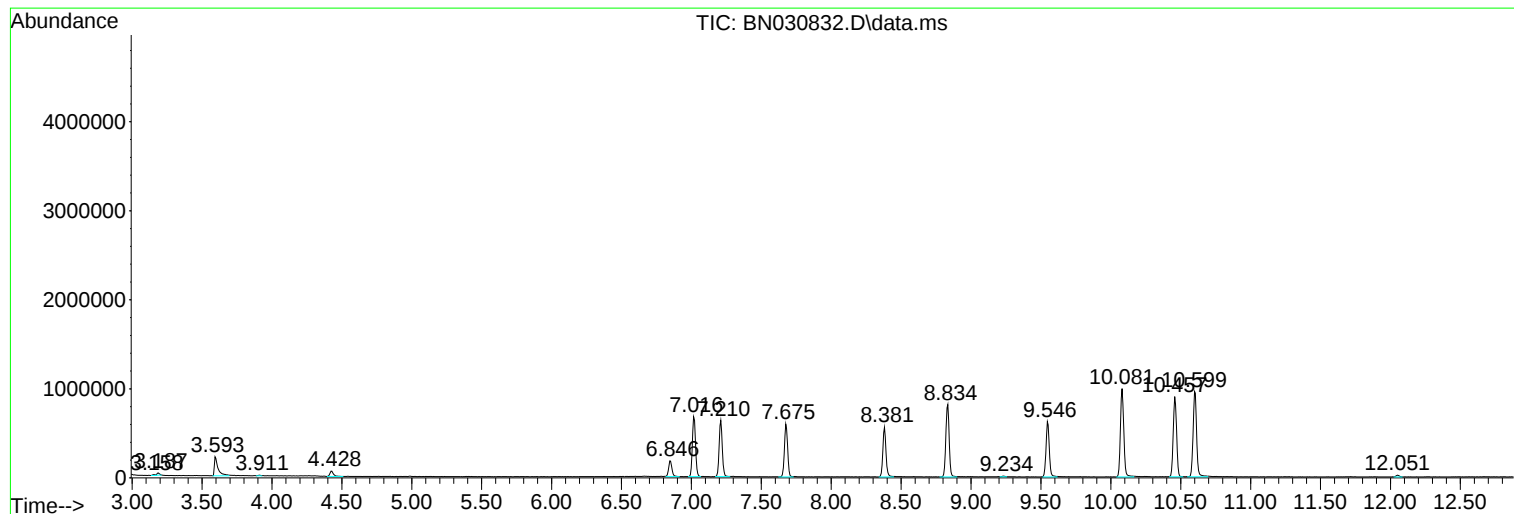

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030832.D
Acq On : 11 Apr 2024 01:45
Operator : MA/JU
Sample : P2014-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030832.D
Acq On : 11 Apr 2024 01:45
Operator : MA/JU
Sample : P2014-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc