

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030833.D
 Acq On : 11 Apr 2024 02:24
 Operator : MA/JU
 Sample : P2035-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030833.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	24	28	32	rBV	119870	177863	2.30%	0.288%
2	3.475	79	83	89	rVB5	6414	10689	0.14%	0.017%
3	3.599	101	104	120	rBV	199708	340992	4.41%	0.551%
4	3.911	155	157	164	rVB2	10241	14552	0.19%	0.024%
5	4.422	240	244	249	rBV5	10946	16487	0.21%	0.027%
6	6.852	651	657	667	rVB	164266	269036	3.48%	0.435%
7	7.016	679	685	698	rVB	744307	1172635	15.18%	1.896%
8	7.211	711	718	728	rBV	681973	1069801	13.85%	1.730%
9	7.299	728	733	738	rVB8	4613	8419	0.11%	0.014%
10	7.675	787	797	805	rBV	646887	1015043	13.14%	1.642%
11	8.381	910	917	931	rBV	547431	875110	11.33%	1.415%
12	8.834	982	994	1008	rBV	927316	1490261	19.29%	2.410%
13	9.234	1057	1062	1067	rVB2	16607	23961	0.31%	0.039%
14	9.399	1086	1090	1097	rBV6	7272	11580	0.15%	0.019%
15	9.546	1109	1115	1124	rBV	666327	1094630	14.17%	1.770%
16	10.081	1197	1206	1225	rBV	1097386	1822960	23.60%	2.948%
17	10.457	1263	1270	1282	rVB	973863	1605250	20.78%	2.596%
18	10.599	1286	1294	1313	rBV	979324	1721926	22.29%	2.785%
19	11.204	1392	1397	1402	rBV6	5928	11872	0.15%	0.019%
20	11.722	1477	1485	1491	rVB3	5121	10064	0.13%	0.016%
21	12.051	1537	1541	1548	rVB2	21380	33575	0.43%	0.054%
22	13.216	1733	1739	1748	rBV3	24326	39097	0.51%	0.063%
23	13.734	1820	1827	1840	rBV	2311417	3216048	41.63%	5.201%
24	14.010	1865	1874	1887	rBV	2680441	4016515	51.99%	6.496%
25	14.322	1919	1927	1940	rBV	1565434	2361044	30.56%	3.818%
26	14.534	1957	1963	1980	rBV	95272	233531	3.02%	0.378%
27	15.316	2089	2096	2105	rBV	3554551	5105004	66.08%	8.256%
28	15.434	2110	2116	2131	rVV	921177	1270677	16.45%	2.055%
29	15.557	2133	2137	2141	rVB	17652	26551	0.34%	0.043%
30	16.098	2224	2229	2237	rVB4	12586	19916	0.26%	0.032%
31	17.069	2387	2394	2404	rBV	2183958	3111731	40.28%	5.032%
32	17.169	2404	2411	2426	rVV	4127206	5933967	76.81%	9.597%
33	17.745	2505	2509	2513	rVB5	17517	24444	0.32%	0.040%
34	17.969	2542	2547	2555	rBV	115854	173882	2.25%	0.281%
35	18.404	2617	2621	2625	rBV5	16653	22432	0.29%	0.036%
36	18.451	2627	2629	2633	rVB5	7854	10537	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030833.D
Acq On : 11 Apr 2024 02:24
Operator : MA/JU
Sample : P2035-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	19.028	2723	2727	2732	rVB	58946	85270	1.10%	0.138%
38	19.098	2735	2739	2744	rBV	58125	83857	1.09%	0.136%
39	19.257	2762	2766	2773	rBV3	52951	78630	1.02%	0.127%
40	19.469	2796	2802	2810	rBV	5446012	7473027	96.73%	12.086%
41	20.998	3059	3062	3072	rBV5	92764	178323	2.31%	0.288%
42	21.304	3108	3114	3124	rBV2	2555397	3787832	49.03%	6.126%
43	24.033	3569	3578	3592	rBV2	3111116	7725331	100.00%	12.494%
44	24.233	3603	3612	3628	rVB	1596117	4058695	52.54%	6.564%




Sum of corrected areas: 61833047

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030833.D
Acq On : 11 Apr 2024 02:24
Operator : MA/JU
Sample : P2035-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

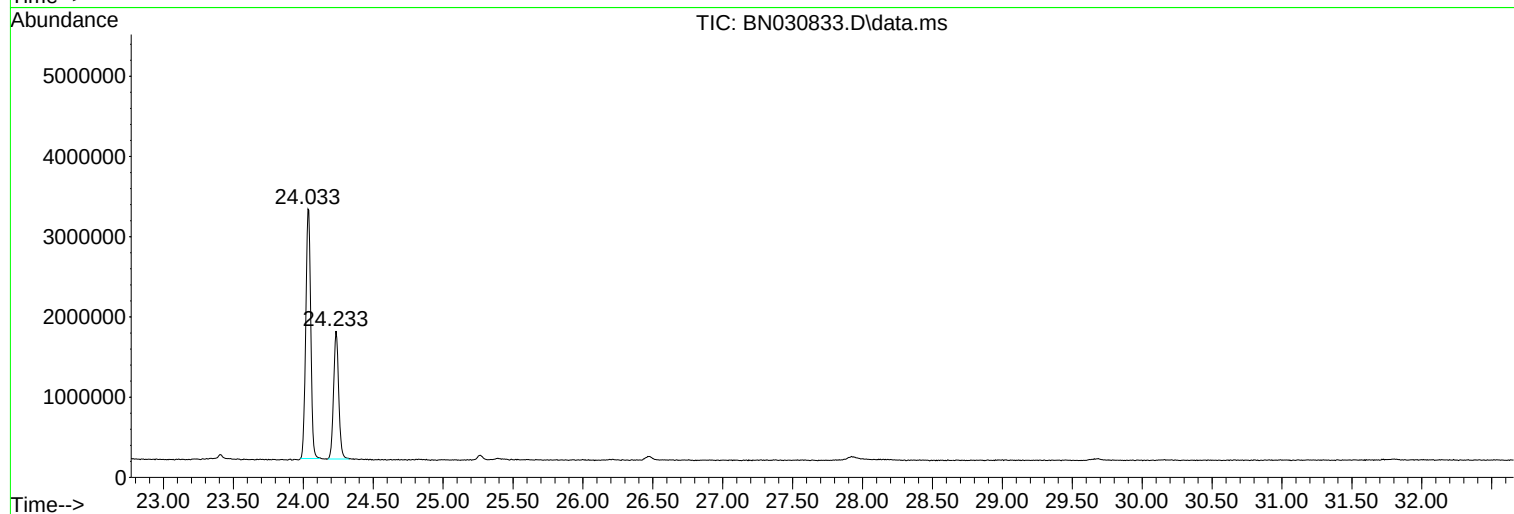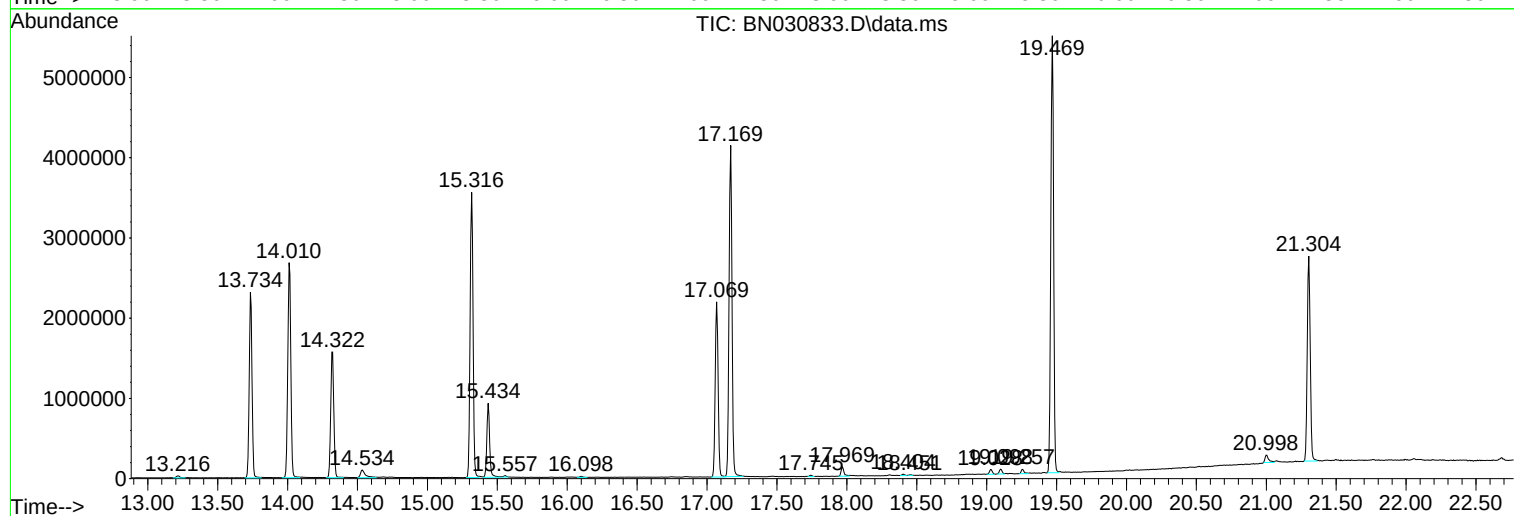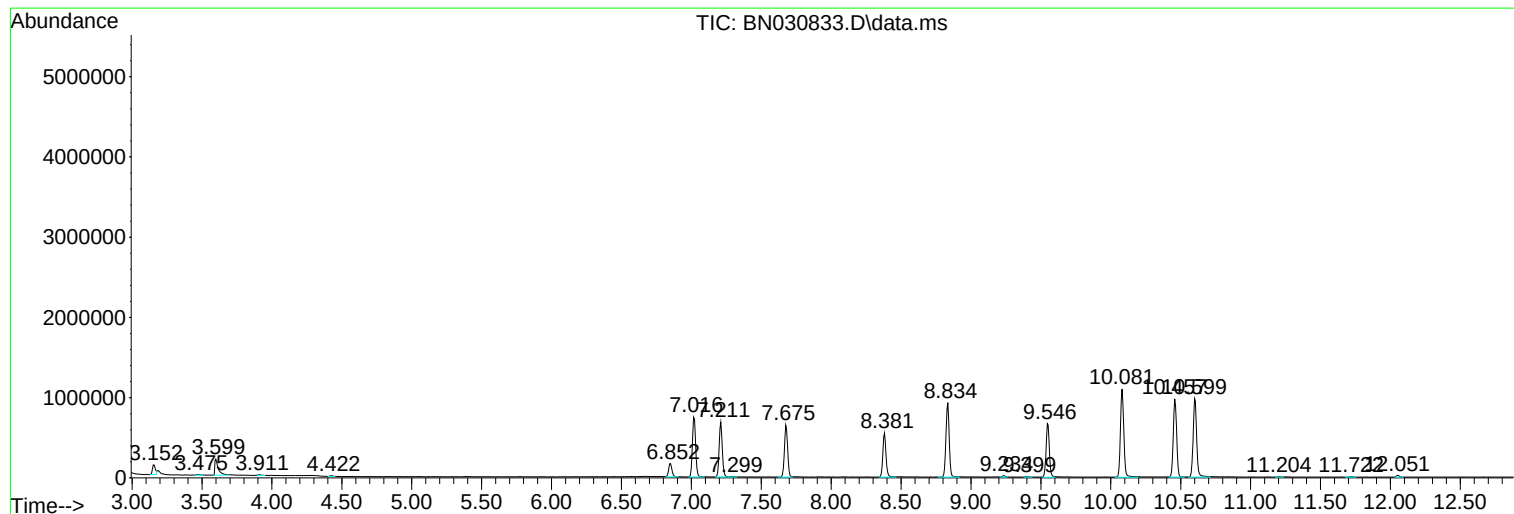

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030833.D
Acq On : 11 Apr 2024 02:24
Operator : MA/JU
Sample : P2035-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030833.D
Acq On : 11 Apr 2024 02:24
Operator : MA/JU
Sample : P2035-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
