

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030834.D
 Acq On : 11 Apr 2024 03:04
 Operator : MA/JU
 Sample : P1982-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030834.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	25	29	31	rBV5	13126	17591	0.22%	0.031%
2	3.187	31	34	38	rVB	22009	28164	0.35%	0.050%
3	3.599	102	104	116	rBV	135315	238248	2.94%	0.420%
4	3.911	155	157	163	rVB5	6469	8593	0.11%	0.015%
5	4.428	239	245	249	rBV5	13171	23369	0.29%	0.041%
6	6.852	650	657	670	rVB	156201	261758	3.23%	0.462%
7	7.017	679	685	697	rBV	651598	1025295	12.66%	1.809%
8	7.211	711	718	728	rBV	620087	972902	12.02%	1.716%
9	7.675	790	797	807	rVB	510553	811115	10.02%	1.431%
10	8.381	910	917	931	rBV	511470	822824	10.16%	1.451%
11	8.834	985	994	1006	rBV	788945	1306146	16.13%	2.304%
12	9.546	1108	1115	1130	rBV	605593	1002874	12.39%	1.769%
13	10.081	1197	1206	1227	rBV	967859	1637537	20.23%	2.889%
14	10.458	1262	1270	1281	rBV	777334	1293380	15.98%	2.282%
15	10.599	1287	1294	1310	rBV	906905	1612395	19.92%	2.844%
16	11.993	1522	1531	1536	rBV	28275	47493	0.59%	0.084%
17	12.052	1536	1541	1546	rVB2	16965	29443	0.36%	0.052%
18	13.216	1734	1739	1744	rVB5	10199	15709	0.19%	0.028%
19	13.734	1820	1827	1842	rBV	2181934	2957788	36.54%	5.218%
20	14.010	1867	1874	1887	rBV	2445794	3625190	44.78%	6.395%
21	14.322	1920	1927	1939	rBV	1302333	1950993	24.10%	3.442%
22	14.534	1957	1963	1977	rBV	100814	233919	2.89%	0.413%
23	14.734	1993	1997	2004	rVB10	5129	10855	0.13%	0.019%
24	15.316	2089	2096	2110	rBV	3218104	4720862	58.31%	8.328%
25	15.434	2110	2116	2133	rVV	901900	1273083	15.73%	2.246%
26	15.557	2133	2137	2142	rVB2	17232	29076	0.36%	0.051%
27	16.098	2225	2229	2233	rBV4	11594	15753	0.19%	0.028%
28	17.069	2387	2394	2404	rBV	1836000	2569077	31.73%	4.532%
29	17.169	2404	2411	2425	rVV	4045007	5770090	71.27%	10.179%
30	17.963	2543	2546	2554	rBV4	33573	52960	0.65%	0.093%
31	19.028	2723	2727	2734	rBV	51872	74308	0.92%	0.131%
32	19.098	2735	2739	2744	rBV2	48524	65682	0.81%	0.116%
33	19.257	2762	2766	2772	rBV3	27608	35828	0.44%	0.063%
34	19.469	2796	2802	2809	rBV	5390910	7297737	90.14%	12.873%
35	21.304	3108	3114	3124	rBV2	2319375	3229670	39.89%	5.697%
36	24.039	3569	3579	3592	rBV2	3300398	8095571	100.00%	14.281%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030834.D
Acq On : 11 Apr 2024 03:04
Operator : MA/JU
Sample : P1982-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSQ2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	24.239	3604	3613	3628	rVB	1360363	3525241	43.55%	6.219%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 56688519

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030834.D
Acq On : 11 Apr 2024 03:04
Operator : MA/JU
Sample : P1982-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

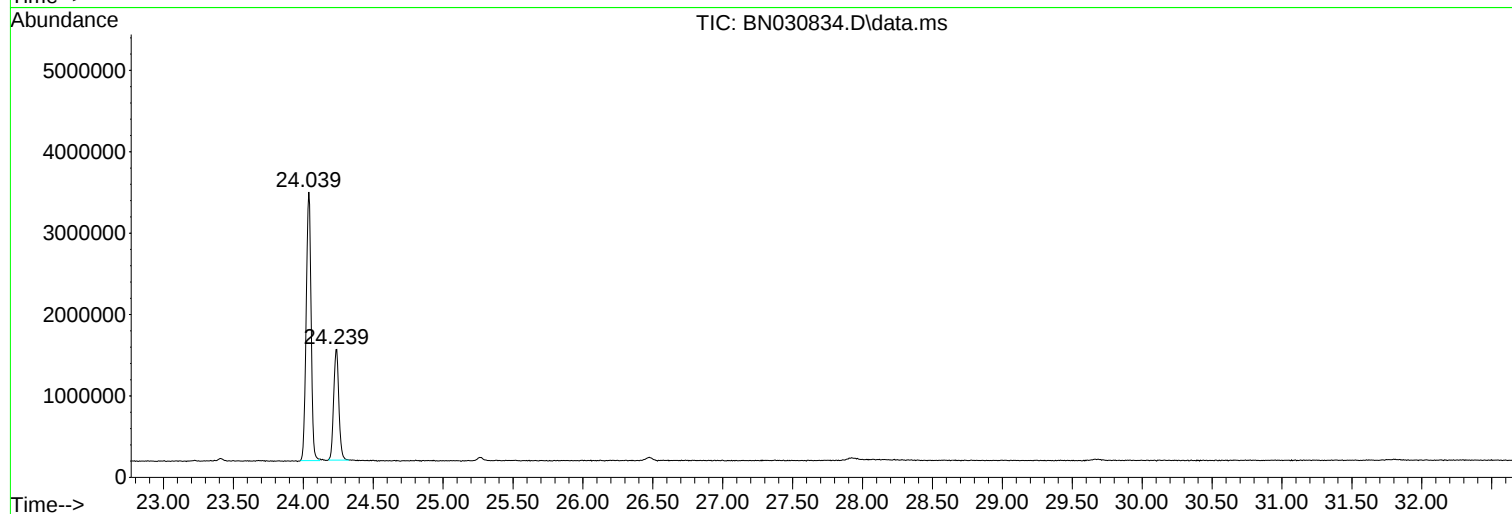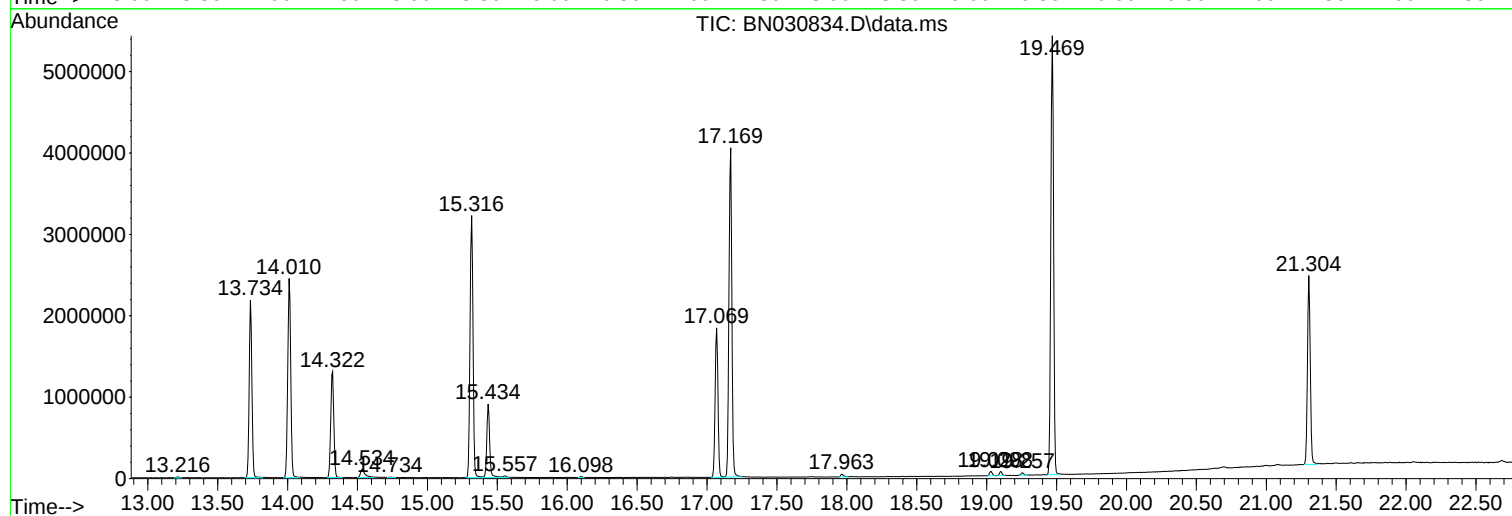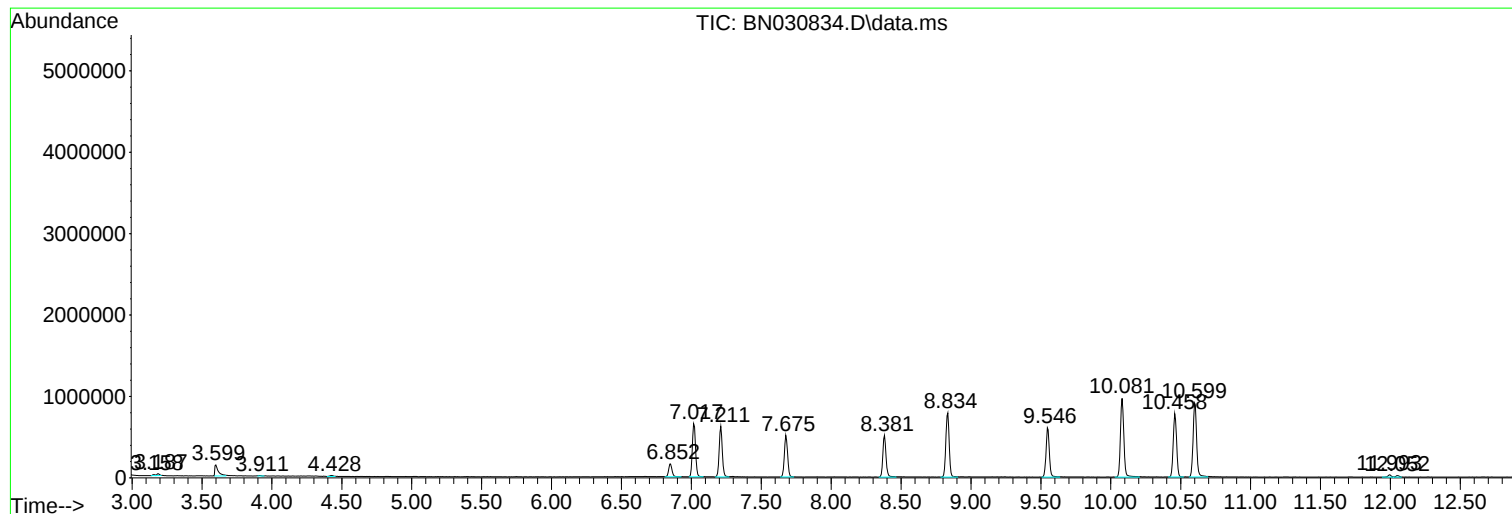

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030834.D
Acq On : 11 Apr 2024 03:04
Operator : MA/JU
Sample : P1982-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030834.D
Acq On : 11 Apr 2024 03:04
Operator : MA/JU
Sample : P1982-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc