

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030839.D
 Acq On : 11 Apr 2024 06:20
 Operator : MA/JU
 Sample : PB160082BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK082

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030839.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	44	rVB	39349	58315	0.86%	0.102%
2	3.593	99	103	126	rBV	524593	937158	13.86%	1.637%
3	3.905	154	156	162	rVB3	7250	9567	0.14%	0.017%
4	6.846	650	656	667	rBV	716848	1134989	16.79%	1.982%
5	7.016	678	685	701	rBV	589722	916083	13.55%	1.600%
6	7.211	711	718	729	rBV	710229	1140852	16.88%	1.992%
7	7.675	790	797	807	rBV	595986	940370	13.91%	1.642%
8	8.381	910	917	927	rBV	935901	1493733	22.10%	2.608%
9	8.834	985	994	1002	rBV	688842	1153714	17.07%	2.015%
10	9.546	1109	1115	1127	rBV	572963	931703	13.78%	1.627%
11	10.081	1199	1206	1219	rBV	924372	1581494	23.40%	2.762%
12	10.457	1263	1270	1279	rBV	923306	1506933	22.29%	2.631%
13	10.599	1286	1294	1314	rBV	988763	1728536	25.57%	3.018%
14	12.052	1535	1541	1547	rBV2	16011	27493	0.41%	0.048%
15	13.216	1734	1739	1746	rBV3	13747	23486	0.35%	0.041%
16	13.734	1821	1827	1835	rBV	1873189	2545028	37.65%	4.444%
17	14.010	1865	1874	1887	rBV	2199457	3200811	47.35%	5.589%
18	14.316	1919	1926	1938	rBV	1520393	2273042	33.63%	3.969%
19	14.528	1955	1962	1989	rBV	722255	1361936	20.15%	2.378%
20	15.316	2089	2096	2110	rBV	2895680	4073008	60.25%	7.112%
21	15.434	2110	2116	2130	rVV	747829	1055814	15.62%	1.844%
22	15.551	2133	2136	2141	rVB2	13488	20668	0.31%	0.036%
23	16.098	2225	2229	2236	rVB5	8535	15134	0.22%	0.026%
24	17.069	2387	2394	2404	rBV	2171229	3066962	45.37%	5.356%
25	17.169	2404	2411	2426	rVV	3388504	4870198	72.05%	8.505%
26	19.028	2722	2727	2732	rBV	47784	68294	1.01%	0.119%
27	19.098	2735	2739	2745	rBV	38979	57922	0.86%	0.101%
28	19.469	2796	2802	2809	rBV2	4523290	6116564	90.48%	10.681%
29	21.304	3108	3114	3125	rBV2	2726320	3970650	58.74%	6.934%
30	24.033	3569	3578	3594	rBV2	2640483	6759812	100.00%	11.804%
31	24.233	3604	3612	3625	rVB	1660587	4225662	62.51%	7.379%




Sum of corrected areas: 57265931

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030839.D
Acq On : 11 Apr 2024 06:20
Operator : MA/JU
Sample : PB160082BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK082

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

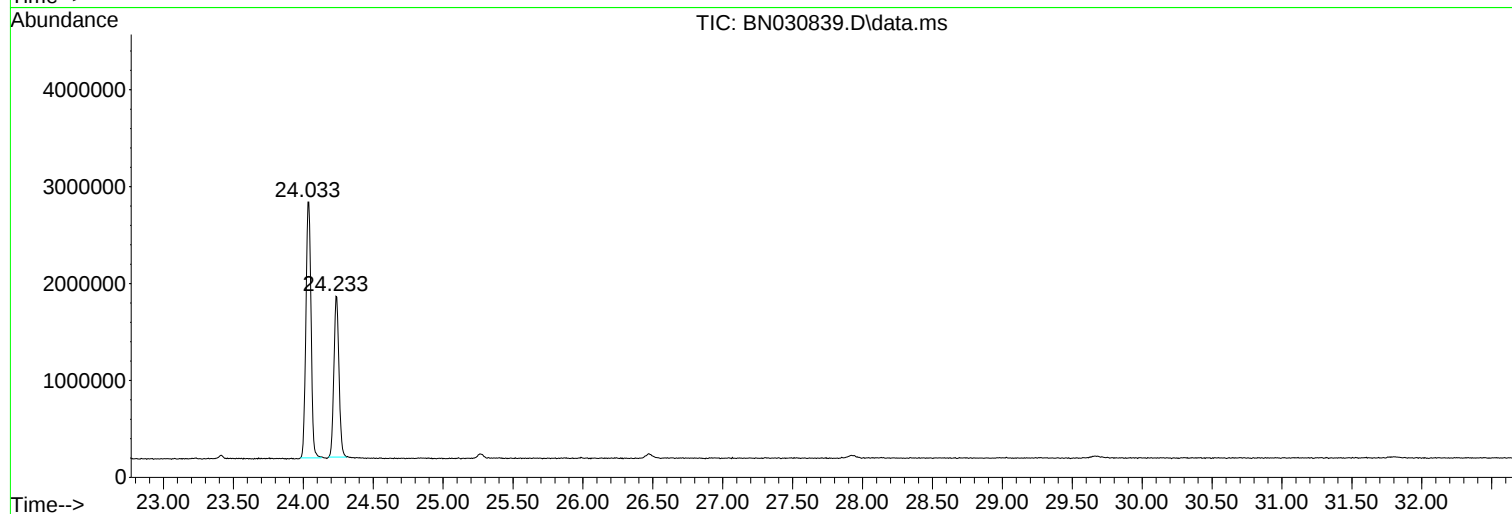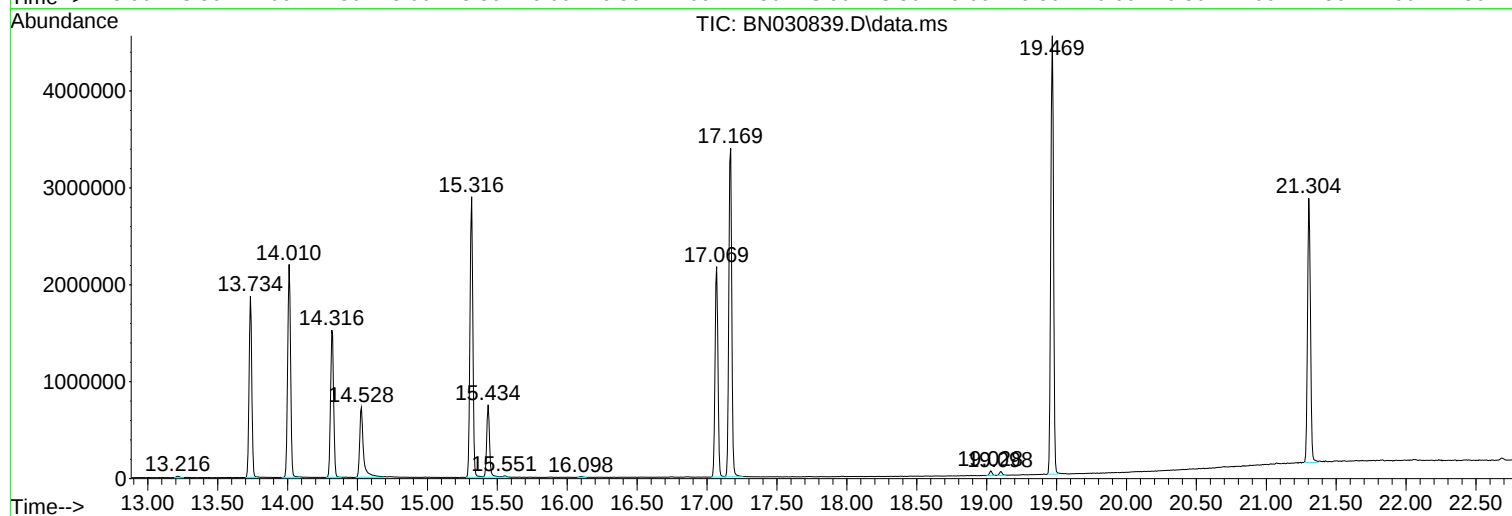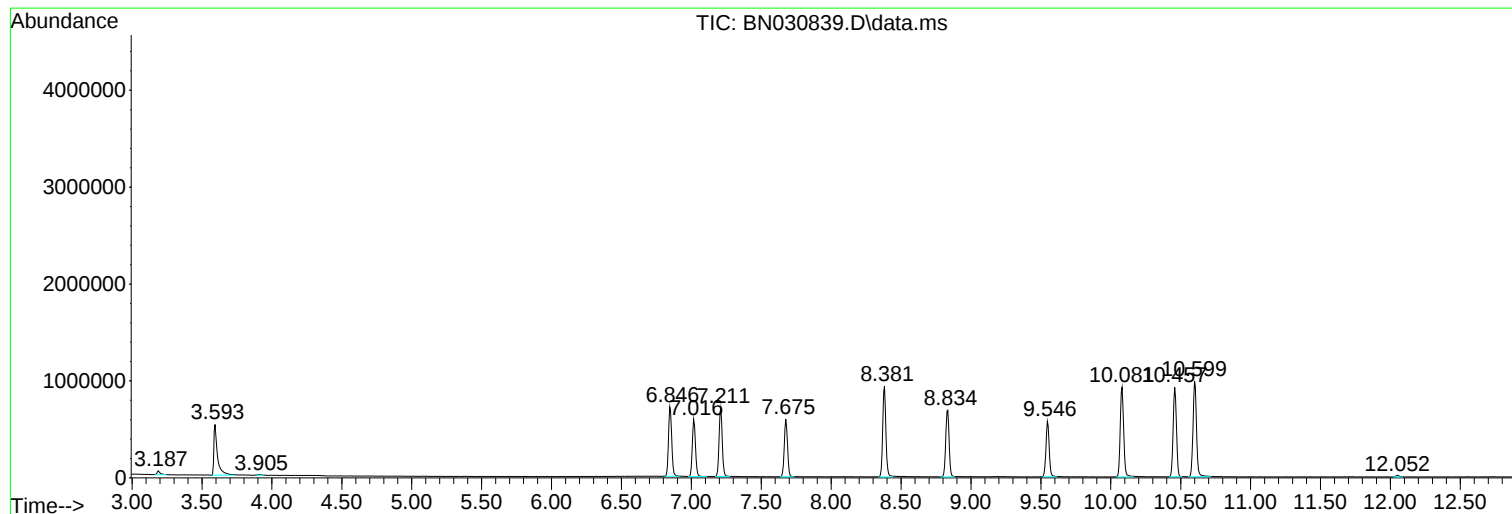

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030839.D
Acq On : 11 Apr 2024 06:20
Operator : MA/JU
Sample : PB160082BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK082

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030839.D
Acq On : 11 Apr 2024 06:20
Operator : MA/JU
Sample : PB160082BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK082

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc