

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
 Data File : BN030841.D
 Acq On : 11 Apr 2024 08:46
 Operator : MA/JU
 Sample : PB160146BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK146

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	41	rVB	38701	57269	0.89%	0.104%
2	3.587	99	102	126	rBV	499493	912882	14.15%	1.665%
3	3.899	153	155	159	rBV3	6990	9056	0.14%	0.017%
4	6.840	649	655	667	rBV	698454	1095575	16.98%	1.998%
5	7.010	677	684	694	rVB	581001	901836	13.98%	1.645%
6	7.205	710	717	727	rBV	689958	1111816	17.23%	2.028%
7	7.669	789	796	806	rBV	571925	912711	14.15%	1.664%
8	8.375	909	916	932	rBV	899184	1464334	22.69%	2.670%
9	8.828	985	993	1003	rBV	698684	1117313	17.32%	2.038%
10	9.540	1108	1114	1125	rBV	535767	886583	13.74%	1.617%
11	10.075	1198	1205	1219	rBV	927228	1542122	23.90%	2.812%
12	10.451	1261	1269	1279	rBV	868295	1469750	22.78%	2.680%
13	10.599	1287	1294	1306	rBV	942720	1646285	25.51%	3.002%
14	12.051	1534	1541	1546	rBV	15416	26231	0.41%	0.048%
15	13.210	1733	1738	1745	rBV3	12291	21678	0.34%	0.040%
16	13.734	1817	1827	1837	rBV	1790268	2487616	38.55%	4.537%
17	14.010	1867	1874	1889	rBV	2050692	3028983	46.94%	5.524%
18	14.316	1919	1926	1937	rBV	1524286	2177594	33.75%	3.971%
19	14.528	1954	1962	1986	rBV	641139	1262741	19.57%	2.303%
20	15.316	2088	2096	2110	rBV	2634117	3897501	60.40%	7.108%
21	15.434	2110	2116	2131	rVV	705413	974274	15.10%	1.777%
22	15.557	2133	2137	2143	rVB4	15167	24368	0.38%	0.044%
23	16.098	2226	2229	2235	rVB5	8451	12823	0.20%	0.023%
24	16.545	2300	2305	2311	rVB3	6968	10901	0.17%	0.020%
25	16.851	2352	2357	2361	rVB3	6040	8984	0.14%	0.016%
26	17.069	2387	2394	2404	rBV	2039576	2907527	45.06%	5.302%
27	17.169	2404	2411	2432	rVB	3145893	4577995	70.95%	8.349%
28	17.616	2483	2487	2490	rBV5	6311	9132	0.14%	0.017%
29	17.963	2542	2546	2551	rBV7	5188	8461	0.13%	0.015%
30	19.033	2723	2728	2733	rVB	41277	56299	0.87%	0.103%
31	19.098	2735	2739	2744	rBV	34905	47358	0.73%	0.086%
32	19.469	2796	2802	2817	rBV	4171013	5853668	90.72%	10.675%
33	21.304	3109	3114	3126	rBV	2515515	3707129	57.45%	6.761%
34	24.039	3570	3579	3597	rBV	2620418	6452526	100.00%	11.767%
35	24.239	3604	3613	3628	rVB2	1614585	4152639	64.36%	7.573%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030841.D
Acq On : 11 Apr 2024 08:46
Operator : MA/JU
Sample : PB160146BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK146

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 54833960

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030841.D
Acq On : 11 Apr 2024 08:46
Operator : MA/JU
Sample : PB160146BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK146

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

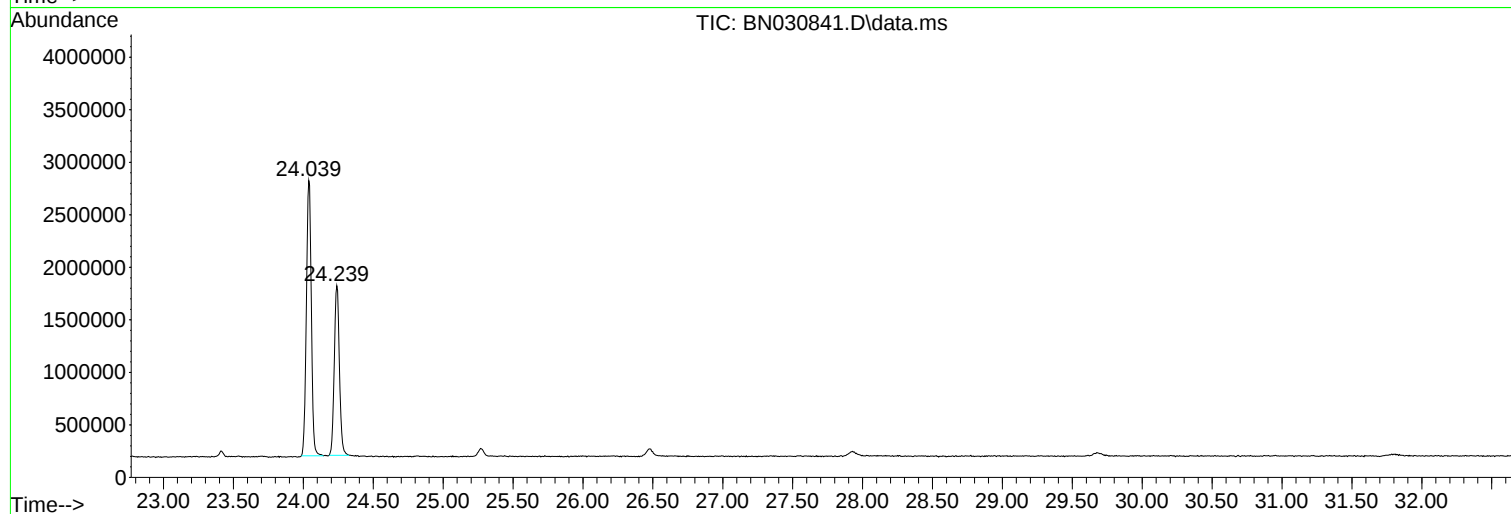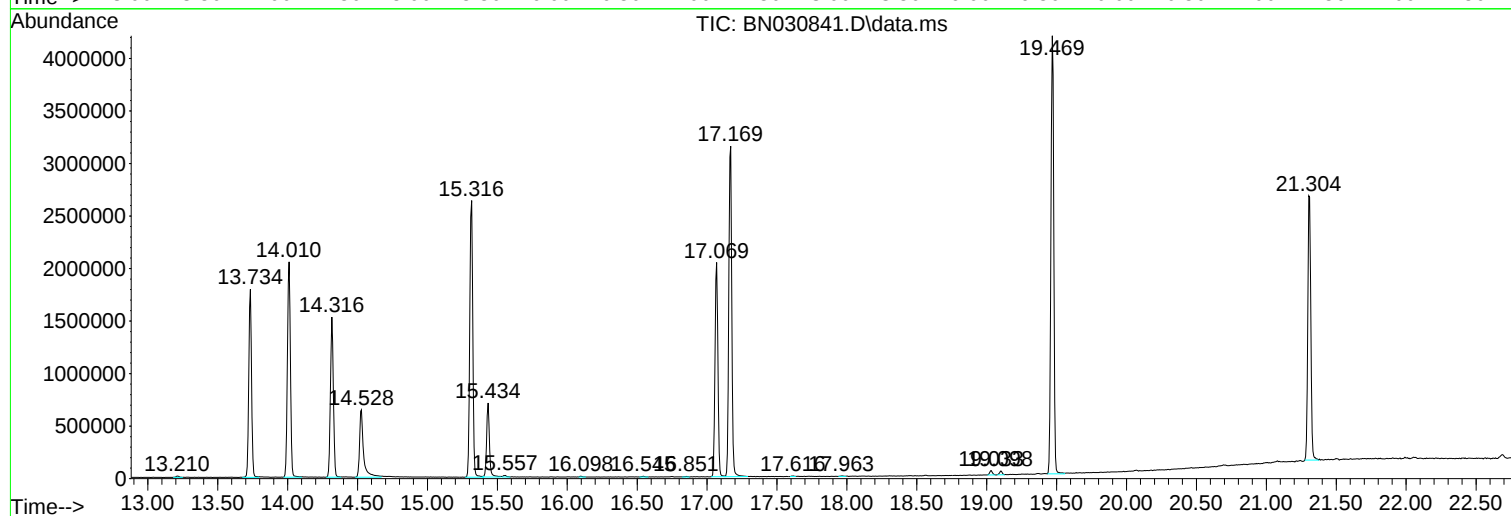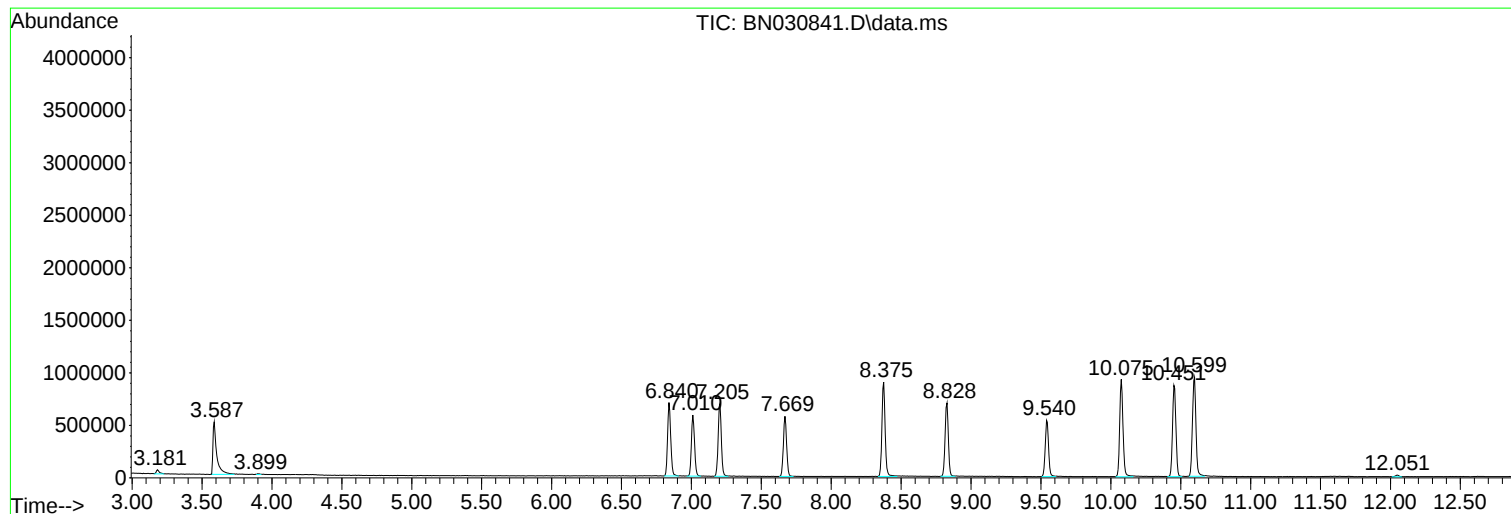

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030841.D
Acq On : 11 Apr 2024 08:46
Operator : MA/JU
Sample : PB160146BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK146

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041024\
Data File : BN030841.D
Acq On : 11 Apr 2024 08:46
Operator : MA/JU
Sample : PB160146BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK146

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------