
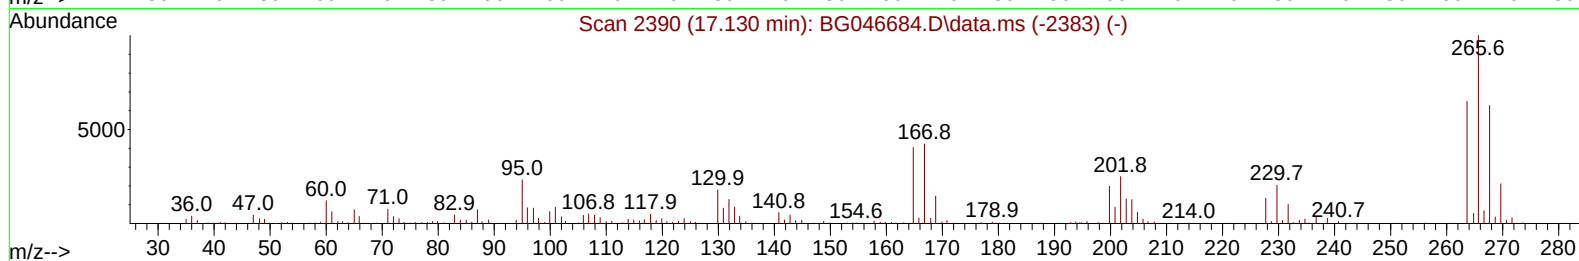
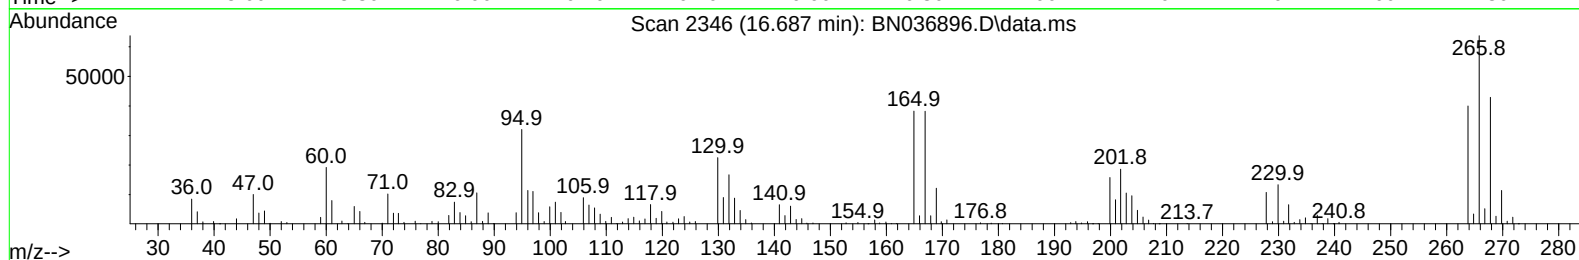


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036896.D
Acq On : 14 Apr 2025 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 19:33:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

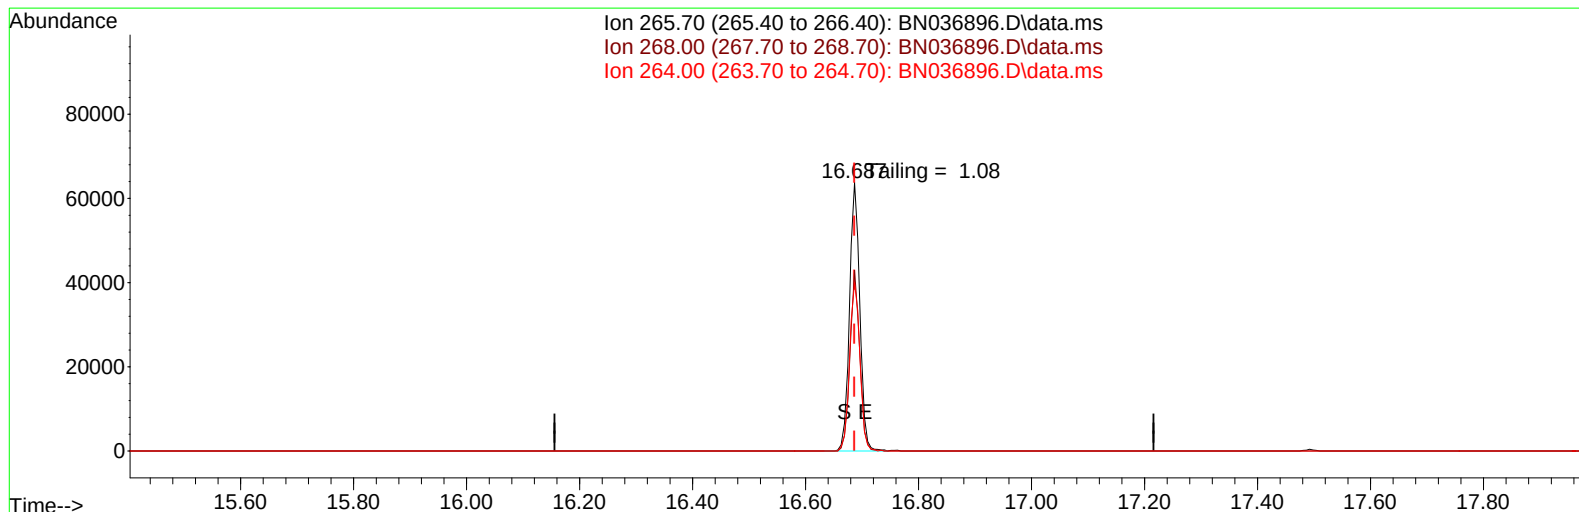

TIC: BN036896.D\data.ms

(70) Pentachlorophenol (C)




16.687min (+ 0.001) 15197.46 ng

response 80743

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.34
264.00	61.60	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036896.D
Acq On : 14 Apr 2025 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 19:23:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

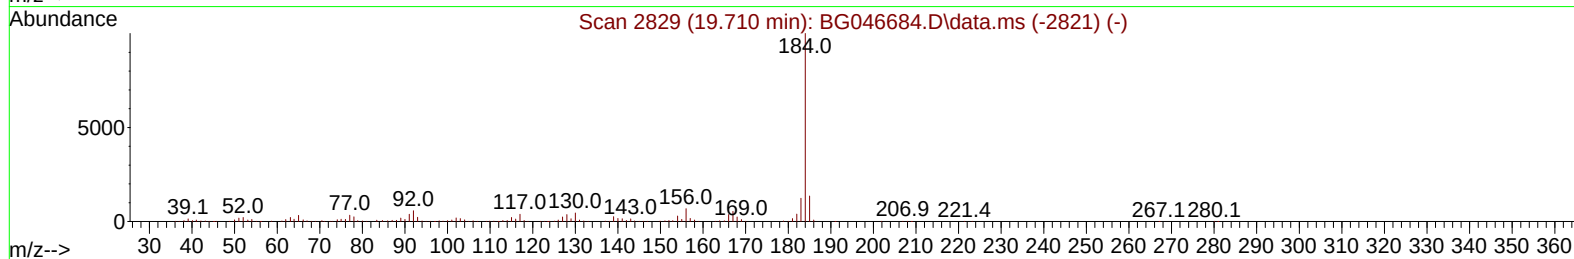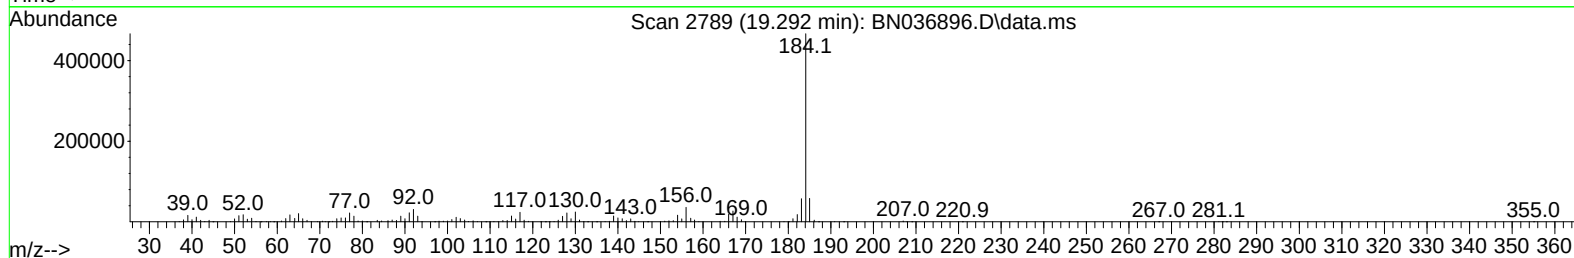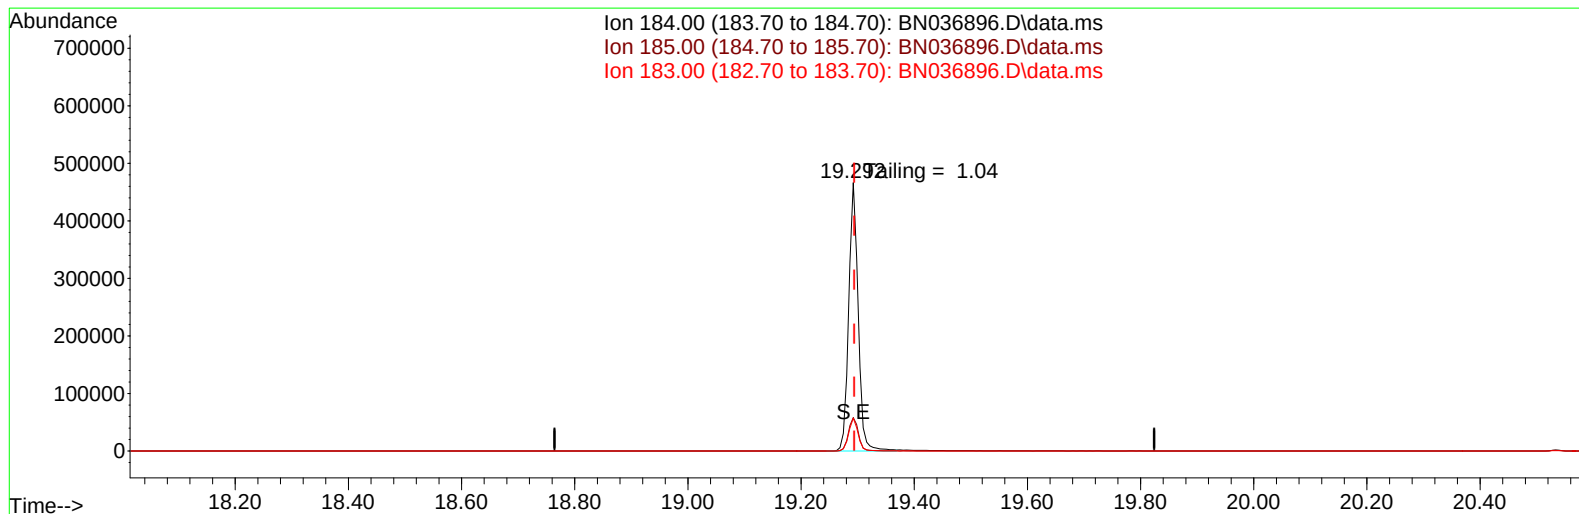

TIC: BN036896.D\data.ms

(77) Benzdine

19.292min (-0.002) 0.00 ng

response 549129

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.46
183.00	13.20	12.25
0.00	0.00	0.00