

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
 Data File : BN024953.D
 Acq On : 17 Apr 2023 13:30
 Operator : CG/JU
 Sample : 02254-14DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	10	14	21	rBV	82670	139949	2.90%	0.400%
2	3.340	21	26	39	rVB	317353	512442	10.64%	1.463%
3	3.581	65	67	71	rBV5	6173	7444	0.15%	0.021%
4	3.758	96	97	110	rBV2	51313	111914	2.32%	0.320%
5	4.064	145	149	156	rVB2	20796	29462	0.61%	0.084%
6	4.605	236	241	246	rVB7	6527	14099	0.29%	0.040%
7	6.022	475	482	489	rVB5	32213	52974	1.10%	0.151%
8	6.263	519	523	529	rBV2	17156	27302	0.57%	0.078%
9	7.093	659	664	671	rVB	54579	85854	1.78%	0.245%
10	7.257	685	692	701	rBV	225370	362409	7.52%	1.035%
11	7.457	720	726	738	rBV	203338	336873	6.99%	0.962%
12	7.928	799	806	815	rBV	1072503	1746168	36.24%	4.985%
13	8.046	820	826	835	rVB	239123	395472	8.21%	1.129%
14	8.640	922	927	937	rBV	141820	249111	5.17%	0.711%
15	9.099	997	1005	1015	rBV	250890	431297	8.95%	1.231%
16	9.216	1020	1025	1029	rVV6	10532	20674	0.43%	0.059%
17	9.504	1069	1074	1079	rBV3	12982	21573	0.45%	0.062%
18	9.828	1122	1129	1138	rBV	174303	306799	6.37%	0.876%
19	10.363	1213	1220	1234	rBV	248828	450221	9.35%	1.285%
20	10.587	1255	1258	1264	rVB7	3850	5449	0.11%	0.016%
21	10.746	1277	1285	1293	rBV	1543987	2585021	53.66%	7.380%
22	10.887	1300	1309	1324	rBV	220404	423583	8.79%	1.209%
23	11.551	1416	1422	1425	rBV6	4230	9589	0.20%	0.027%
24	11.998	1494	1498	1502	rBV4	6951	10190	0.21%	0.029%
25	12.340	1552	1556	1558	rBV5	5715	8118	0.17%	0.023%
26	13.304	1717	1720	1727	rVB9	5802	7562	0.16%	0.022%
27	13.369	1727	1731	1733	rBV5	6173	7555	0.16%	0.022%
28	13.987	1829	1836	1843	rBV	607869	835380	17.34%	2.385%
29	14.098	1852	1855	1858	rBV4	4808	5861	0.12%	0.017%
30	14.269	1878	1884	1896	rBV	585356	868631	18.03%	2.480%
31	14.575	1929	1936	1947	rBV	2248589	3473396	72.10%	9.916%
32	14.792	1968	1973	1983	rBV7	13514	37989	0.79%	0.108%
33	15.128	2027	2030	2034	rBV5	4106	6856	0.14%	0.020%
34	15.310	2059	2061	2065	rBV5	3535	5299	0.11%	0.015%
35	15.357	2065	2069	2074	rVV7	9282	14276	0.30%	0.041%
36	15.569	2096	2105	2118	rBV	902560	1293163	26.84%	3.692%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
 Data File : BN024953.D
 Acq On : 17 Apr 2023 13:30
 Operator : CG/JU
 Sample : 02254-14DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

37	15.686	2120	2125	2134	rVV	211150	302062	6.27%	0.862%
38	15.804	2141	2145	2150	rVB7	5384	8268	0.17%	0.024%
39	15.933	2161	2167	2174	rBV	47009	74653	1.55%	0.213%
40	16.498	2260	2263	2268	rVB5	5863	8030	0.17%	0.023%
41	16.922	2331	2335	2340	rVB7	3851	7711	0.16%	0.022%
42	17.022	2349	2352	2358	rVB8	8111	11343	0.24%	0.032%
43	17.075	2358	2361	2365	rBV5	3675	7270	0.15%	0.021%
44	17.116	2365	2368	2371	rVB4	5290	7148	0.15%	0.020%
45	17.322	2397	2403	2414	rBV	2925147	4215487	87.50%	12.035%
46	17.422	2414	2420	2429	rVV2	1066845	1498503	31.10%	4.278%
47	18.210	2550	2554	2560	rBV3	28949	41339	0.86%	0.118%
48	18.427	2587	2591	2594	rBV5	5389	9188	0.19%	0.026%
49	19.286	2733	2737	2741	rBV6	16677	26020	0.54%	0.074%
50	19.486	2768	2771	2776	rBV5	23711	36167	0.75%	0.103%
51	19.716	2805	2810	2821	rBV	1416521	1919332	39.84%	5.480%
52	21.521	3111	3117	3129	rBV2	3525765	4791849	99.46%	13.681%
53	23.198	3399	3402	3408	rVB2	144070	208607	4.33%	0.596%
54	23.798	3498	3504	3517	rVB	925334	2136092	44.34%	6.098%
55	23.957	3524	3531	3543	rBV2	2482124	4817768	100.00%	13.755%




Sum of corrected areas: 35026792

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
Data File : BN024953.D
Acq On : 17 Apr 2023 13:30
Operator : CG/JU
Sample : 02254-14DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

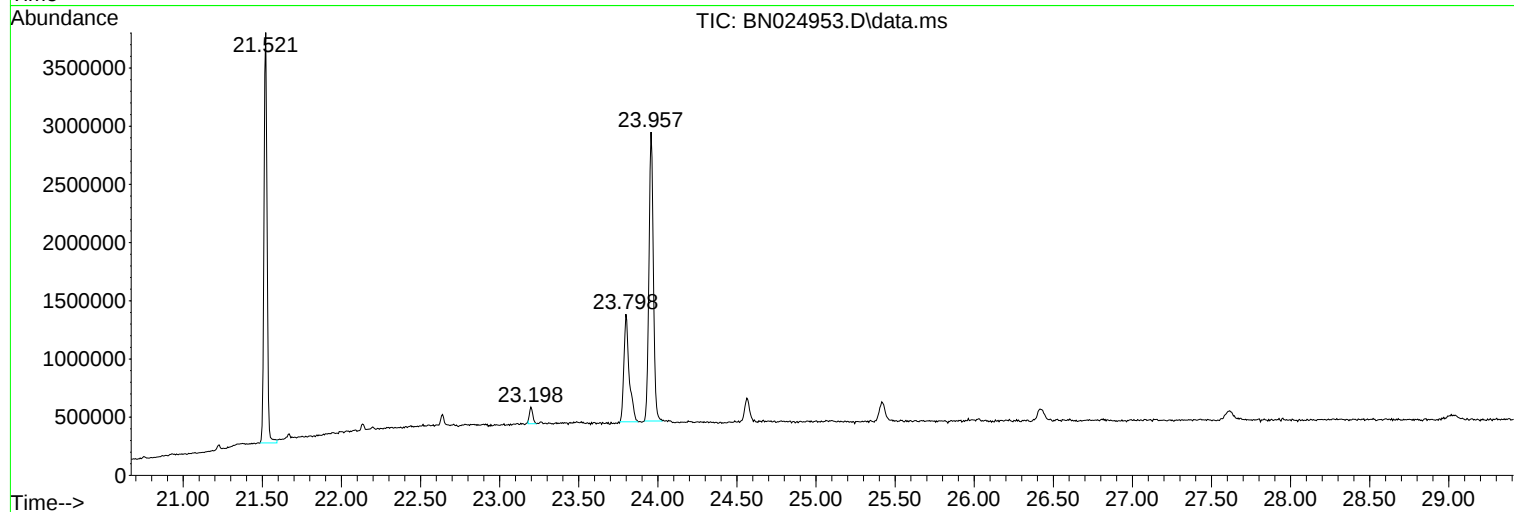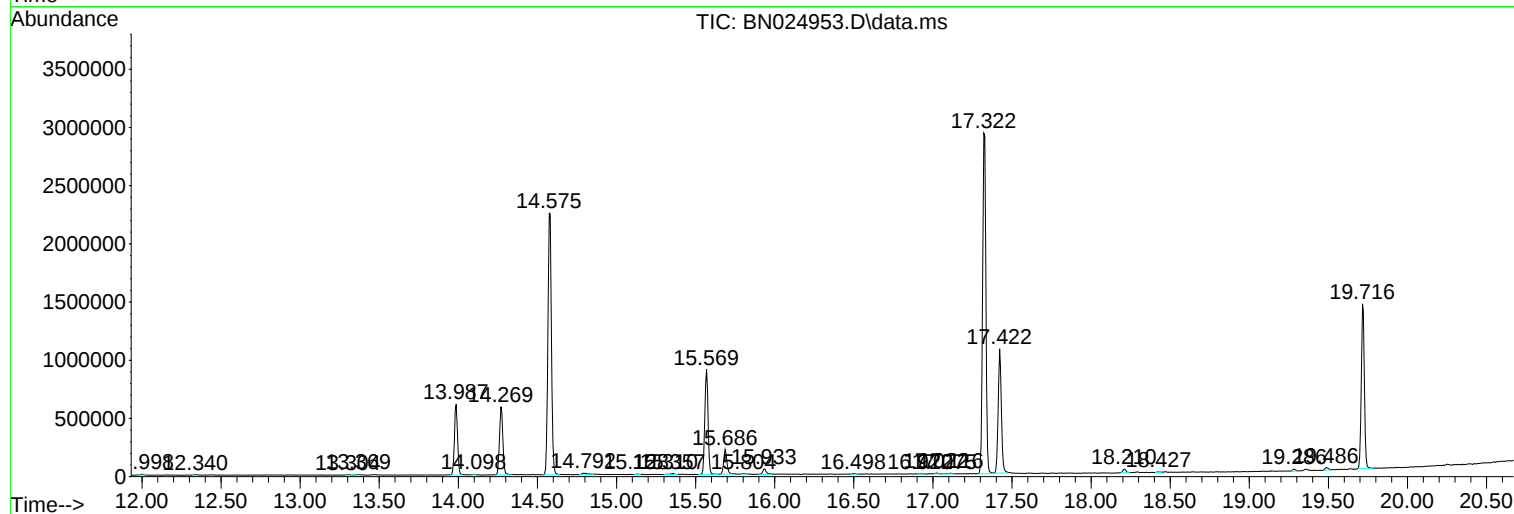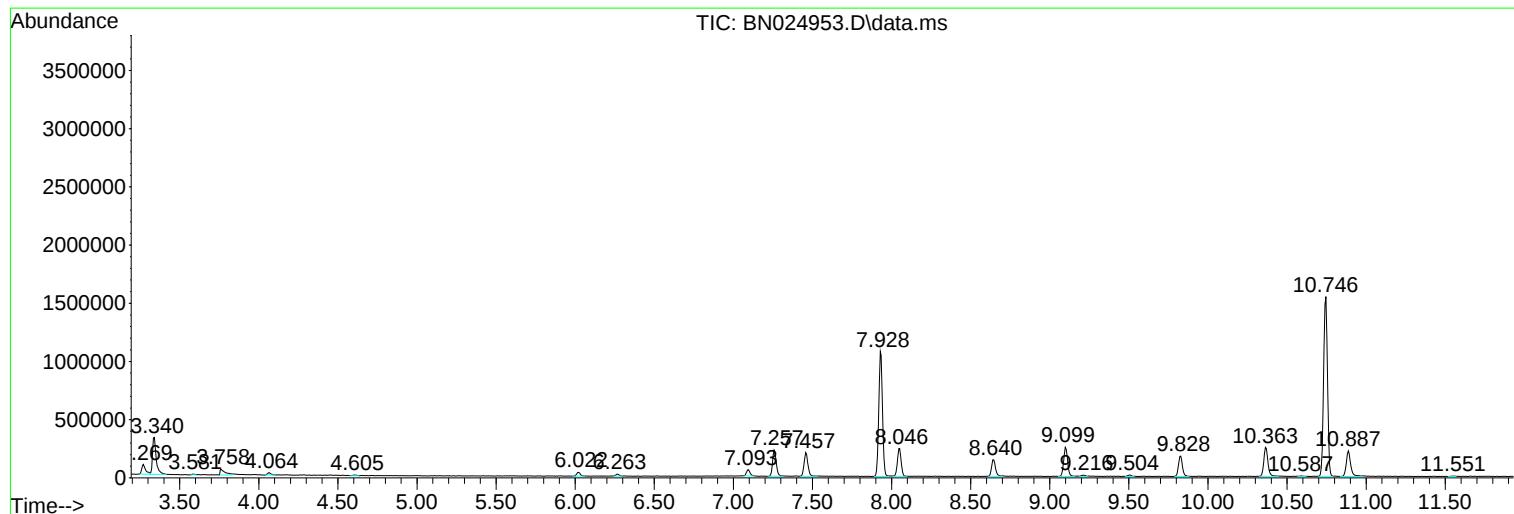

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
Data File : BN024953.D
Acq On : 17 Apr 2023 13:30
Operator : CG/JU
Sample : 02254-14DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC5DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.046	4.53 ng/ul	395472	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopropane, 1,1-dichloro-2-chl...	172	C5H7Cl3	015997-19-0	32
2			Methyl 3,3-dichloropropenoate	154	C4H4Cl2O2	002257-46-7	25
3			2,2-Dichloroethyl ethyl carbonate	186	C5H8Cl2O3	1010373-78-3	25
4			1-Propene, 3,3,3-trichloro-2-met...	158	C4H5Cl3	004749-27-3	25
5			1-Propene, 1,1,3-trichloro-2-met...	158	C4H5Cl3	031702-33-7	16

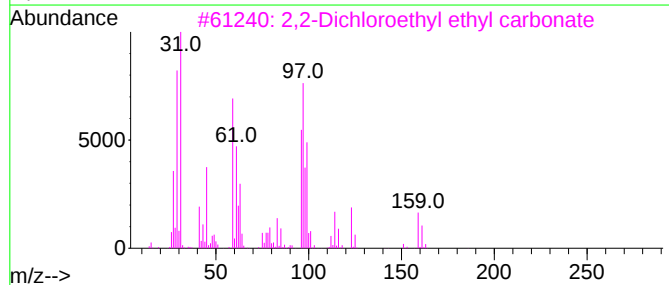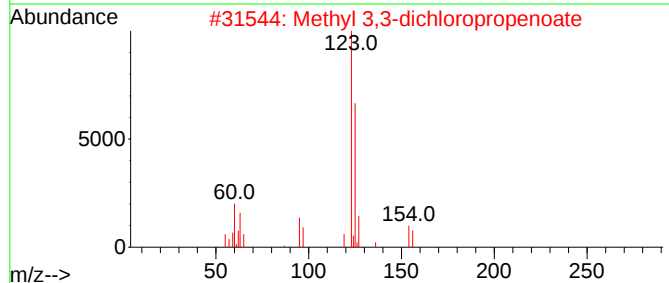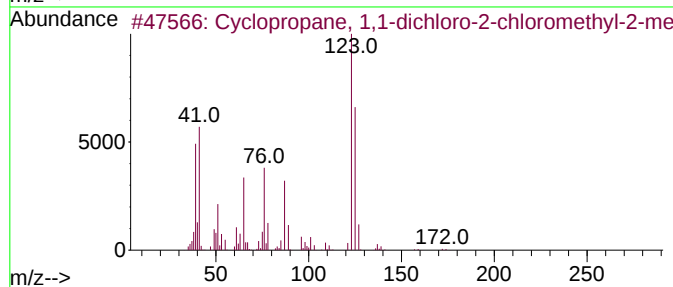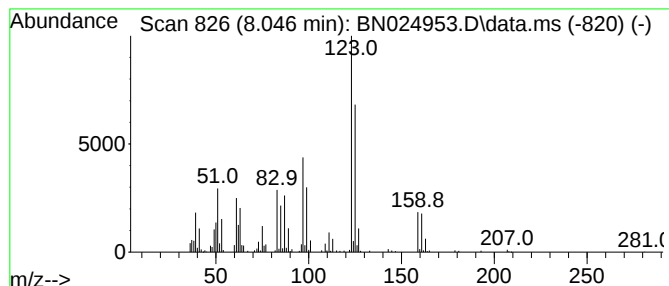

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
Data File : BN024953.D
Acq On : 17 Apr 2023 13:30
Operator : CG/JU
Sample : 02254-14DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	8.046	4.5	ng/u1	395472	1	7.934	1746170	20.0