

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
 Data File : BN024954.D
 Acq On : 17 Apr 2023 14:06
 Operator : CG/JU
 Sample : 02254-16DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	10	14	22	rBV2	83877	145327	2.83%	0.409%
2	3.340	22	26	40	rVB	354499	563708	10.96%	1.587%
3	3.581	64	67	72	rBV5	8581	16684	0.32%	0.047%
4	3.763	95	98	112	rBV	41790	97821	1.90%	0.275%
5	4.063	145	149	158	rVB	22392	38855	0.76%	0.109%
6	4.275	183	185	192	rVB8	5747	9440	0.18%	0.027%
7	4.604	237	241	245	rVB7	8015	11684	0.23%	0.033%
8	5.346	363	367	370	rBV6	5712	8063	0.16%	0.023%
9	6.022	478	482	491	rVB9	9516	15852	0.31%	0.045%
10	6.263	521	523	528	rVB5	3724	5251	0.10%	0.015%
11	7.093	659	664	674	rVB	57418	100707	1.96%	0.283%
12	7.257	686	692	703	rBV	228147	365664	7.11%	1.029%
13	7.457	719	726	736	rBV	199970	334543	6.51%	0.942%
14	7.928	800	806	815	rBV	1146427	1895599	36.86%	5.336%
15	8.051	822	827	833	rVB	35998	60466	1.18%	0.170%
16	8.645	921	928	936	rBV	150430	263946	5.13%	0.743%
17	8.945	973	979	982	rBV5	3156	5144	0.10%	0.014%
18	9.022	987	992	998	rBV7	2640	5448	0.11%	0.015%
19	9.098	998	1005	1014	rBV	252466	428665	8.34%	1.207%
20	9.504	1069	1074	1078	rVB4	5530	9653	0.19%	0.027%
21	9.828	1121	1129	1138	rBV	174067	307439	5.98%	0.865%
22	10.363	1214	1220	1235	rBV	250630	450260	8.76%	1.267%
23	10.745	1276	1285	1296	rBV	1670637	2823354	54.90%	7.947%
24	10.887	1302	1309	1318	rBV	242896	431550	8.39%	1.215%
25	12.339	1551	1556	1557	rBV4	5136	5401	0.11%	0.015%
26	13.398	1734	1736	1740	rVV4	5494	7176	0.14%	0.020%
27	13.469	1744	1748	1756	rVV8	7045	12217	0.24%	0.034%
28	13.986	1830	1836	1843	rBV	603264	824159	16.03%	2.320%
29	14.269	1878	1884	1891	rBV	594019	867924	16.88%	2.443%
30	14.575	1927	1936	1947	rBV	2549892	3752910	72.97%	10.563%
31	14.792	1970	1973	1980	rBV5	11211	26972	0.52%	0.076%
32	15.316	2058	2062	2068	rVB3	6590	8822	0.17%	0.025%
33	15.392	2072	2075	2078	rBV4	4156	5271	0.10%	0.015%
34	15.569	2098	2105	2114	rBV	894604	1277841	24.85%	3.597%
35	15.686	2119	2125	2135	rBV	176633	266526	5.18%	0.750%
36	15.810	2143	2146	2151	rVB6	5215	7616	0.15%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
 Data File : BN024954.D
 Acq On : 17 Apr 2023 14:06
 Operator : CG/JU
 Sample : 02254-16DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA6DL

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

37	15.933	2162	2167	2173	rBV	82538	115537	2.25%	0.325%
38	17.074	2357	2361	2365	rBV6	3954	5270	0.10%	0.015%
39	17.116	2365	2368	2374	rVV3	8243	12151	0.24%	0.034%
40	17.327	2397	2404	2412	rBV	3269316	4559204	88.65%	12.833%
41	17.421	2415	2420	2429	rVV2	977901	1380394	26.84%	3.885%
42	18.210	2550	2554	2559	rBV3	58219	78233	1.52%	0.220%
43	19.280	2734	2736	2743	rVB7	15048	21708	0.42%	0.061%
44	19.486	2768	2771	2776	rBV6	29367	44509	0.87%	0.125%
45	19.715	2805	2810	2819	rBV	1293005	1773941	34.49%	4.993%
46	21.521	3112	3117	3125	rBV	3998753	5142858	100.00%	14.476%
47	23.798	3498	3504	3517	rVB2	783486	1817584	35.34%	5.116%
48	23.956	3525	3531	3541	rVB2	2604540	5118221	99.52%	14.406%




Sum of corrected areas: 35527568

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
Data File : BN024954.D
Acq On : 17 Apr 2023 14:06
Operator : CG/JU
Sample : 02254-16DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

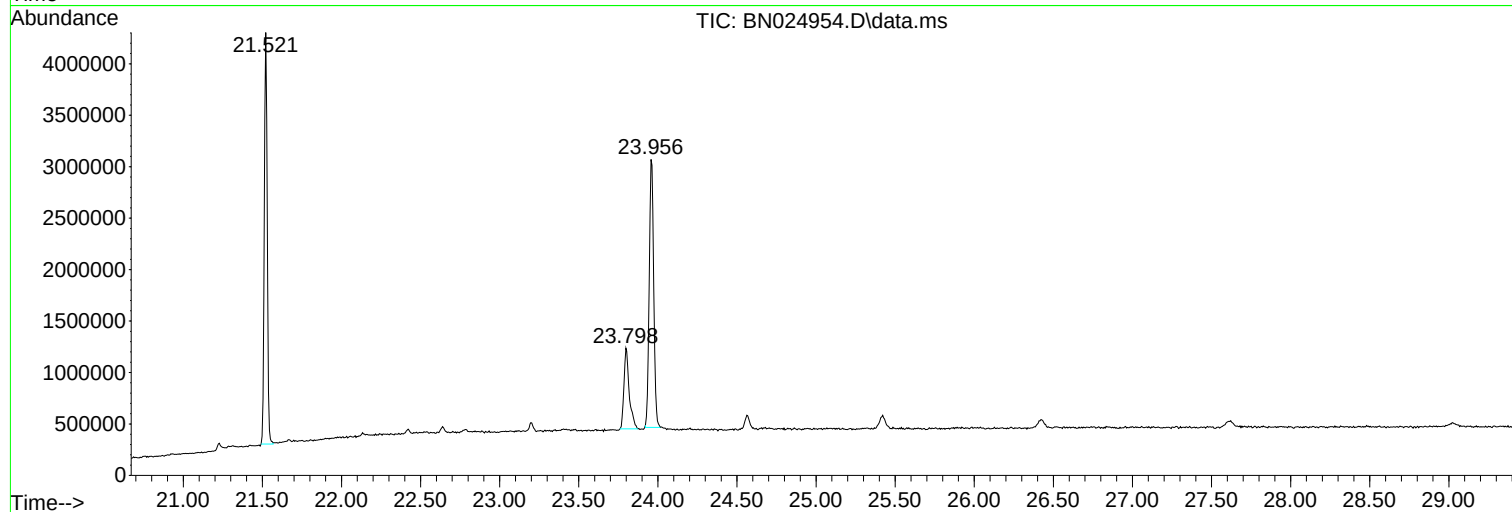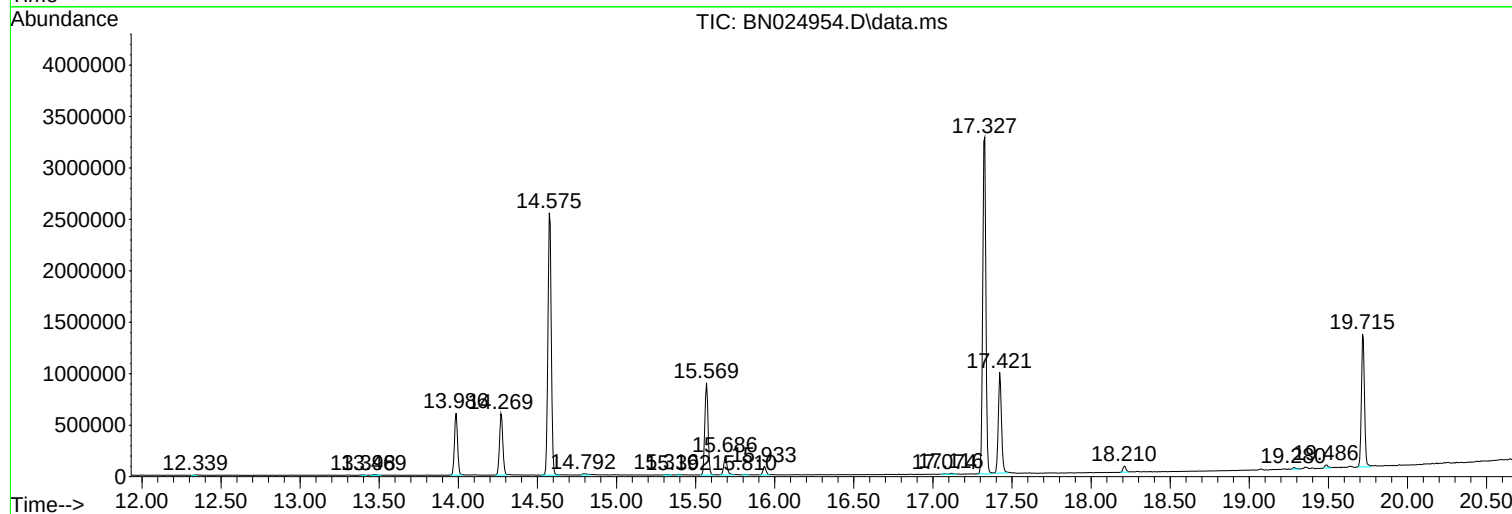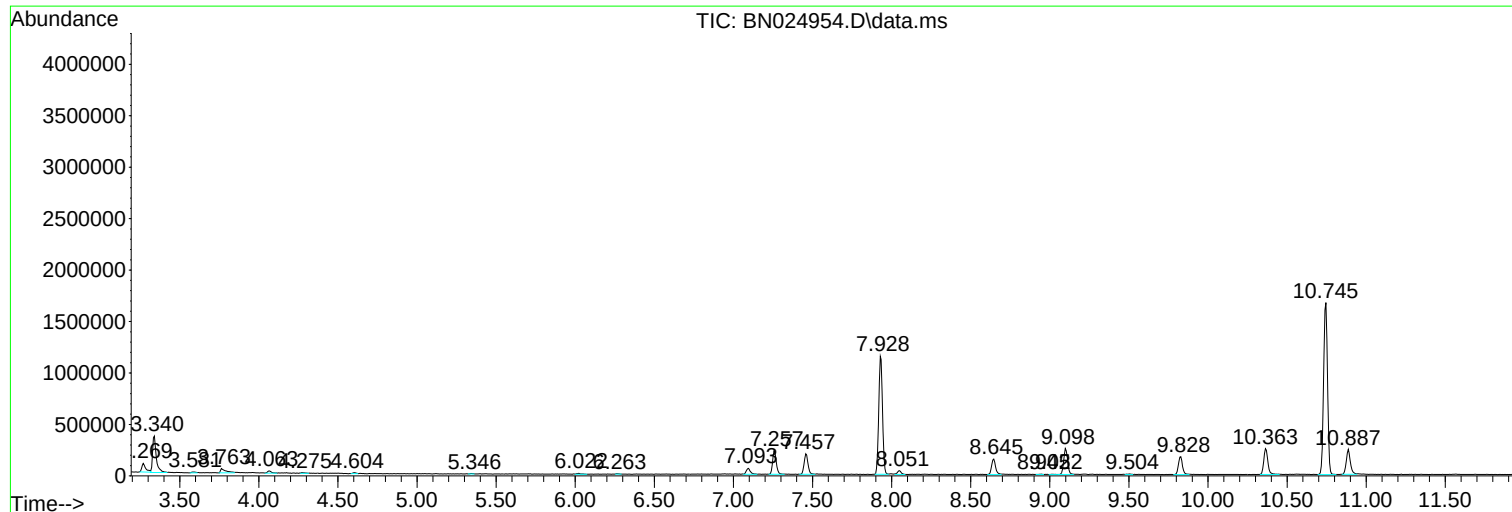

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
Data File : BN024954.D
Acq On : 17 Apr 2023 14:06
Operator : CG/JU
Sample : 02254-16DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
Data File : BN024954.D
Acq On : 17 Apr 2023 14:06
Operator : CG/JU
Sample : 02254-16DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc