

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
 Data File : BN024956.D
 Acq On : 17 Apr 2023 15:18
 Operator : CG/JU
 Sample : 02254-18DL 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024956.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	9	14	22	rBV2	185279	327766	6.24%	0.570%
2	3.334	22	25	45	rVB	442678	735072	13.99%	1.279%
3	3.587	64	68	79	rBV2	19553	31295	0.60%	0.054%
4	3.752	94	96	105	rBV	88412	154450	2.94%	0.269%
5	4.064	145	149	155	rVB	23577	38344	0.73%	0.067%
6	4.605	237	241	245	rVB5	11454	15077	0.29%	0.026%
7	5.005	302	309	310	rBV6	3505	6802	0.13%	0.012%
8	7.093	658	664	673	rVB	162015	267402	5.09%	0.465%
9	7.258	685	692	704	rBV	653291	1047266	19.94%	1.822%
10	7.458	718	726	737	rBV	632313	1005204	19.14%	1.749%
11	7.540	737	740	745	rVB7	4539	7438	0.14%	0.013%
12	7.928	798	806	815	rBV	1167433	1899334	36.16%	3.305%
13	8.046	821	826	832	rVB	71310	114118	2.17%	0.199%
14	8.640	920	927	937	rBV	473992	770656	14.67%	1.341%
15	9.099	997	1005	1018	rBV	804848	1313877	25.01%	2.286%
16	9.210	1020	1024	1030	rBV8	5240	11377	0.22%	0.020%
17	9.504	1067	1074	1081	rVB	16896	29211	0.56%	0.051%
18	9.822	1119	1128	1141	rBV	599289	999407	19.03%	1.739%
19	10.363	1213	1220	1234	rBV	854136	1410621	26.86%	2.455%
20	10.746	1275	1285	1295	rBV	1691197	2832591	53.93%	4.929%
21	10.887	1301	1309	1321	rBV	684968	1204108	22.92%	2.095%
22	11.540	1414	1420	1424	rBV6	4564	10559	0.20%	0.018%
23	12.004	1493	1499	1505	rVB2	16636	25972	0.49%	0.045%
24	12.334	1550	1555	1560	rBV4	13885	24265	0.46%	0.042%
25	13.987	1829	1836	1846	rBV	1700403	2306351	43.91%	4.013%
26	14.104	1851	1856	1861	rVV9	4240	6952	0.13%	0.012%
27	14.269	1877	1884	1897	rBV	1862672	2677878	50.98%	4.660%
28	14.575	1927	1936	1952	rBV	2483558	3738697	71.18%	6.506%
29	14.781	1965	1971	1981	rBV2	59904	137506	2.62%	0.239%
30	14.992	2003	2007	2009	rBV5	5064	6008	0.11%	0.010%
31	15.322	2057	2063	2067	rBV5	5133	7780	0.15%	0.014%
32	15.569	2098	2105	2116	rBV	2516447	3550477	67.59%	6.178%
33	15.686	2119	2125	2137	rVV	779709	1067856	20.33%	1.858%
34	15.810	2141	2146	2151	rVB6	11978	19333	0.37%	0.034%
35	15.934	2160	2167	2175	rVB	36492	53896	1.03%	0.094%
36	17.081	2356	2362	2364	rBV7	5258	8401	0.16%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
 Data File : BN024956.D
 Acq On : 17 Apr 2023 15:18
 Operator : CG/JU
 Sample : 02254-18DL 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

37	17.116	2364	2368	2370	rBV2	6083	7700	0.15%	0.013%
38	17.233	2385	2388	2393	rBV6	5201	7277	0.14%	0.013%
39	17.322	2397	2403	2414	rVV	3093390	4455366	84.82%	7.753%
40	17.422	2414	2420	2433	rVV	2857563	4020284	76.54%	6.996%
41	17.604	2448	2451	2456	rVB6	6593	9386	0.18%	0.016%
42	18.210	2549	2554	2560	rBV	82329	109850	2.09%	0.191%
43	18.292	2564	2568	2574	rVB2	15881	22918	0.44%	0.040%
44	19.286	2732	2737	2741	rBV4	37068	56412	1.07%	0.098%
45	19.357	2744	2749	2755	rBV2	34575	61611	1.17%	0.107%
46	19.486	2767	2771	2776	rBV2	54726	73790	1.40%	0.128%
47	19.639	2793	2797	2801	rBV7	11113	20614	0.39%	0.036%
48	19.716	2805	2810	2825	rVV	3686346	4897245	93.23%	8.522%
49	21.221	3063	3066	3070	rBV4	63690	90540	1.72%	0.158%
50	21.521	3111	3117	3129	rBV	4065694	5213162	99.25%	9.071%
51	23.815	3500	3507	3521	rBV2	2226783	4987820	94.96%	8.679%
52	23.974	3527	3534	3552	rVB2	2707173	5252730	100.00%	9.140%
53	24.592	3636	3639	3648	rVB2	169741	318860	6.07%	0.555%




Sum of corrected areas: 57468912

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
Data File : BN024956.D
Acq On : 17 Apr 2023 15:18
Operator : CG/JU
Sample : 02254-18DL 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

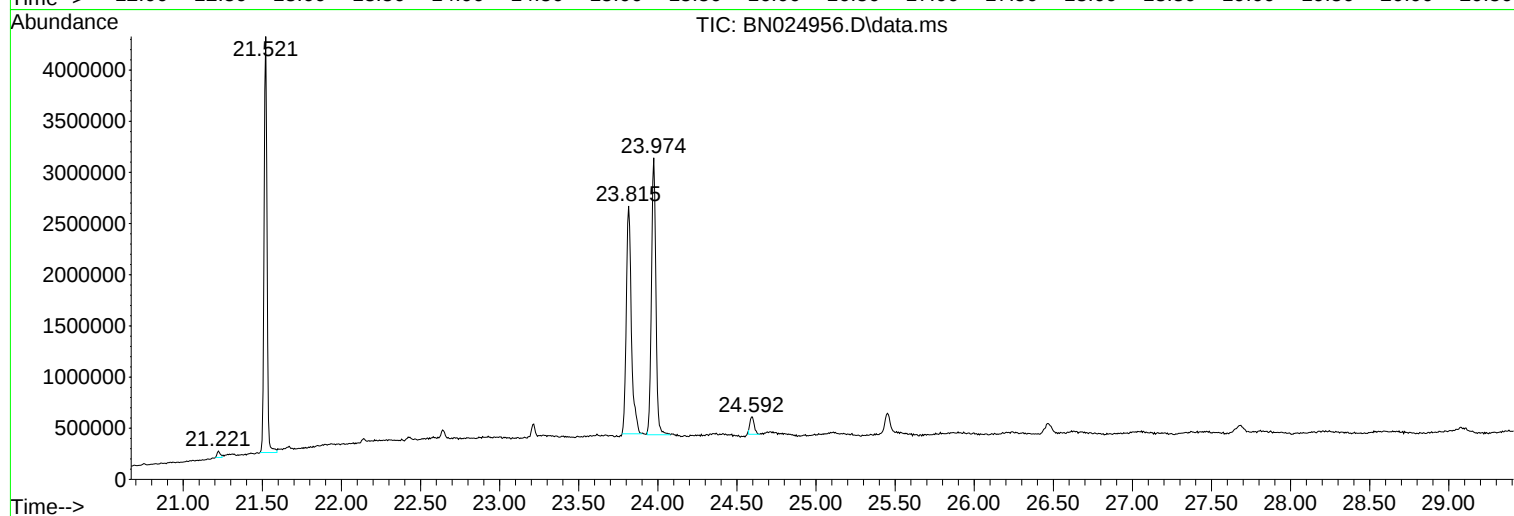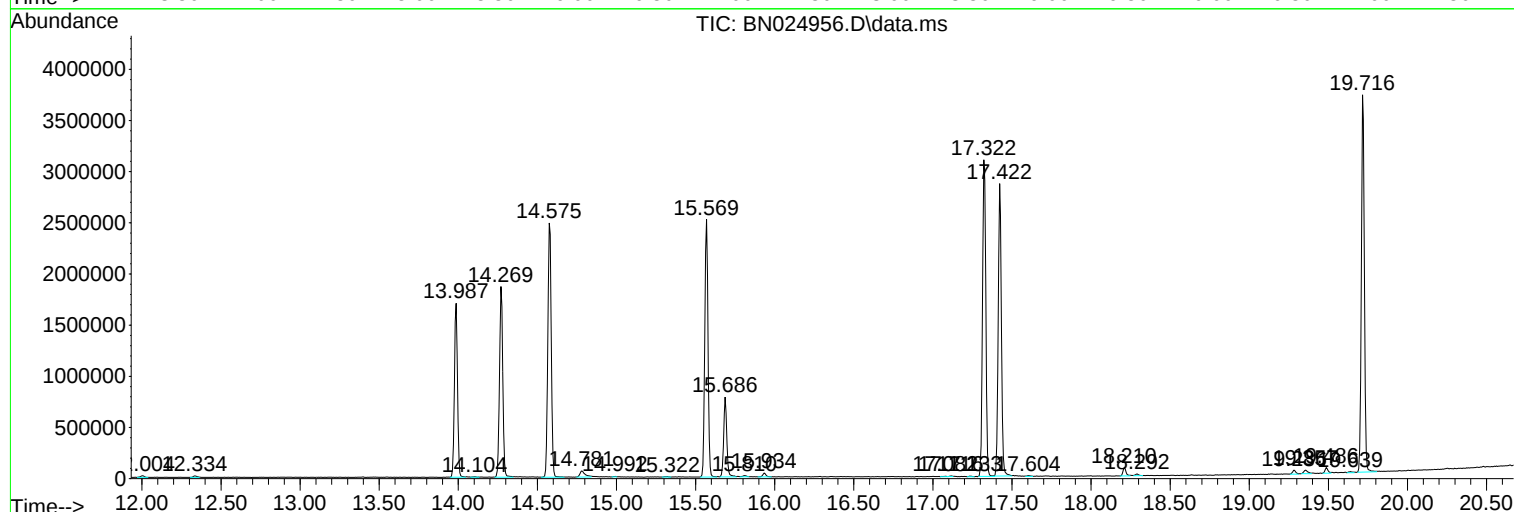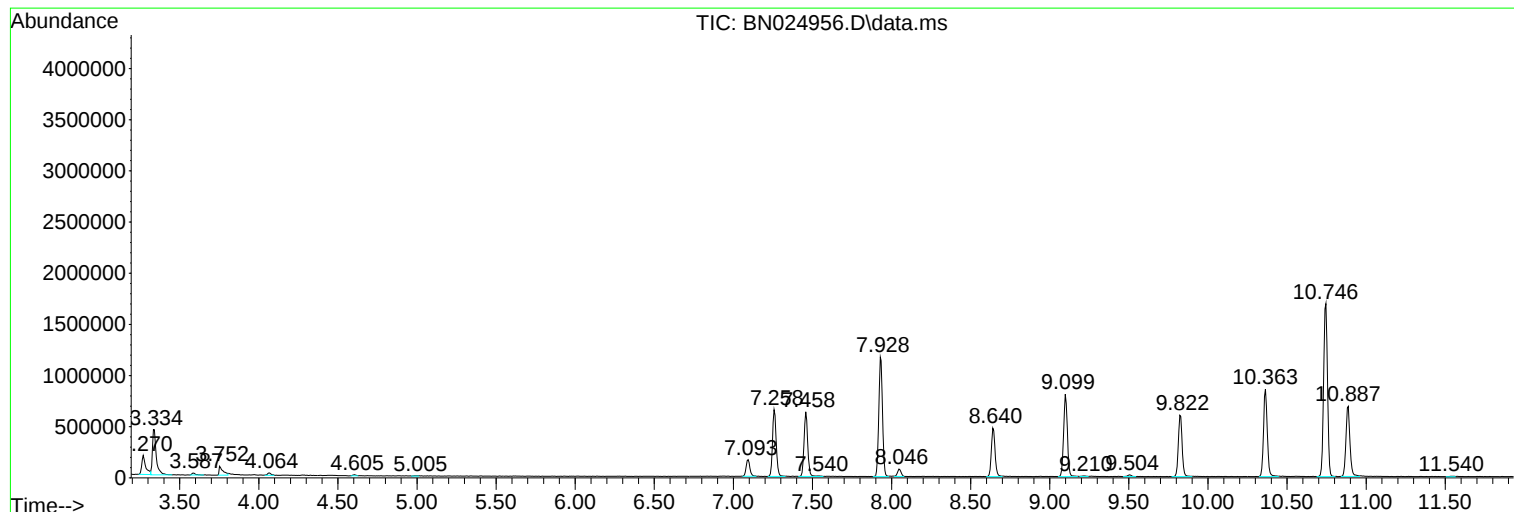

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
Data File : BN024956.D
Acq On : 17 Apr 2023 15:18
Operator : CG/JU
Sample : 02254-18DL 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041723\
Data File : BN024956.D
Acq On : 17 Apr 2023 15:18
Operator : CG/JU
Sample : 02254-18DL 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------