
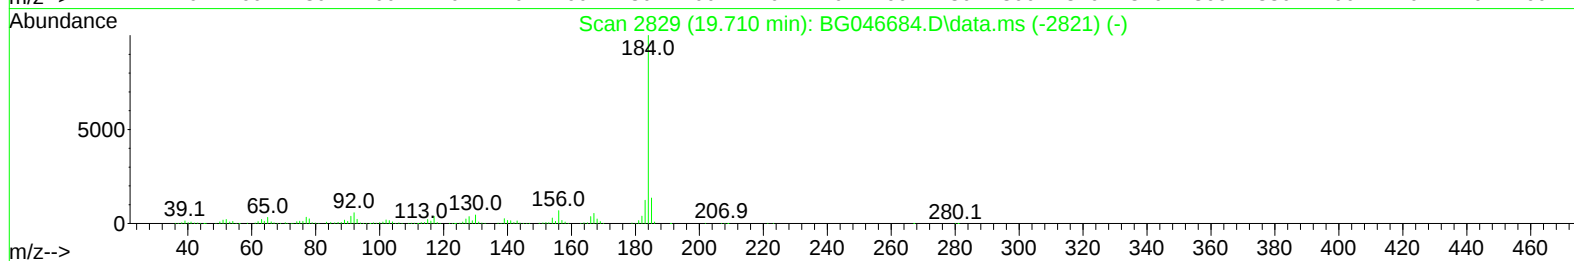
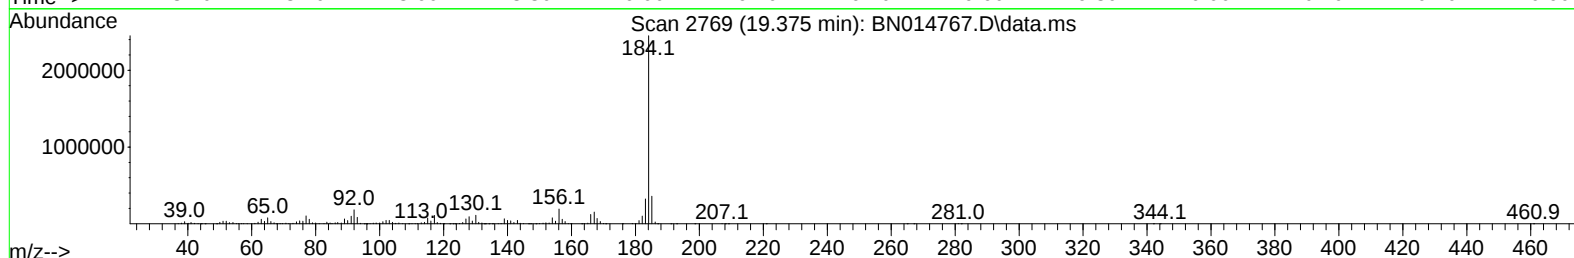


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052621\
Data File : BN014767.D
Acq On : 26 May 2021 15:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 16:21:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

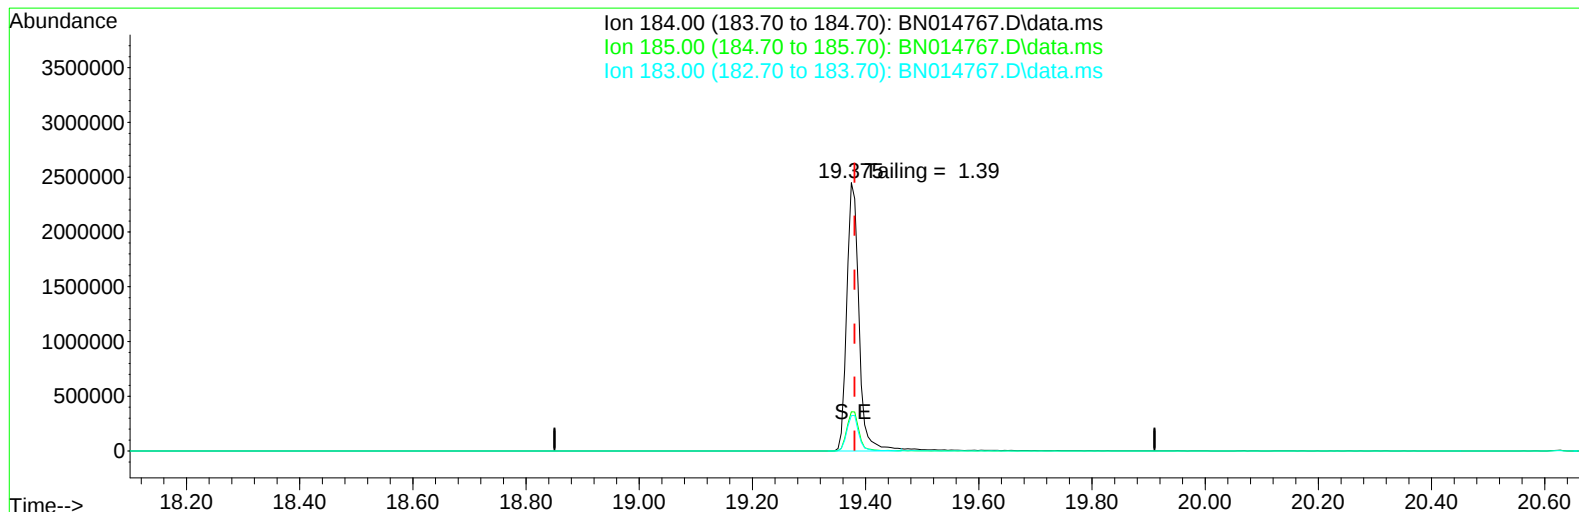




TIC: BN014767.D\data.ms

(77) Benzidine**19.375min (-0.005) 1096752.87 ng****response 3651244**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.63
183.00	13.20	13.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052621\
Data File : BN014767.D
Acq On : 26 May 2021 15:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 16:21:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

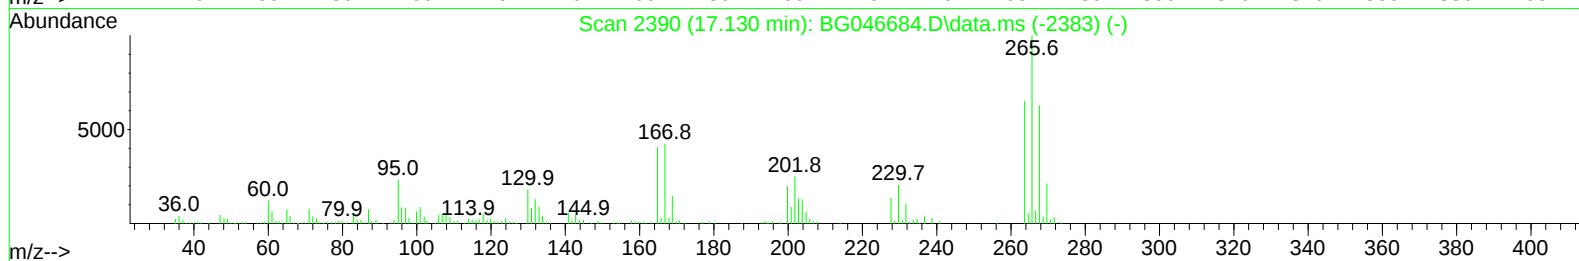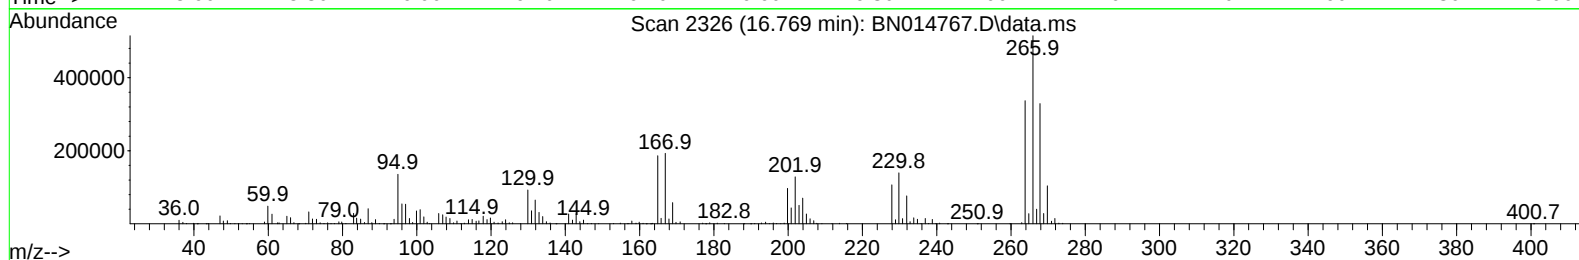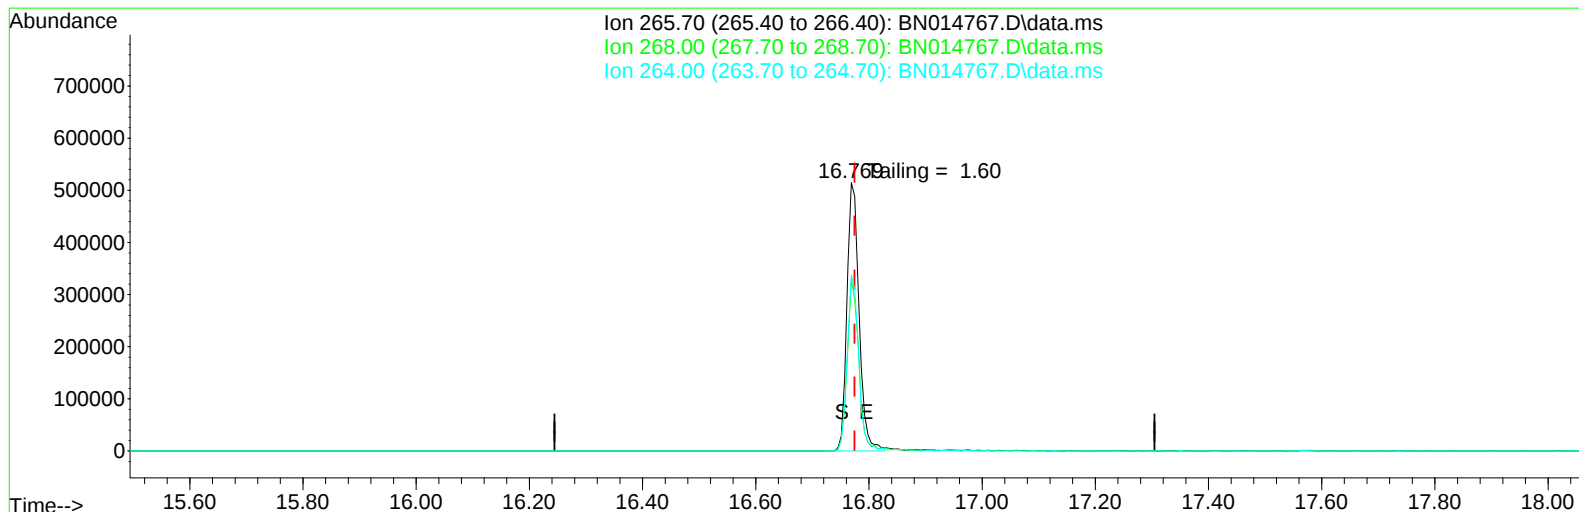

TIC: BN014767.D\data.ms

(70) Pentachlorophenol (C)

16.769min (-0.005) 17237.26 ng

response 772142

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.91
264.00	61.60	65.43
0.00	0.00	0.00