
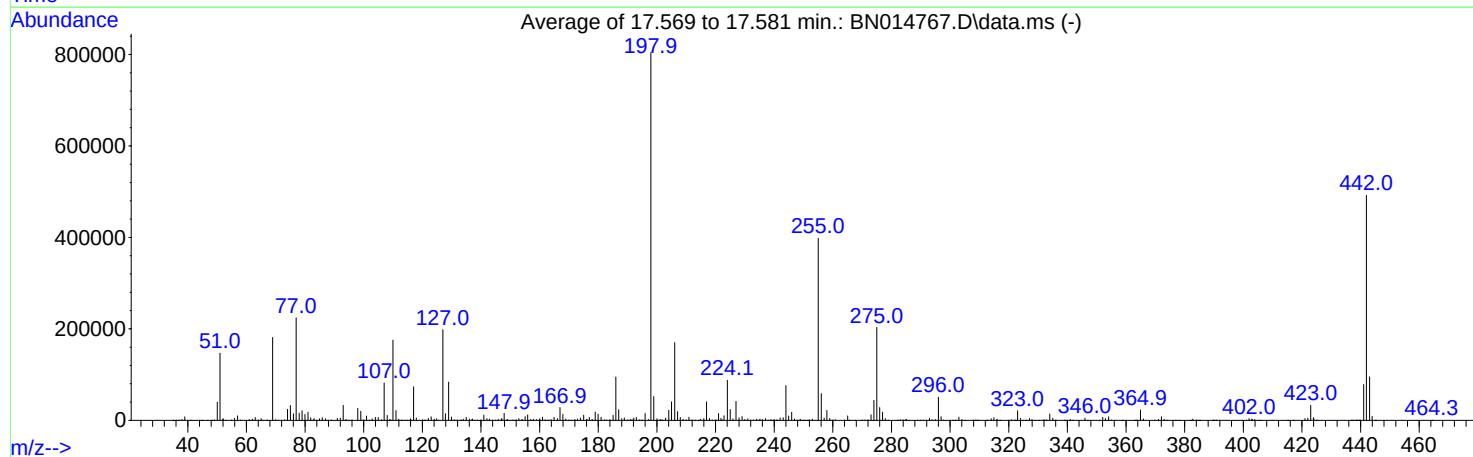


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052621\
 Data File : BN014767.D
 Acq On : 26 May 2021 15:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN052621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 27 01:39:07 2021

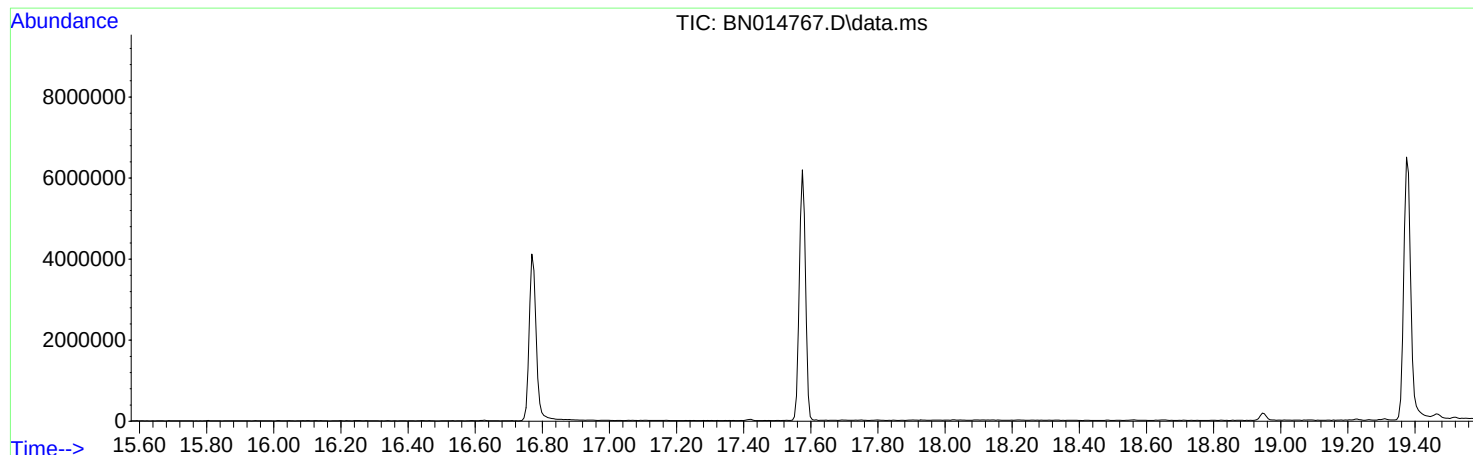




AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.3	146939	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	22.5	181227	PASS
70	69	0.00	2	0.8	1365	PASS
127	198	10	80	24.6	198229	PASS
197	198	0.00	2	0.2	1807	PASS
198	198	100	100	100.0	804331	PASS
199	198	5	9	6.5	51981	PASS
275	198	10	60	25.3	203243	PASS
365	198	1	100	2.8	22661	PASS
441	198	0.01	100	9.8	78515	PASS
442	442	50	100	100.0	491989	PASS
443	442	15	24	19.4	95291	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052621\
Data File : BN014767.D
Acq On : 26 May 2021 15:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 26 16:21:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

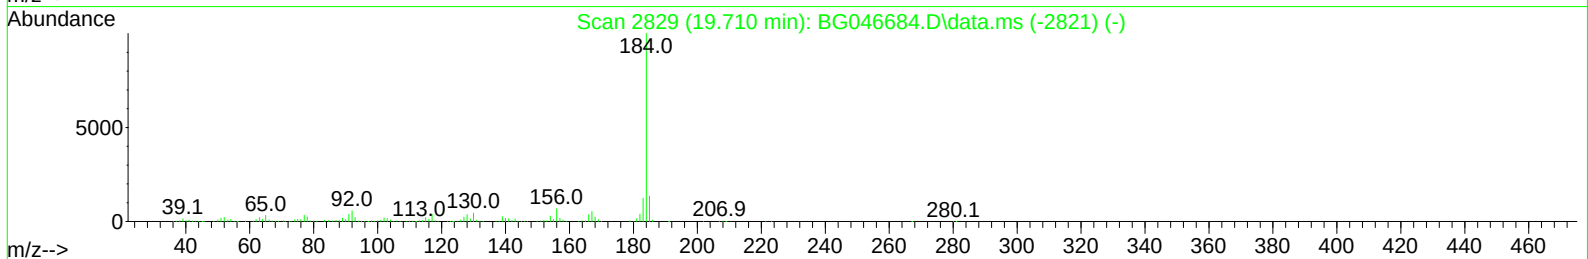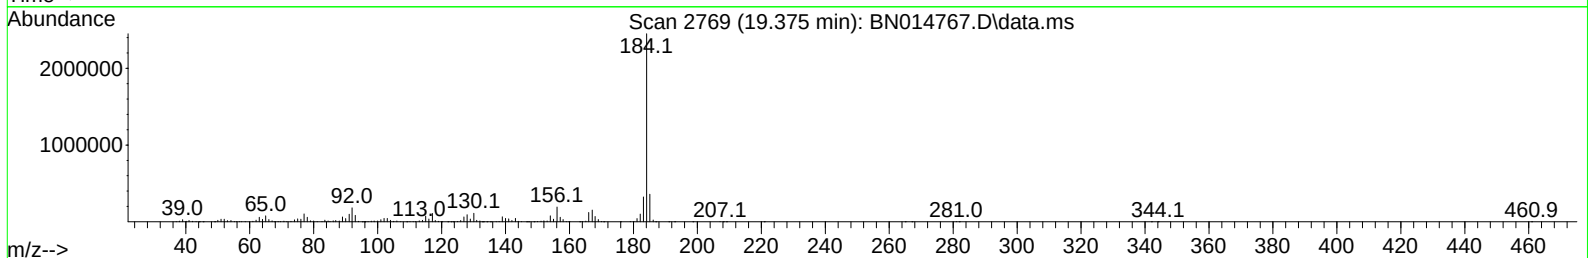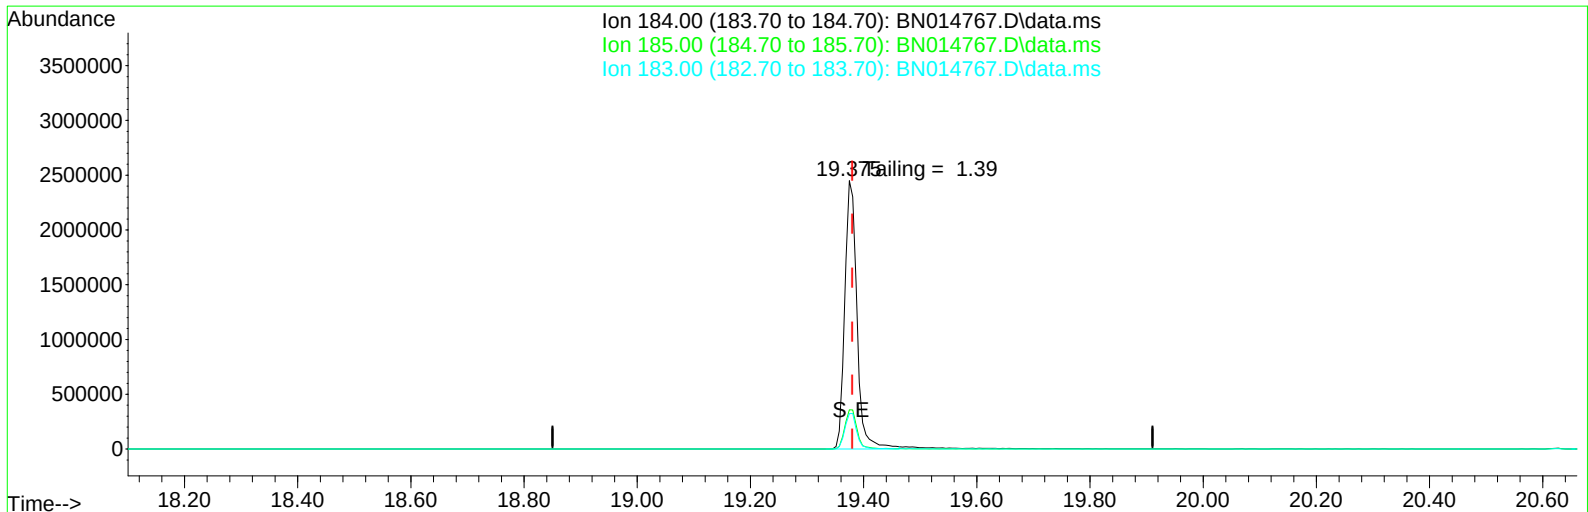

TIC: BN014767.D\data.ms

(77) Benzidine

19.375min (-0.005) 1096752.87 ng




response 3651244

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.63
183.00	13.20	13.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052621\
Data File : BN014767.D
Acq On : 26 May 2021 15:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 26 16:21:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

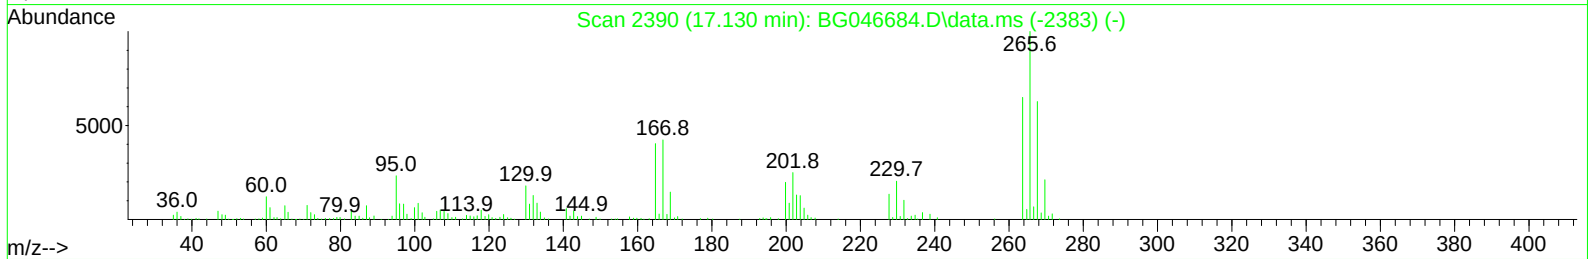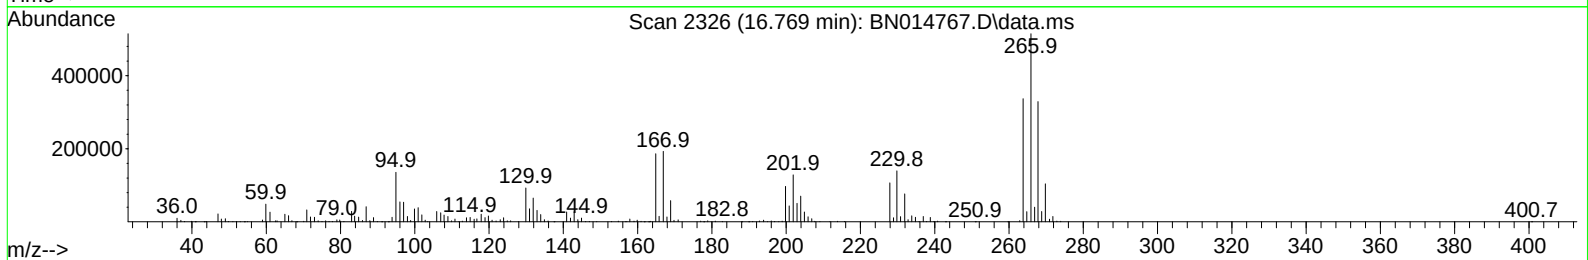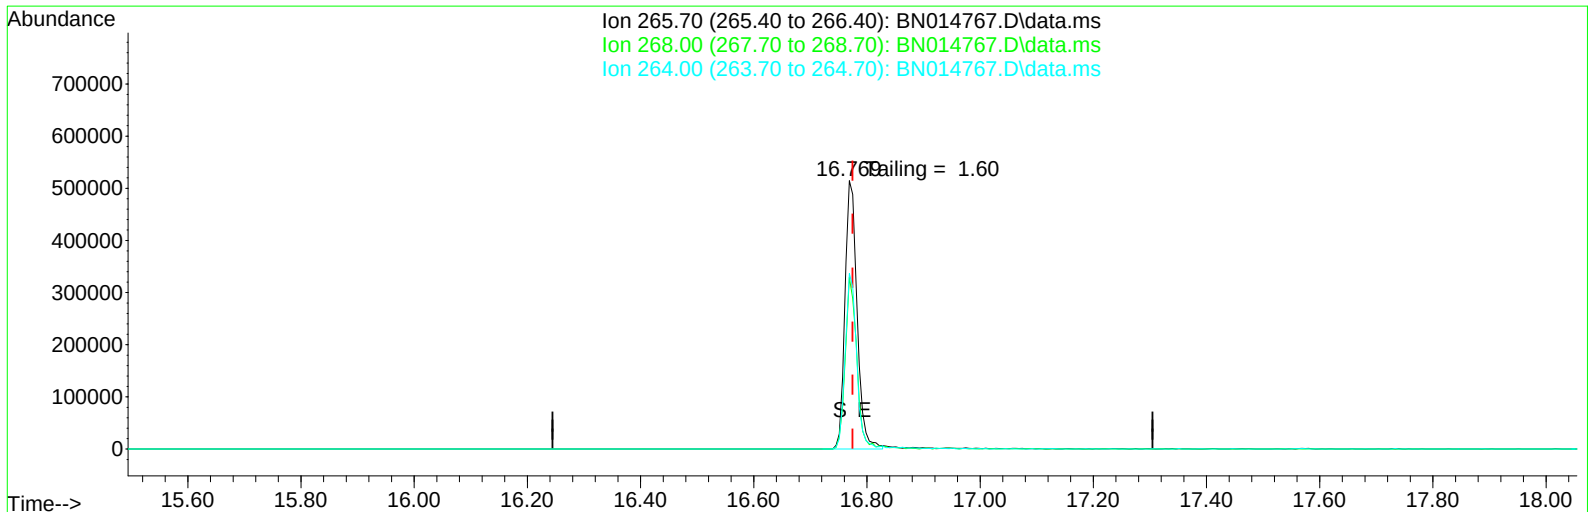

TIC: BN014767.D\data.ms

(70) Pentachlorophenol (C)

16.769min (-0.005) 17237.26 ng

response 772142

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.91
264.00	61.60	65.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/26/2021	BNA_N	<u>BN014767.D</u>
Compound Name	Response	Retention Time
DDT	2186551	20.62
DDD	85920	20.17
DDE	8112	19.66
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
94032	2280583	4.12