
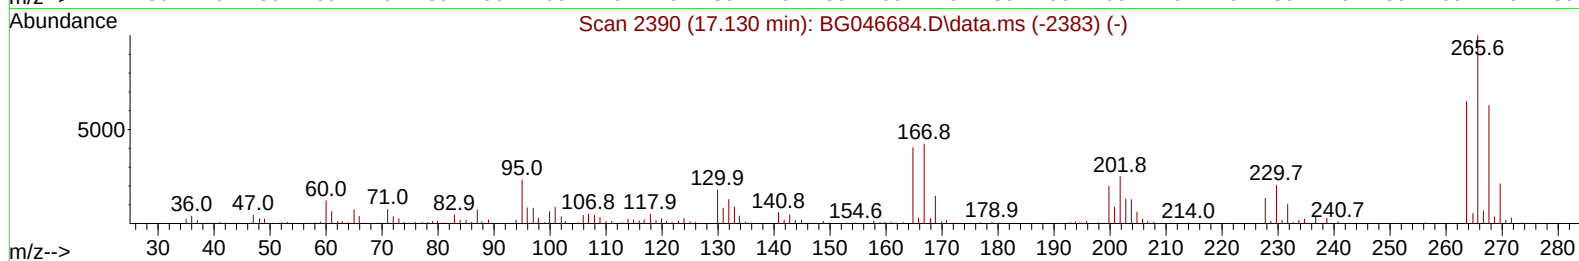
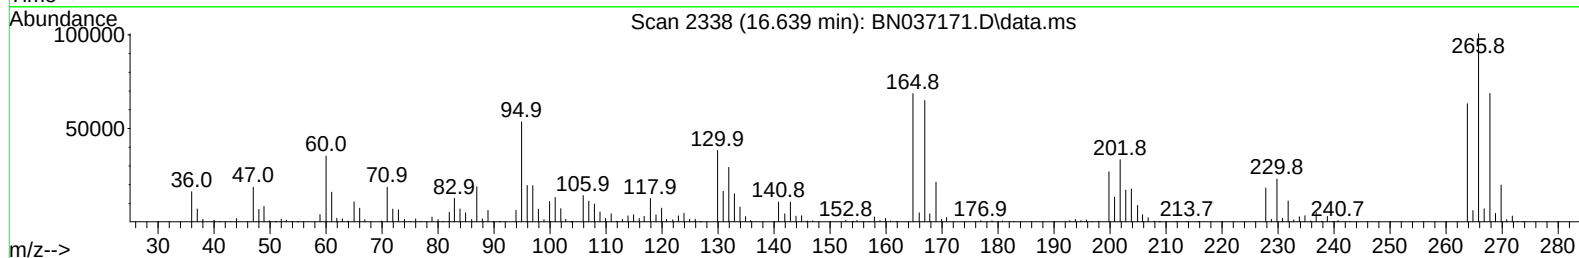


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060525\
Data File : BN037171.D
Acq On : 05 Jun 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 19:08:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:36:29 2025
Response via : Initial Calibration

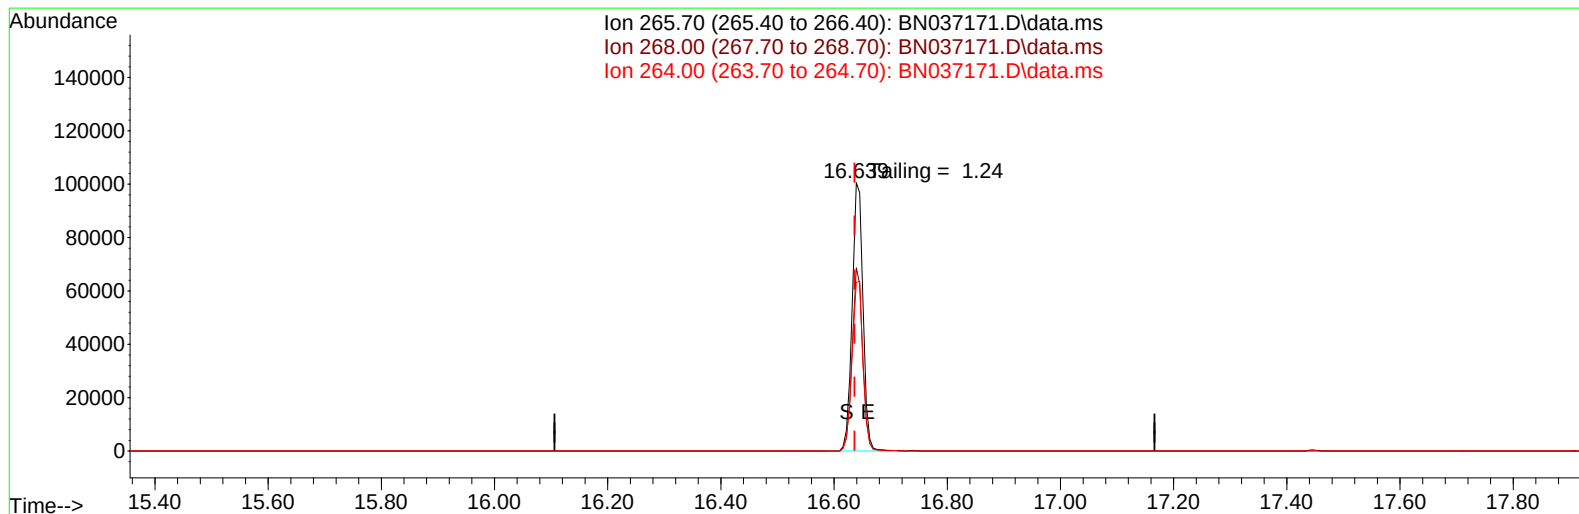

TIC: BN037171.D\data.ms

(70) Pentachlorophenol (C)




16.639min (+ 0.003) 18579.66 ng

response 133998

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.28
264.00	61.60	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060525\
Data File : BN037171.D
Acq On : 05 Jun 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 19:10:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:36:29 2025
Response via : Initial Calibration

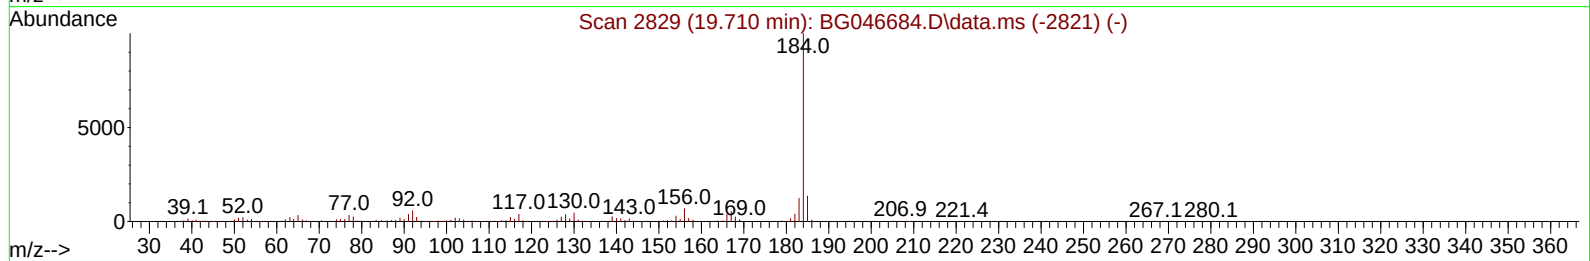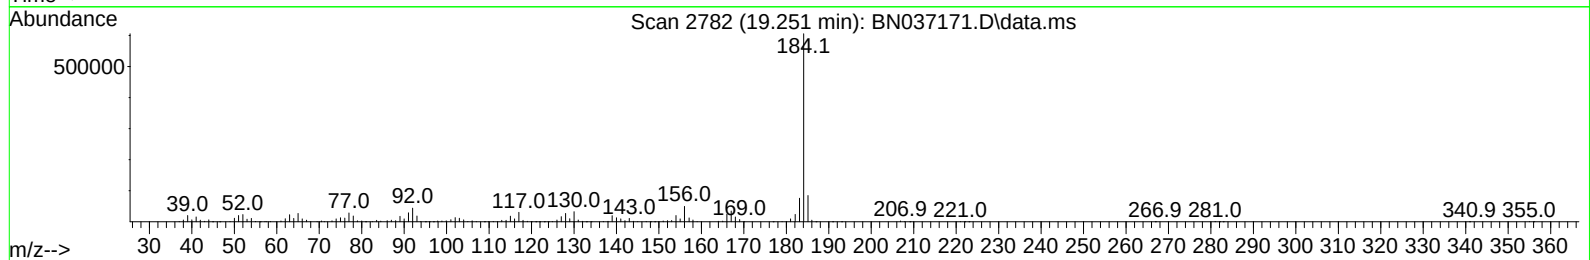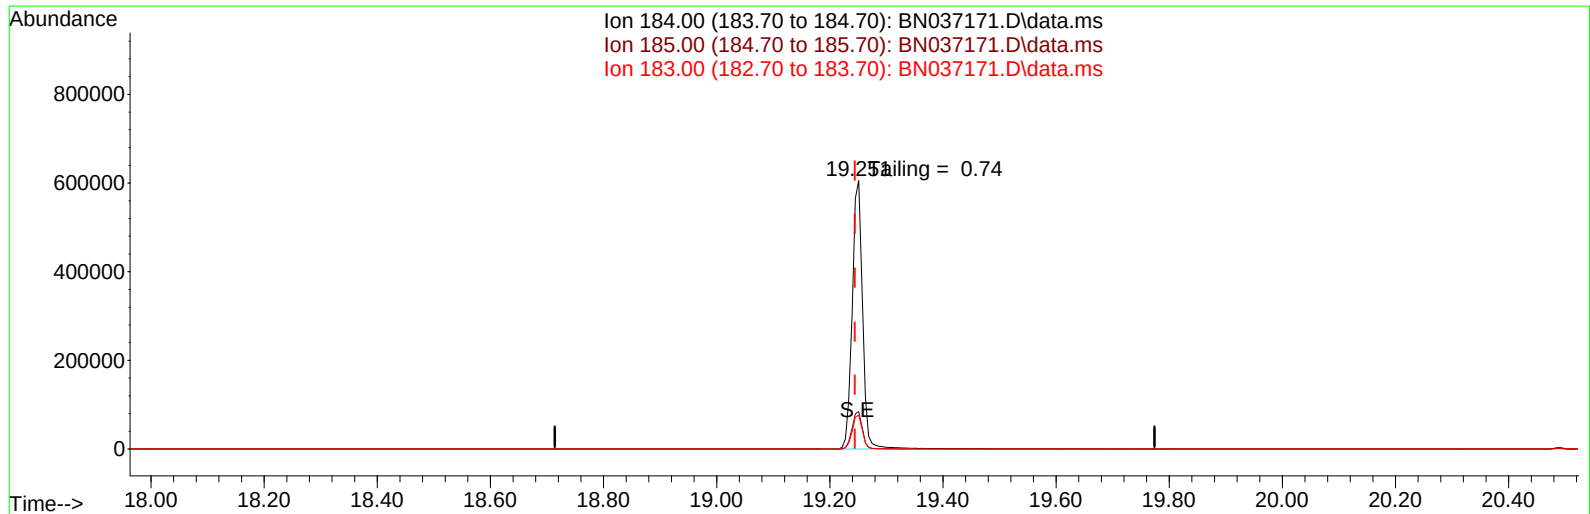

TIC: BN037171.D\data.ms

(77) Benzidine

19.251min (+ 0.007) 0.00 ng

response 772403

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.95
183.00	13.20	12.58
0.00	0.00	0.00