

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060525\
 Data File : BN037181.D
 Acq On : 05 Jun 2025 15:08
 Operator : RC/JU
 Sample : Q2200-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW-11B-37.5-060325

Quant Time: Jun 05 15:42:26 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN060325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 04 01:52:03 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.589	152	2014	0.400	ng	0.00
7) Naphthalene-d8	10.372	136	5256	0.400	ng	0.00
13) Acenaphthene-d10	14.235	164	2798	0.400	ng	0.00
19) Phenanthrene-d10	16.984	188	4922	0.400	ng	0.00
29) Chrysene-d12	21.189	240	3314	0.400	ng	# 0.00
35) Perylene-d12	23.377	264	3148	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.192	112	778	0.156	ng	0.00
5) Phenol-d6	6.773	99	531	0.088	ng	0.00
8) Nitrobenzene-d5	8.739	82	1803	0.325	ng	0.00
11) 2-Methylnaphthalene-d10	11.966	152	2201	0.301	ng	0.00
14) 2,4,6-Tribromophenol	15.730	330	423	0.375	ng	-0.01
15) 2-Fluorobiphenyl	12.858	172	3823	0.320	ng	0.00
27) Fluoranthene-d10	19.022	212	4519	0.361	ng	0.00
31) Terphenyl-d14	19.630	244	3411	0.437	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.119	88	57659	21.478	ng	98
34) Bis(2-ethylhexyl)phtha...	21.117	149	2890	0.382	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060525\
Data File : BN037181.D
Acq On : 05 Jun 2025 15:08
Operator : RC/JU
Sample : Q2200-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW-11B-37.5-060325


Quant Time: Jun 05 15:42:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN060325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 01:52:03 2025
Response via : Initial Calibration

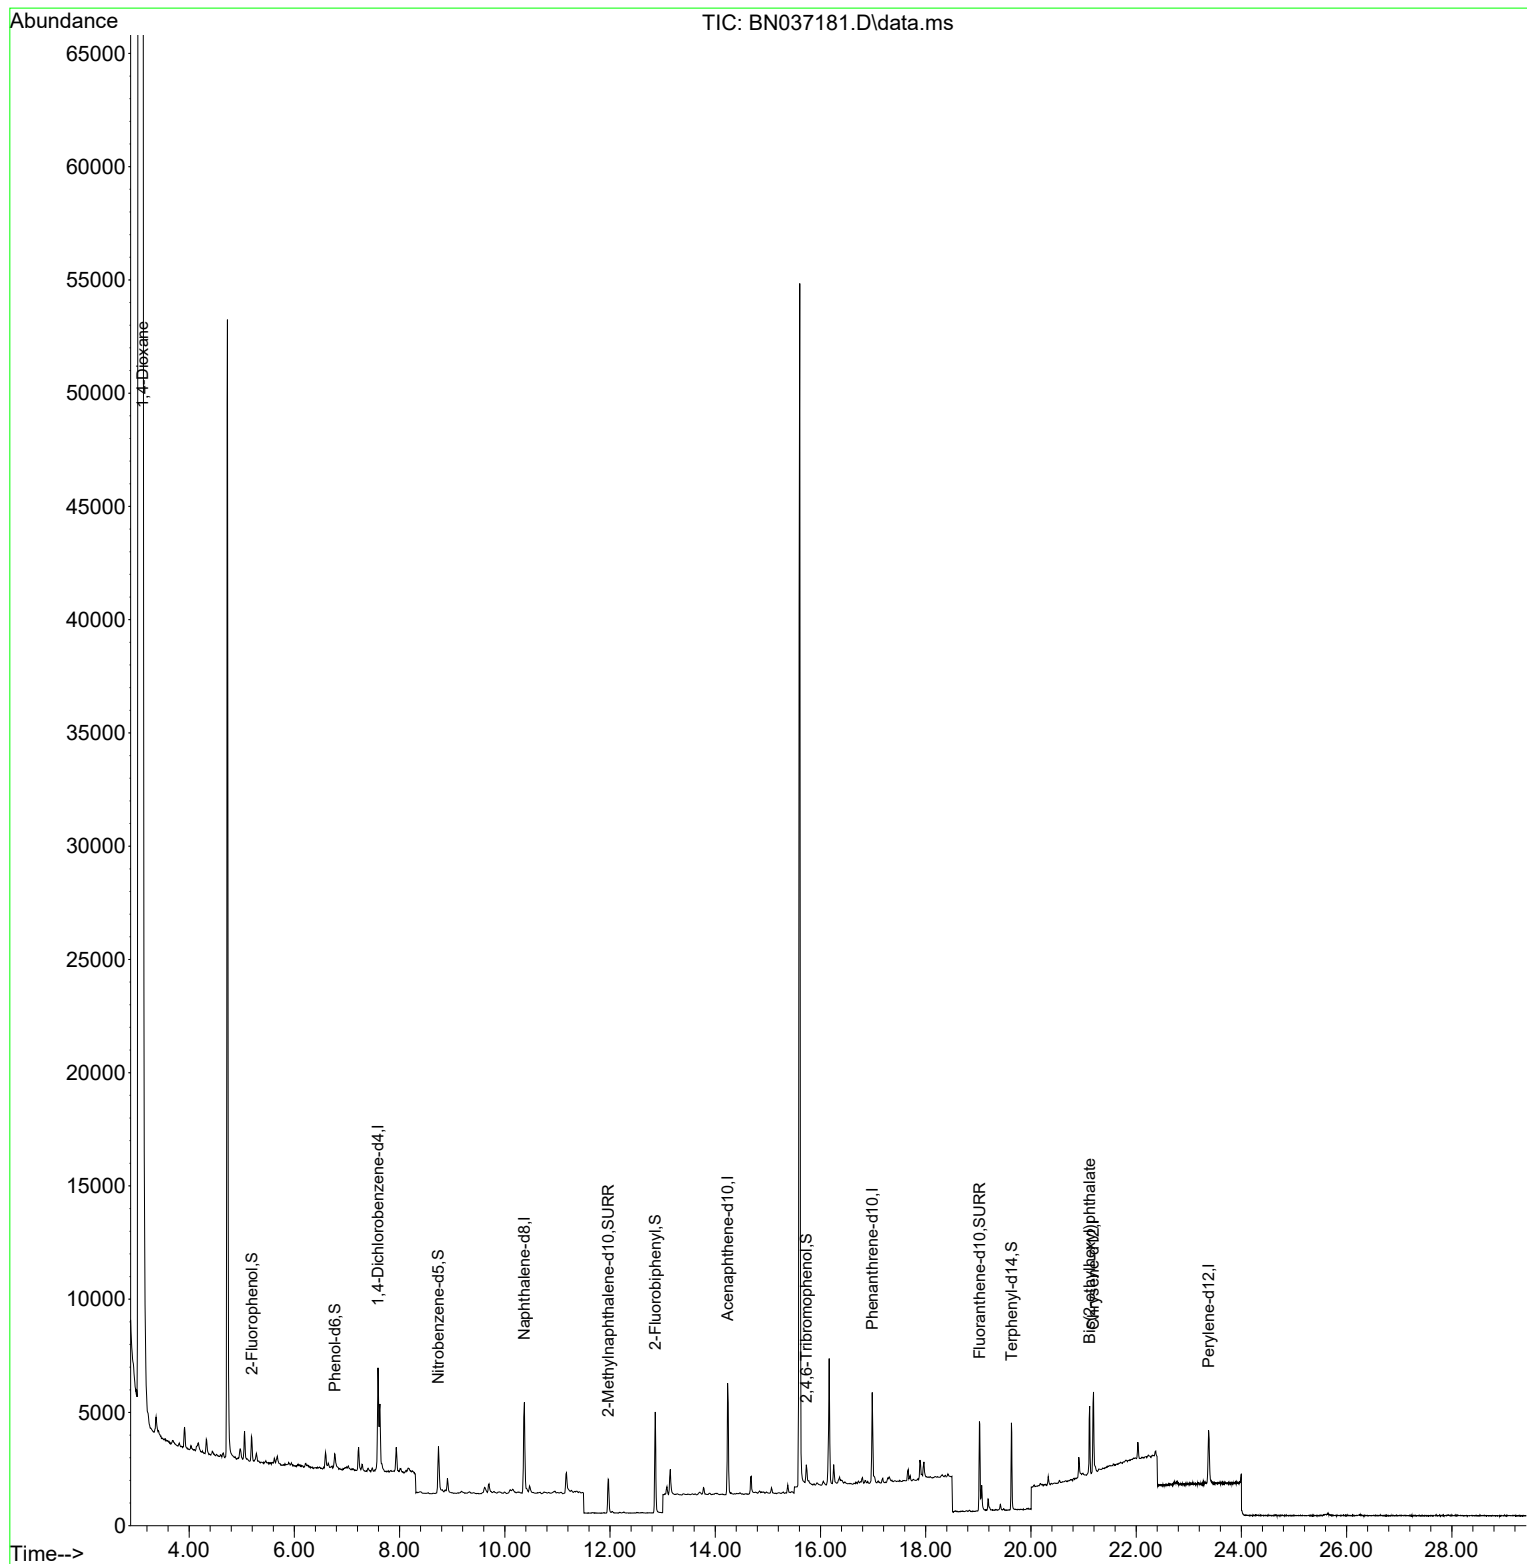






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.589 min Scan# 61
 Delta R.T. -0.001 min
 Lab File: BN037181.D
 Acq: 05 Jun 2025 15:08

Instrument :
 BNA_N
 ClientSampleId :
 MW-11B-37.5-060325

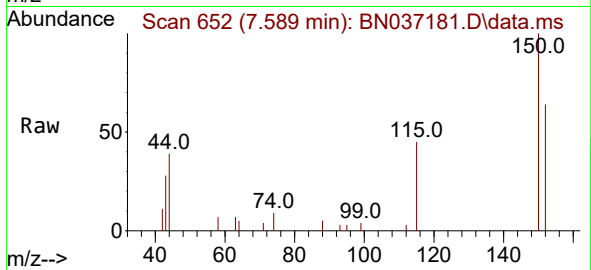

Tgt Ion:152 Resp: 2014




Ion	Ratio	Lower	Upper
152	100		
150	157.3	123.2	184.8
115	70.7	56.6	85.0

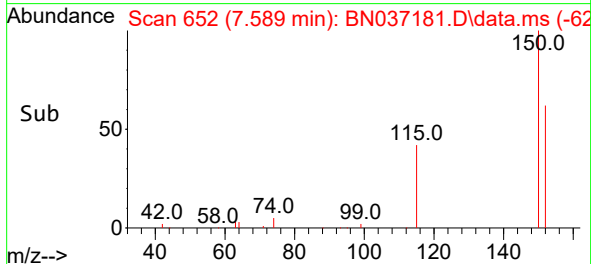


#2
 1,4-Dioxane
 Concen: 21.478 ng
 RT: 3.119 min Scan# 33
 Delta R.T. -0.007 min
 Lab File: BN037181.D
 Acq: 05 Jun 2025 15:08

Tgt Ion: 88 Resp: 57659

Ion	Ratio	Lower	Upper
88	100		
43	52.9	43.5	65.3
58	85.7	67.7	101.5


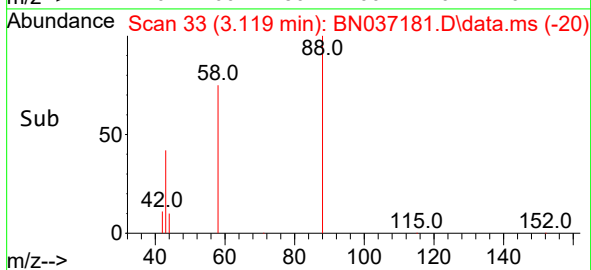

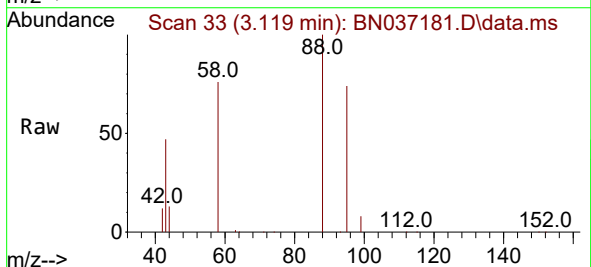




#4
2-Fluorophenol
Concen: 0.156 ng
RT: 5.192 min Scan# 319
Delta R.T. 0.007 min
Lab File: BN037181.D
Acq: 05 Jun 2025 15:08




Instrument :
BNA_N
ClientSampleId :
MW-11B-37.5-060325


Tgt Ion:112 Resp: 778
Ion Ratio Lower Upper
112 100
64 67.6 56.3 84.5
63 41.9 36.2 54.4

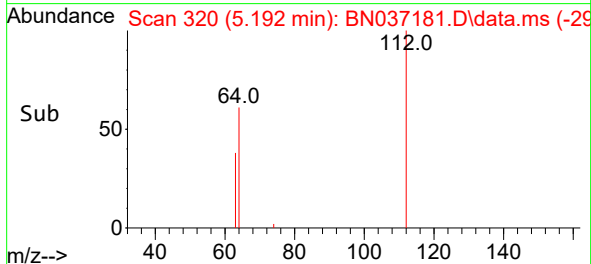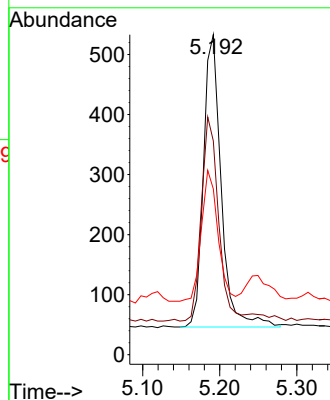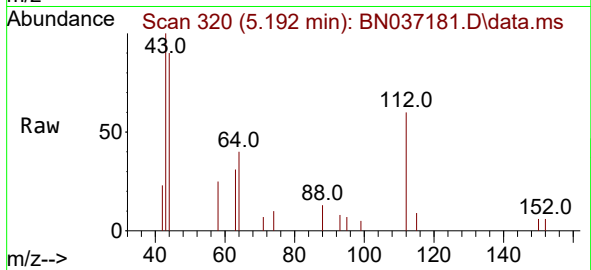

#5
Phenol-d6
Concen: 0.088 ng
RT: 6.773 min Scan# 539
Delta R.T. -0.000 min
Lab File: BN037181.D
Acq: 05 Jun 2025 15:08

Tgt Ion: 99 Resp: 531
Ion Ratio Lower Upper
99 100
42 48.2 31.3 46.9#
71 55.2 38.2 57.2



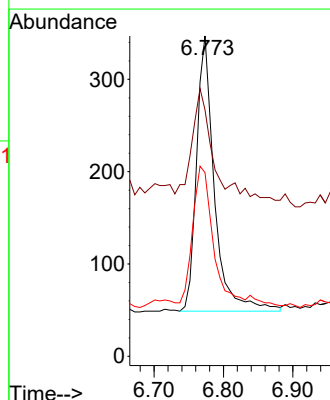
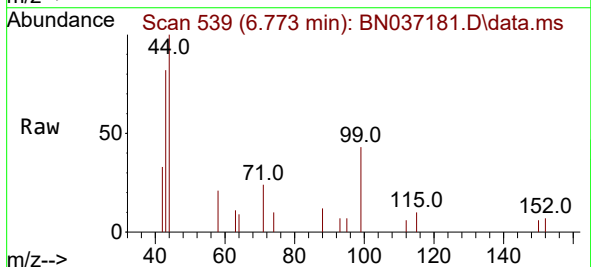


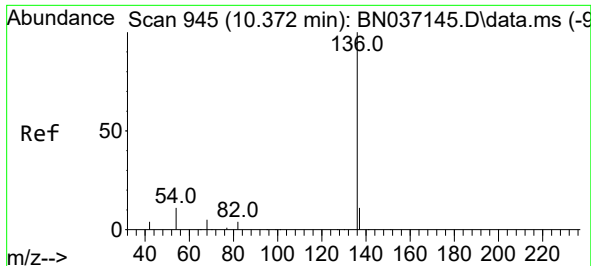

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.372 min Scan# 945
Delta R.T. -0.000 min
Lab File: BN037181.D
Acq: 05 Jun 2025 15:08




Instrument :
BNA_N
ClientSampleId :
MW-11B-37.5-060325


Tgt Ion:	136	Resp:	5256
Ion	Ratio	Lower	Upper
136	100		
137	12.0	9.7	14.5
54	11.4	9.7	14.5
68	6.2	5.4	8.2

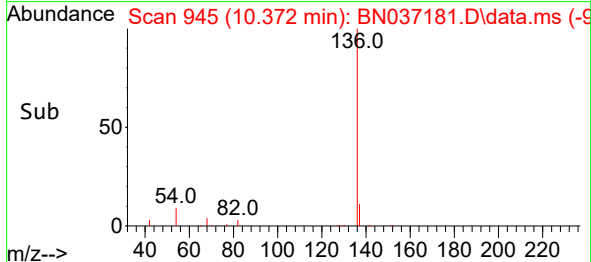

#8
Nitrobenzene-d5
Concen: 0.325 ng
RT: 8.739 min Scan# 792
Delta R.T. -0.000 min
Lab File: BN037181.D
Acq: 05 Jun 2025 15:08

Tgt Ion:	82	Resp:	1803
Ion	Ratio	Lower	Upper
82	100		
128	34.3	26.9	40.3
54	72.2	61.4	92.2


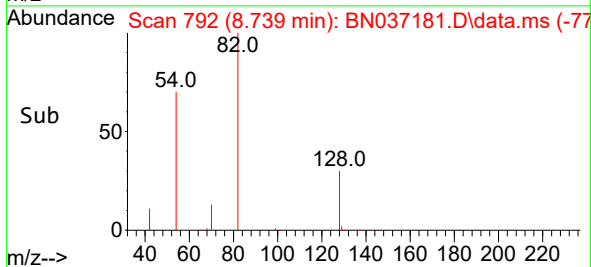

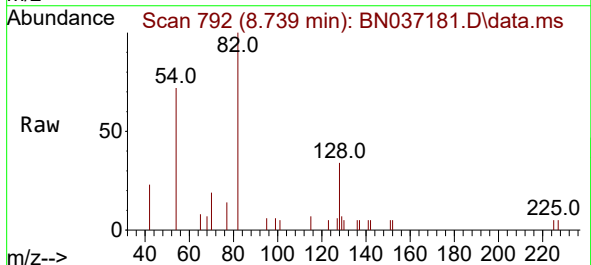


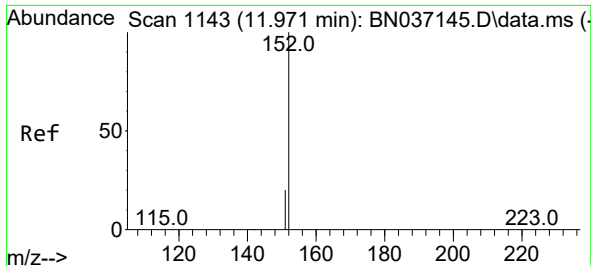

#11
2-Methylnaphthalene-d10
Concen: 0.301 ng
RT: 11.966 min Scan# 1142
Delta R.T. -0.005 min
Lab File: BN037181.D
Acq: 05 Jun 2025 15:08




Instrument :
BNA_N
ClientSampleId :
MW-11B-37.5-060325


Tgt Ion:152 Resp: 2201
Ion Ratio Lower Upper
152 100
151 21.6 17.1 25.7

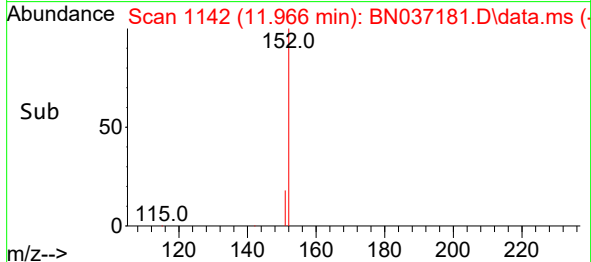

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.235 min Scan# 1462
Delta R.T. -0.000 min
Lab File: BN037181.D
Acq: 05 Jun 2025 15:08

Tgt Ion:164 Resp: 2798
Ion Ratio Lower Upper
164 100
162 106.1 85.5 128.3
160 56.2 44.6 67.0


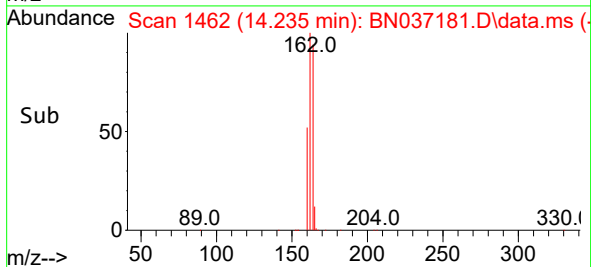

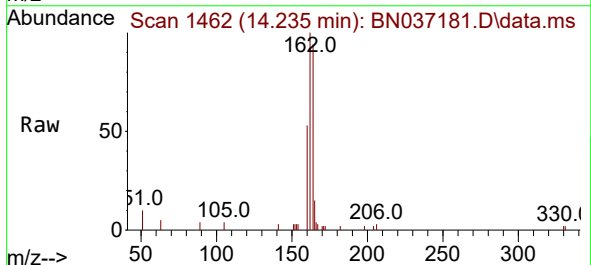


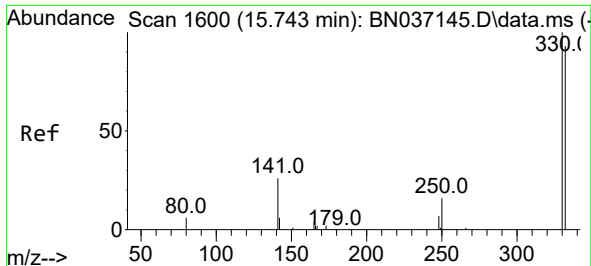

#14
2,4,6-Tribromophenol
Concen: 0.375 ng
RT: 15.730 min Scan# 11
Delta R.T. -0.012 min
Lab File: BN037181.D
Acq: 05 Jun 2025 15:08




Instrument :
BNA_N
ClientSampleId :
MW-11B-37.5-060325


Tgt Ion:330 Resp: 423
Ion Ratio Lower Upper
330 100
332 93.9 77.1 115.7
141 68.6 46.4 69.6

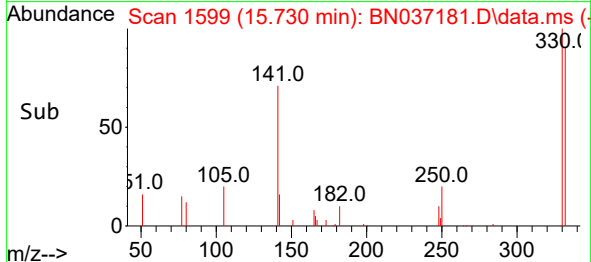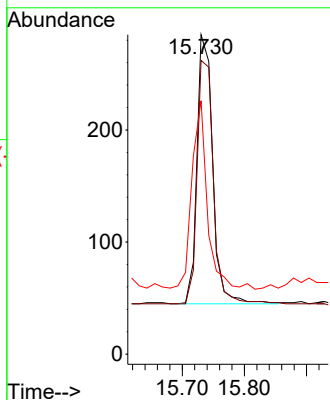

#15
2-Fluorobiphenyl
Concen: 0.320 ng
RT: 12.858 min Scan# 1318
Delta R.T. -0.005 min
Lab File: BN037181.D
Acq: 05 Jun 2025 15:08

Tgt Ion:172 Resp: 3823
Ion Ratio Lower Upper
172 100
171 36.6 29.6 44.4
170 26.0 20.3 30.5


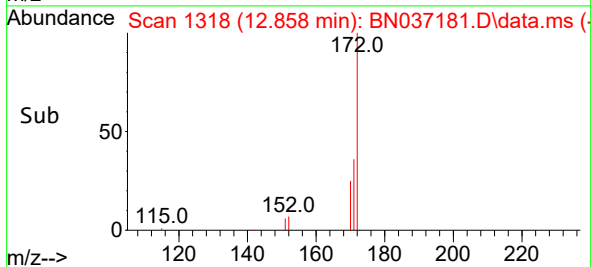
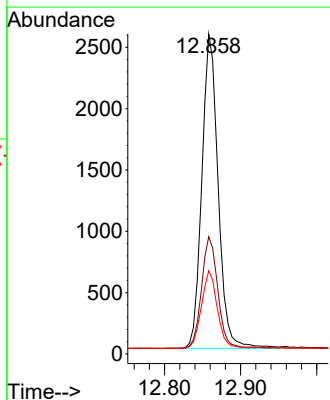
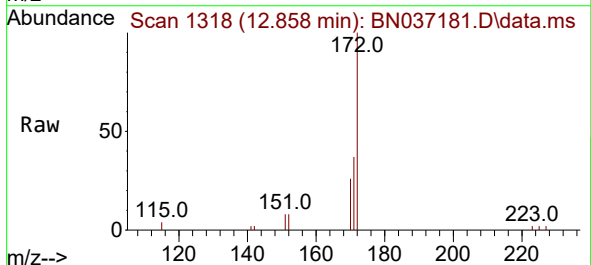


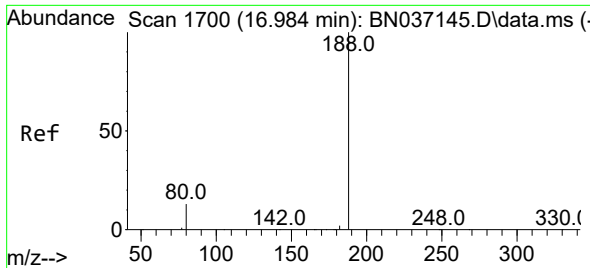

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.984 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN037181.D
Acq: 05 Jun 2025 15:08




Instrument :
BNA_N
ClientSampleId :
MW-11B-37.5-060325


Tgt Ion:188 Resp: 4922
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 14.3 11.3 16.9

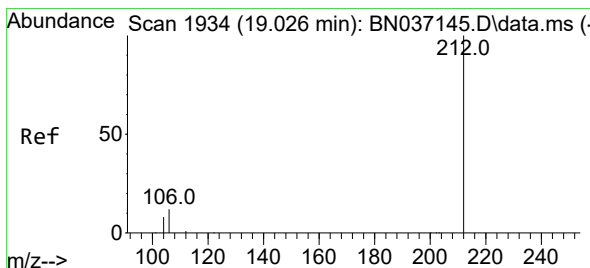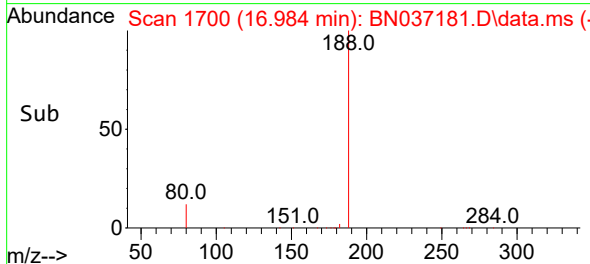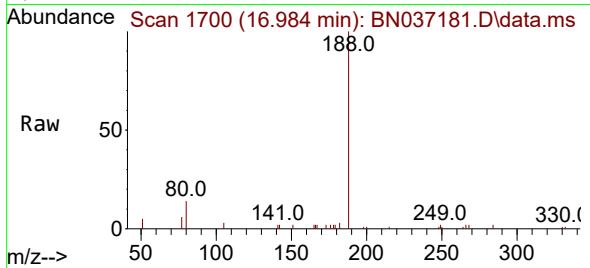

#27
Fluoranthene-d10
Concen: 0.361 ng
RT: 19.022 min Scan# 1933
Delta R.T. -0.005 min
Lab File: BN037181.D
Acq: 05 Jun 2025 15:08

Tgt Ion:212 Resp: 4519
Ion Ratio Lower Upper
212 100
106 13.5 10.6 15.8
104 8.4 6.6 9.8


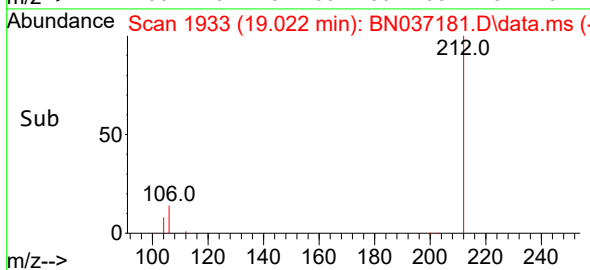

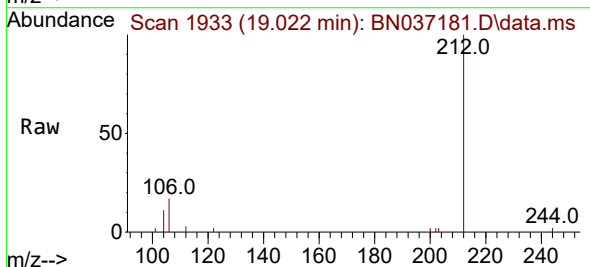




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.189 min Scan# 2118
Delta R.T. -0.000 min
Lab File: BN037181.D
Acq: 05 Jun 2025 15:08




Instrument :
BNA_N
ClientSampleId :
MW-11B-37.5-060325


Tgt Ion:240 Resp: 3314
Ion Ratio Lower Upper
240 100
120 13.8 9.0 13.4#
236 29.8 23.0 34.4

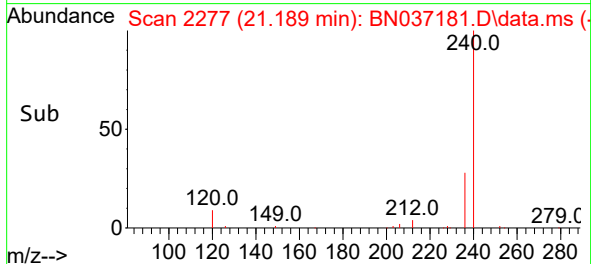

#31
Terphenyl-d14
Concen: 0.437 ng
RT: 19.630 min Scan# 2064
Delta R.T. -0.005 min
Lab File: BN037181.D
Acq: 05 Jun 2025 15:08

Tgt Ion:244 Resp: 3411
Ion Ratio Lower Upper
244 100
212 12.4 10.0 15.0
122 18.2 13.2 19.8


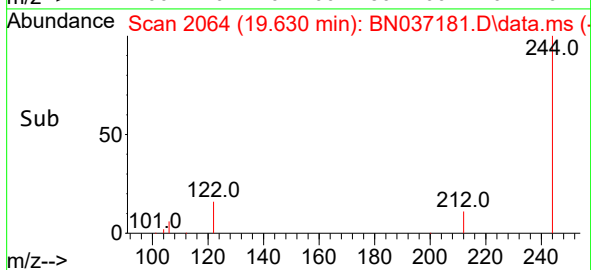

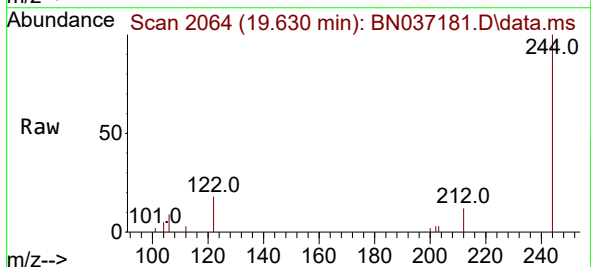


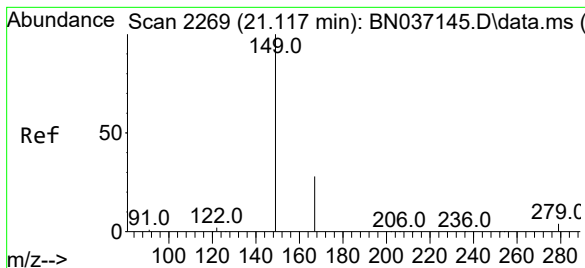

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.382 ng
 RT: 21.117 min Scan# 2117
 Delta R.T. -0.000 min
 Lab File: BN037181.D
 Acq: 05 Jun 2025 15:08

Instrument :
 BNA_N
 ClientSampleId :
 MW-11B-37.5-060325

Tgt Ion:149 Resp: 2890
 Ion Ratio Lower Upper
 149 100
 167 25.0 21.0 31.4
 279 2.9 2.9 4.3

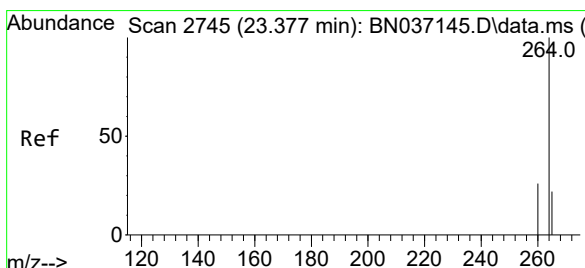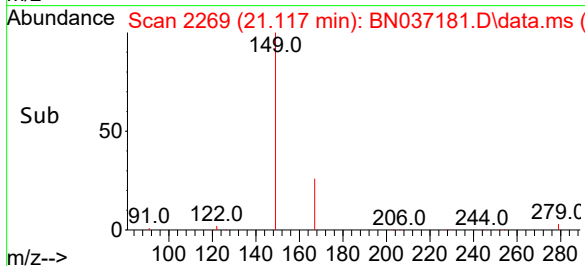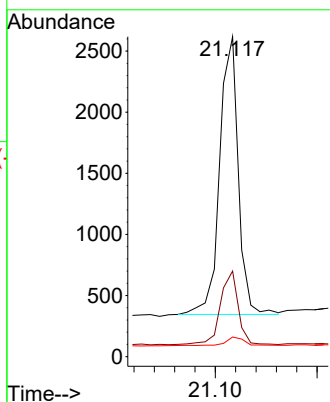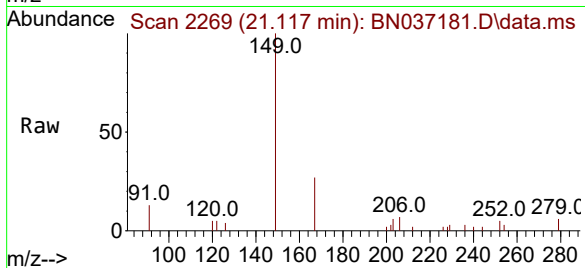

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.377 min Scan# 2745
 Delta R.T. -0.000 min
 Lab File: BN037181.D
 Acq: 05 Jun 2025 15:08

Tgt Ion:264 Resp: 3148
 Ion Ratio Lower Upper
 264 100
 260 28.1 22.1 33.1
 265 76.8 55.8 83.8

