
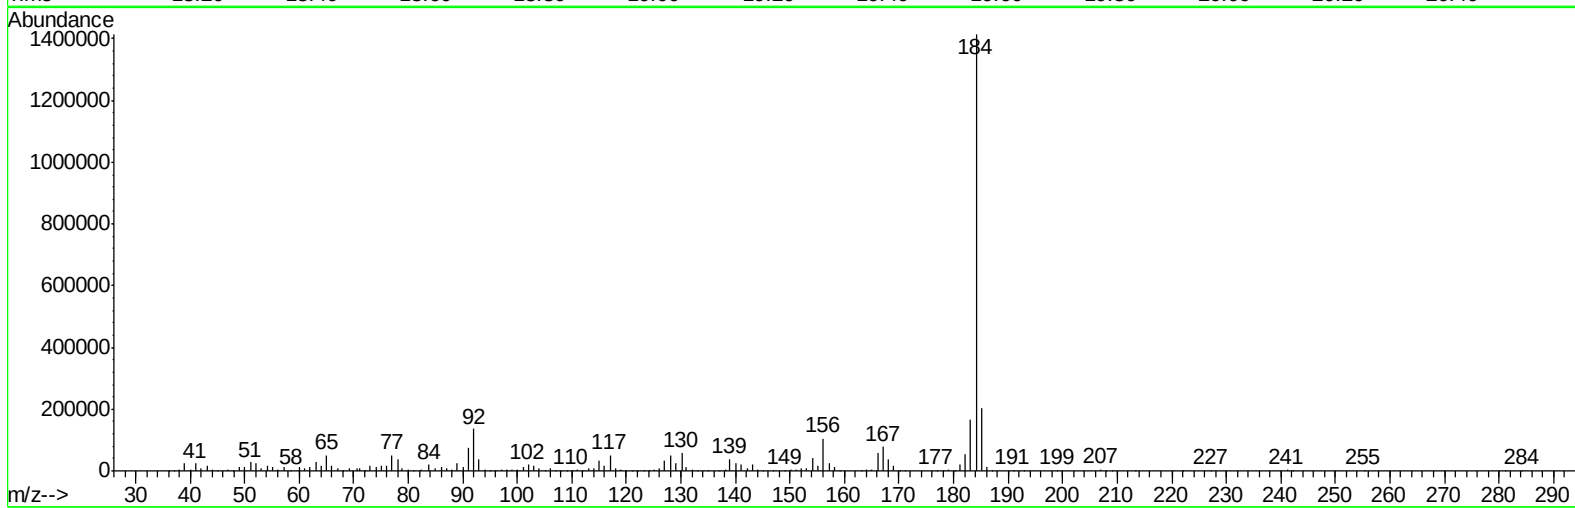


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN070219\
 Data File : BN006687.D
 Acq On : 02 Jul 2019 11:17
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 09:34:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 05:27:09 2019
 Response via : Initial Calibration

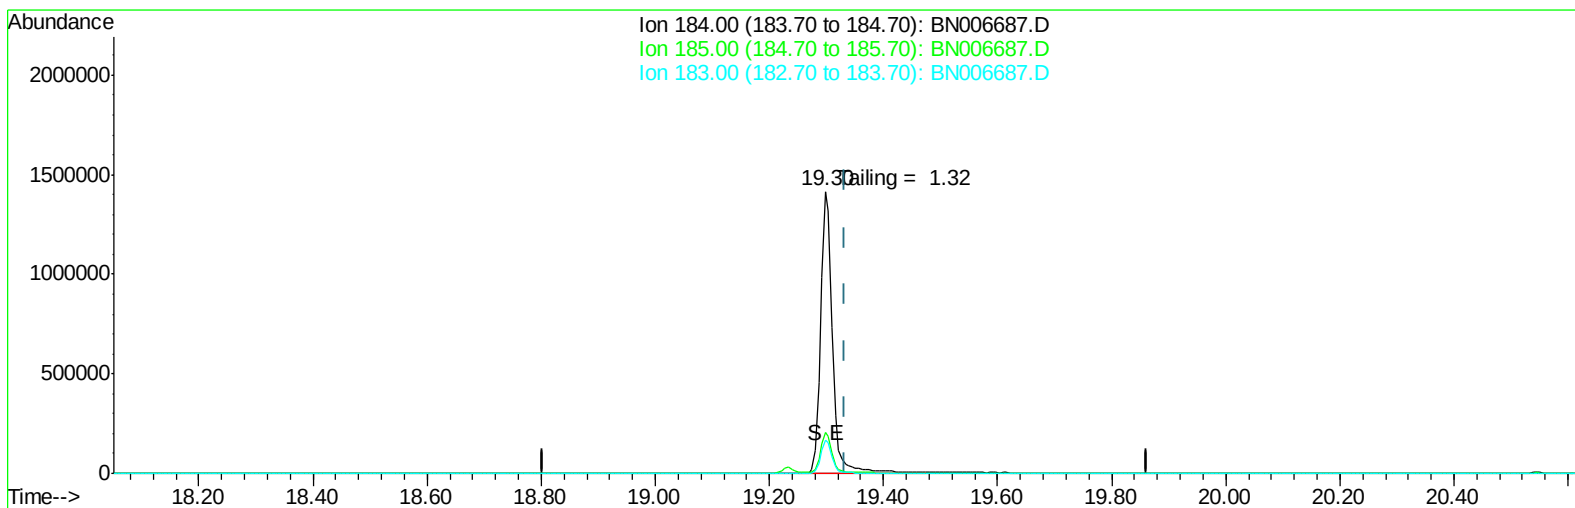

TIC: BN006687.D

(77) Benzidine



19.298min (-0.035) 146390.85ng

response 2107748

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.34
183.00	12.40	11.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN070219\
Data File : BN006687.D
Acq On : 02 Jul 2019 11:17
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 09:34:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 05:27:09 2019
Response via : Initial Calibration

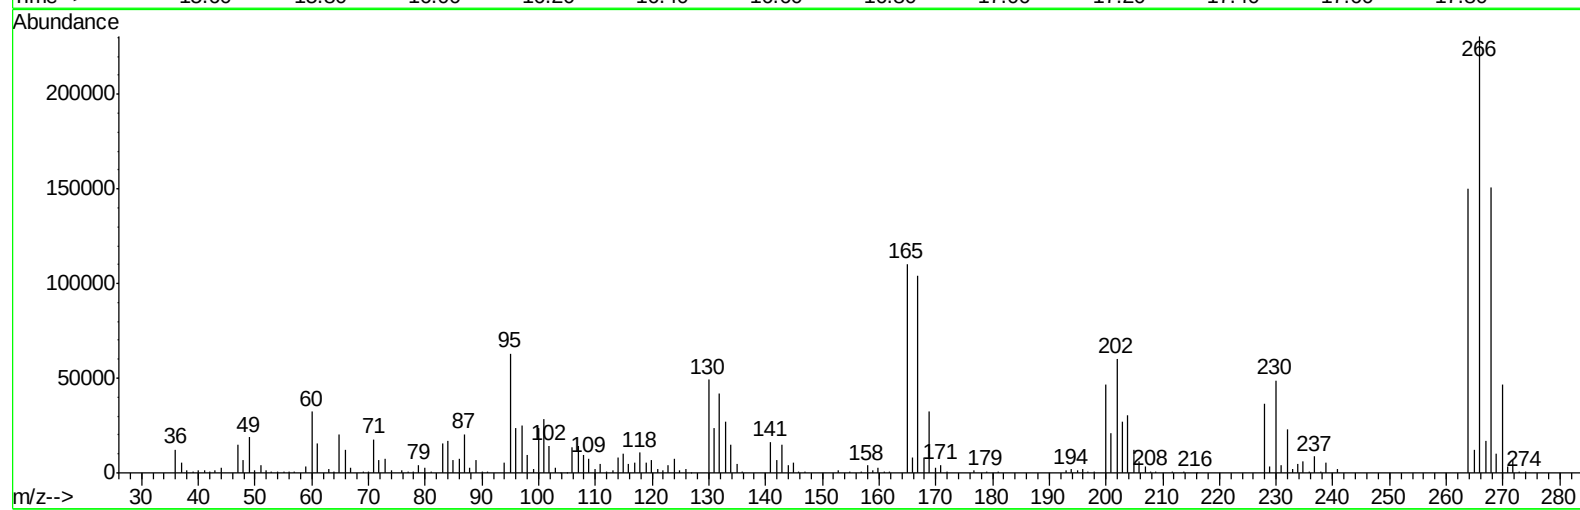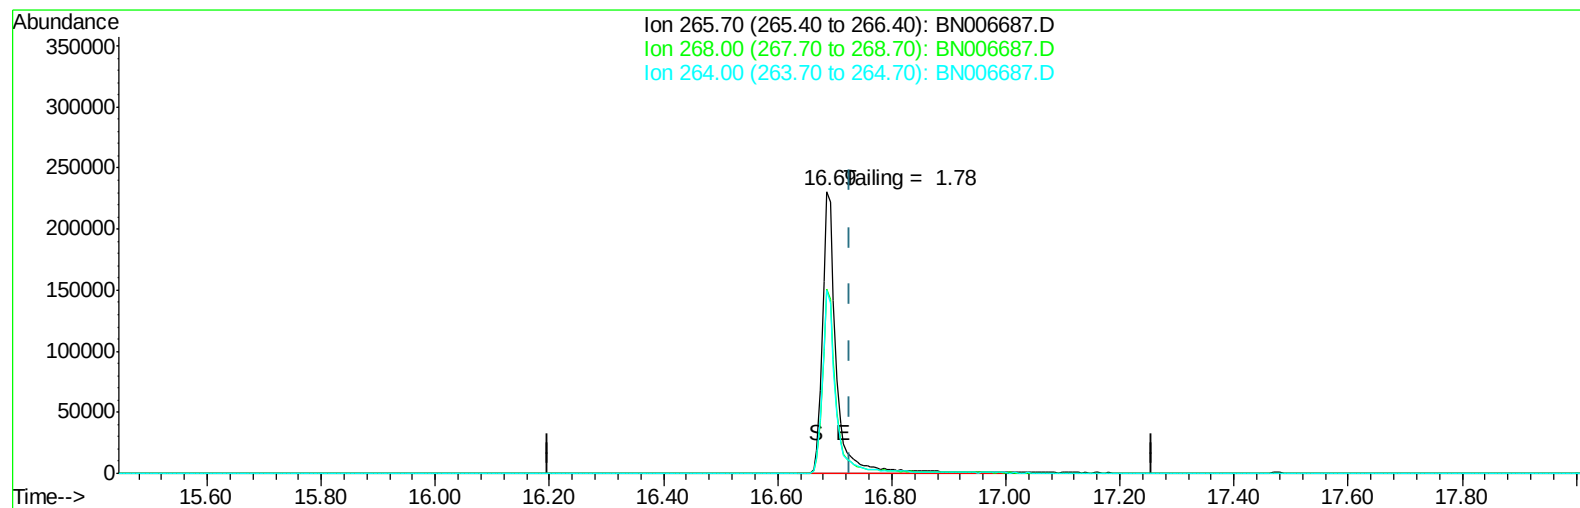

TIC: BN006687.D

(70) Pentachlorophenol (C)

16.686min (-0.041) 29958.06ng

response 398852

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	65.27
264.00	62.50	65.05
0.00	0.00	0.00