


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN070219\
 Data File : BN006687.D
 Acq On : 02 Jul 2019 11:17
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN070219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 02 17:43:33 2019

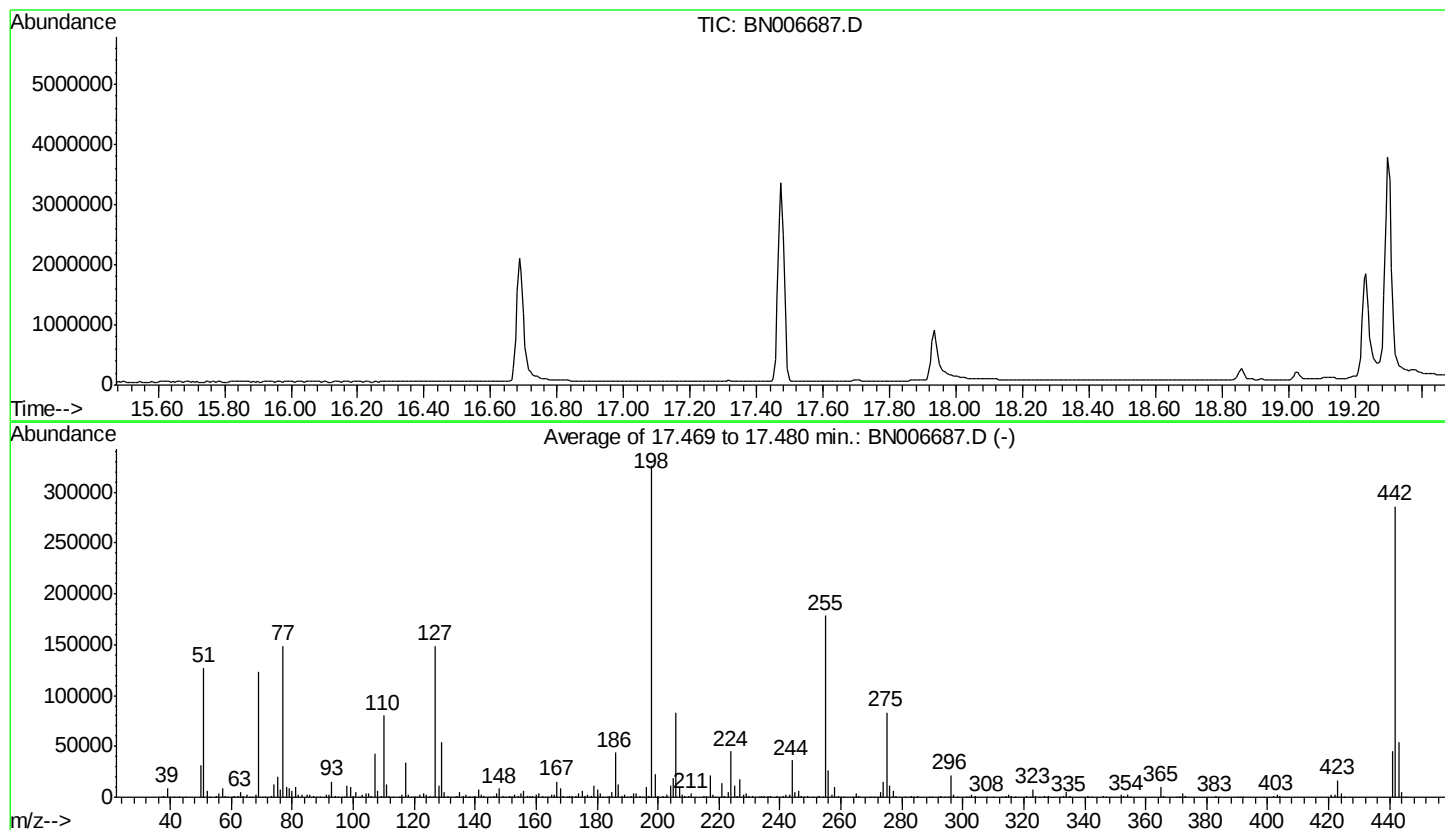

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	127623	PASS
68	69	0.00	2	1.8	2222	PASS
69	198	0.00	100	37.7	122845	PASS
70	69	0.00	2	0.5	600	PASS
127	198	10	80	45.6	148845	PASS
197	198	0.00	2	0.5	1552	PASS
198	198	100	100	100.0	326186	PASS
199	198	5	9	6.9	22365	PASS
275	198	10	60	25.6	83586	PASS
365	198	1	100	3.2	10355	PASS
441	198	0.01	100	13.8	44869	PASS
442	198	50	100	87.7	285952	PASS
443	442	15	24	19.1	54642	PASS