


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN070819\
 Data File : BN006747.D
 Acq On : 08 Jul 2019 08:27
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN070219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 05 05:30:28 2019

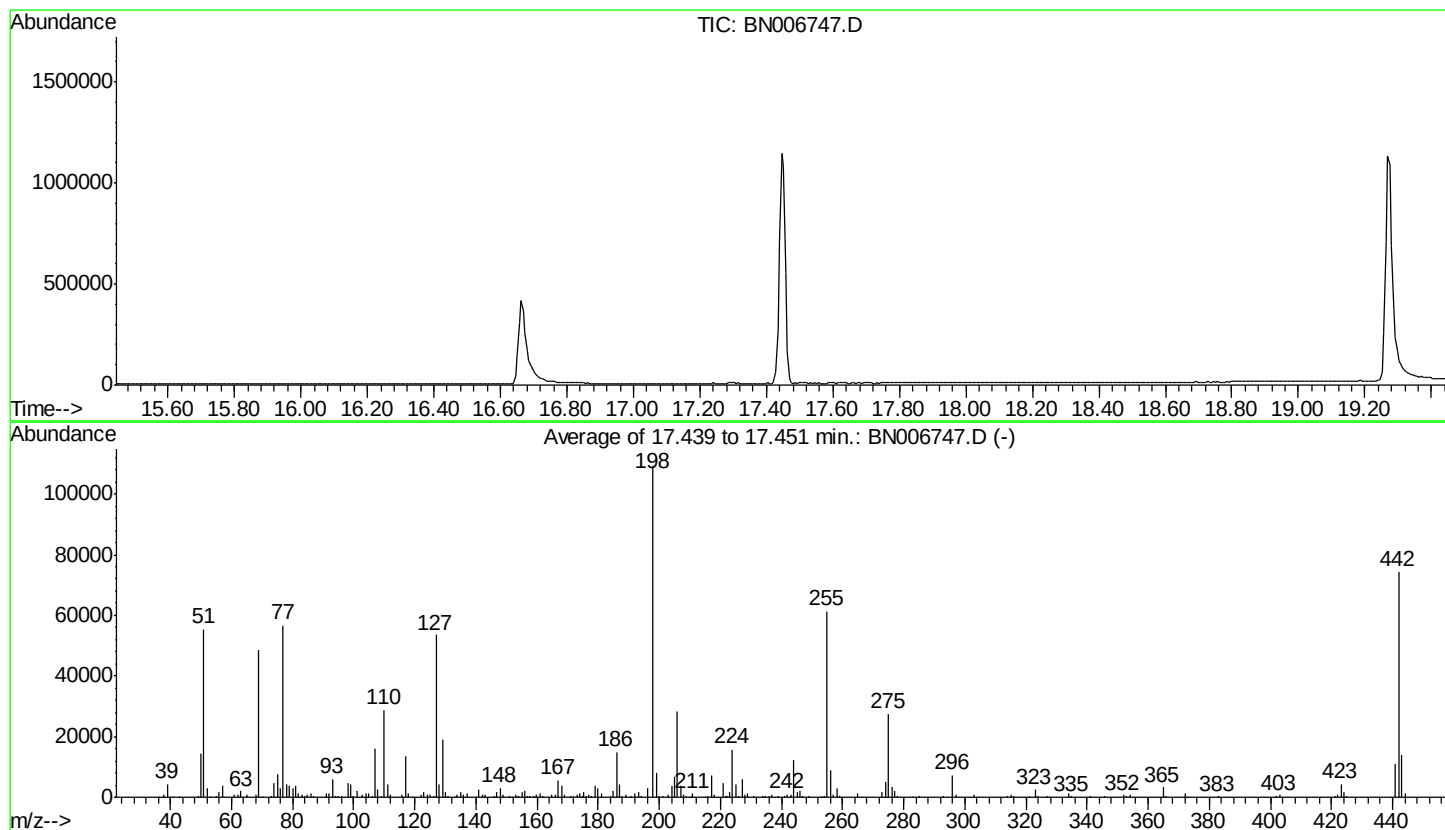

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.7	55453	PASS
68	69	0.00	2	1.4	685	PASS
69	198	0.00	100	44.6	48773	PASS
70	69	0.00	2	0.3	143	PASS
127	198	10	80	48.9	53522	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109368	PASS
199	198	5	9	7.2	7847	PASS
275	198	10	60	25.2	27514	PASS
365	198	1	100	3.1	3357	PASS
441	198	0.01	100	10.1	11012	PASS
442	198	50	100	68.0	74400	PASS
443	442	15	24	18.7	13898	PASS