

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080421\
 Data File : BN015792.D
 Acq On : 04 Aug 2021 14:13
 Operator : CG/JU
 Sample : M1458-08
 Misc : LOQ-WATER-0.2ng
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 LOQ-WATER-02-QT1-2021

Manual Integrations
 APPROVED

mohammad
 8/5/2021 5:07:34 PM

Quant Time: Aug 05 10:47:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 05 10:46:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.790	152	41129	0.400	ng	0.00
7) Naphthalene-d8	10.571	136	184302	0.400	ng	0.00
13) Acenaphthene-d10	14.408	164	96208	0.400	ng	0.00
19) Phenanthrene-d10	17.163	188	180470	0.400	ng	0.00
29) Chrysene-d12	21.365	240	160942	0.400	ng	0.00
35) Perylene-d12	23.710	264	156041	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.383	112	29709	0.295	ng	0.00
5) Phenol-d6	6.951	99	34791	0.286	ng	0.00
8) Nitrobenzene-d5	8.924	82	29132	0.246	ng	0.00
11) 2-Methylnaphthalene-d10	12.158	152	105308	0.380	ng	0.00
14) 2,4,6-Tribromophenol	15.905	330	8006	0.230	ng	0.00
15) 2-Fluorobiphenyl	13.038	172	100586	0.262	ng	0.00
27) Fluoranthene-d10	19.202	212	172774	0.368	ng	0.00
31) Terphenyl-d14	19.807	244	107322	0.269	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.354	88	2050	0.154	ng	# 35
3) n-Nitrosodimethylamine	3.723	42	4740	0.173	ng	# 97
6) bis(2-Chloroethyl)ether	7.218	93	23923	0.217	ng	99
9) Naphthalene	10.609	128	98073	0.203	ng	99
10) Hexachlorobutadiene	10.913	225	16582	0.197	ng	# 100
12) 2-Methylnaphthalene	12.234	142	64374	0.207	ng	99
16) Acenaphthylene	14.129	152	69672	0.176	ng	100
17) Acenaphthene	14.471	154	52393	0.189	ng	99
18) Fluorene	15.461	166	62932	0.190	ng	100
20) 4,6-Dinitro-2-methylph...	15.550	198	673	0.131	ng	# 70
21) 4-Bromophenyl-phenylether	16.360	248	19456	0.183	ng	92
22) Hexachlorobenzene	16.470	284	23721	0.195	ng	100
23) Atrazine	16.628	200	11427	0.175	ng	96
24) Pentachlorophenol	16.810	266	5500	0.146	ng	99
25) Phenanthrene	17.200	178	104083	0.194	ng	100
26) Anthracene	17.297	178	82648	0.183	ng	100
28) Fluoranthene	19.231	202	107489	0.192	ng	99
30) Pyrene	19.599	202	104051	0.194	ng	100
32) Benzo(a)anthracene	21.355	228	90893	0.185	ng	100
33) Chrysene	21.408	228	102670	0.193	ng	99
34) Bis(2-ethylhexyl)phtha...	21.301	149	30814	0.156	ng	99
36) Indeno(1,2,3-cd)pyrene	26.110	276	96737	0.175	ng	96
37) Benzo(b)fluoranthene	23.002	252	103115	0.190	ng	99
38) Benzo(k)fluoranthene	23.046	252	109787m	0.196	ng	
39) Benzo(a)pyrene	23.607	252	85719	0.190	ng	99
40) Dibenzo(a,h)anthracene	26.127	278	78276	0.169	ng	# 87
41) Benzo(g,h,i)perylene	26.839	276	84739	0.175	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080421\
Data File : BN015792.D
Acq On : 04 Aug 2021 14:13
Operator : CG/JU
Sample : M1458-08
Misc : LOQ-WATER-0.2ng
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021

Manual Integrations
APPROVED

mohammad
8/5/2021 5:07:34 PM


Quant Time: Aug 05 10:47:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 05 10:46:09 2021
Response via : Initial Calibration





#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.790 min Scan# 511
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021




Tgt Ion:152 Resp: 41129
Ion Ratio Lower Upper
152 100
150 154.5 123.5 185.3
115 58.7 46.8 70.2

Manual Integrations
APPROVED



mohammad
8/5/2021 5:07:34 PM




#2
1,4-Dioxane
Concen: 0.154 ng
RT: 3.354 min Scan# 30
Delta R.T. -0.001 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13



Tgt Ion: 88 Resp: 2050
Ion Ratio Lower Upper
88 100
43 28.5 23.1 34.7
58 0.0 62.2 93.4#



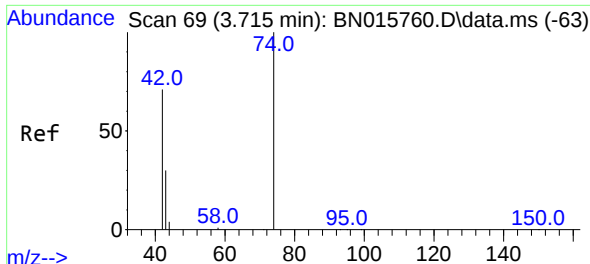





#3
n-Nitrosodimethylamine
Concen: 0.173 ng
RT: 3.723 min Scan# 70
Delta R.T. 0.009 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion: 42 Resp: 4740
Ion Ratio Lower Upper
42 100
74 146.2 114.4 171.6
44 9.6 3.6 5.4#

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021




Manual Integrations
APPROVED


mohammad
8/5/2021 5:07:34 PM




#4
2-Fluorophenol
Concen: 0.295 ng
RT: 5.383 min Scan# 250
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion: 112 Resp: 29709
Ion Ratio Lower Upper
112 100
64 53.2 42.2 63.4
63 28.0 22.2 33.2








#5
Phenol-d6
Concen: 0.286 ng
RT: 6.951 min Scan# 420
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13




Tgt Ion: 99 Resp: 34791

Ion	Ratio	Lower	Upper
99	100		
42	16.5	13.2	19.8
71	29.7	23.8	35.8





#6
bis(2-Chloroethyl)ether
Concen: 0.217 ng
RT: 7.218 min Scan# 449
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13



Tgt Ion: 93 Resp: 23923


Ion	Ratio	Lower	Upper
93	100		
63	74.3	58.8	88.2
95	33.3	26.6	39.8



Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Manual Integrations
APPROVED

mohammad
8/5/2021 5:07:34 PM



#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.571 min Scan# 746
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13



Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021




Tgt Ion:	136	Resp:	184302
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.7	13.1
54	4.8	3.9	5.9
68	3.9	3.3	4.9

Manual Integrations
APPROVED



mohammad
8/5/2021 5:07:34 PM




#8
Nitrobenzene-d5
Concen: 0.246 ng
RT: 8.924 min Scan# 616
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13



Tgt Ion:	82	Resp:	29132
Ion	Ratio	Lower	Upper
82	100		
128	33.4	26.2	39.4
54	56.1	45.1	67.7









#9
Naphthalene
Concen: 0.203 ng
RT: 10.609 min Scan# 749
Delta R.T. -0.013 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion:	128	Resp:	98073
Ion Ratio	Lower	Upper	
128	100		
129	11.1	8.8	13.2
127	13.3	10.2	15.2

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021




Manual Integrations
APPROVED

mohammad
8/5/2021 5:07:34 PM



#10
Hexachlorobutadiene
Concen: 0.197 ng
RT: 10.913 min Scan# 773
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion:	225	Resp:	16582
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	64.4	51.5	77.3









#11
2-Methylnaphthalene-d10
Concen: 0.380 ng
RT: 12.158 min Scan# 966
Delta R.T. -0.005 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion:152 Resp: 105308
Ion Ratio Lower Upper
152 100
151 19.0 16.2 24.4

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021




Manual Integrations
APPROVED

mohammad
8/5/2021 5:07:34 PM

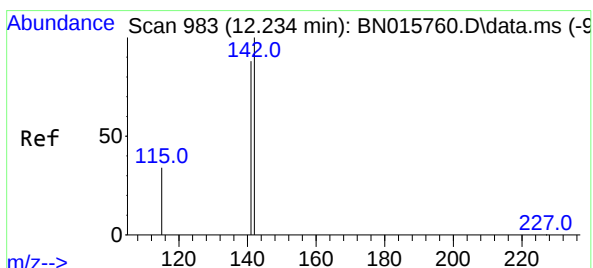

#12
2-Methylnaphthalene
Concen: 0.207 ng
RT: 12.234 min Scan# 983
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13


Tgt Ion:142 Resp: 64374
Ion Ratio Lower Upper
142 100
141 87.4 70.5 105.7
115 33.9 27.4 41.0





#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.408 min Scan# 1194
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021



Tgt Ion:164 Resp: 96208
Ion Ratio Lower Upper
164 100
162 104.0 84.2 126.2
160 48.7 39.8 59.6




Manual Integrations
APPROVED


mohammad
8/5/2021 5:07:34 PM



#14
2,4,6-Tribromophenol
Concen: 0.230 ng
RT: 15.905 min Scan# 1312
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13


Tgt Ion:330 Resp: 8006
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.7 28.2 42.2





#15
2-Fluorobiphenyl
Concen: 0.262 ng
RT: 13.038 min Scan# 1086
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021



Tgt Ion:172 Resp: 100586
Ion Ratio Lower Upper
172 100
171 34.7 27.8 41.8
170 23.2 18.7 28.1




Manual Integrations
APPROVED


mohammad
8/5/2021 5:07:34 PM



#16
Acenaphthylene
Concen: 0.176 ng
RT: 14.129 min Scan# 1172
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13


Tgt Ion:152 Resp: 69672
Ion Ratio Lower Upper
152 100
151 19.5 15.7 23.5
153 13.0 10.5 15.7





#17
Acenaphthene
Concen: 0.189 ng
RT: 14.471 min Scan# 1199
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021



Tgt Ion:154 Resp: 52393
Ion Ratio Lower Upper
154 100
153 114.1 90.5 135.7
152 56.6 44.4 66.6




Manual Integrations
APPROVED


mohammad
8/5/2021 5:07:34 PM



#18
Fluorene
Concen: 0.190 ng
RT: 15.461 min Scan# 1277
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion:166 Resp: 62932
Ion Ratio Lower Upper
166 100
165 97.8 78.2 117.2
167 13.4 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.163 min Scan# 1415
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion:188 Resp: 180470
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.1 7.7 11.5

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021




Manual Integrations
APPROVED


mohammad
8/5/2021 5:07:34 PM

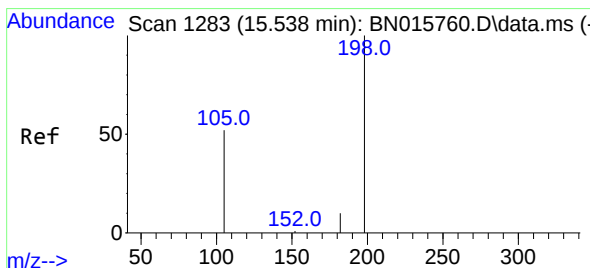


#20
4,6-Dinitro-2-methylphenol
Concen: 0.131 ng
RT: 15.550 min Scan# 1284
Delta R.T. 0.012 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion:198 Resp: 673
Ion Ratio Lower Upper
198 100
182 25.9 11.1 16.7#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.183 ng
RT: 16.360 min Scan# 1349
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13





Tgt Ion:248 Resp: 19456
Ion Ratio Lower Upper
248 100
250 98.3 75.8 113.6
141 54.9 52.8 79.2



#22
Hexachlorobenzene
Concen: 0.195 ng
RT: 16.470 min Scan# 1358
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13




Tgt Ion:284 Resp: 23721
Ion Ratio Lower Upper
284 100
142 36.9 29.4 44.2
249 29.2 23.8 35.6



Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Manual Integrations
APPROVED

mohammad
8/5/2021 5:07:34 PM

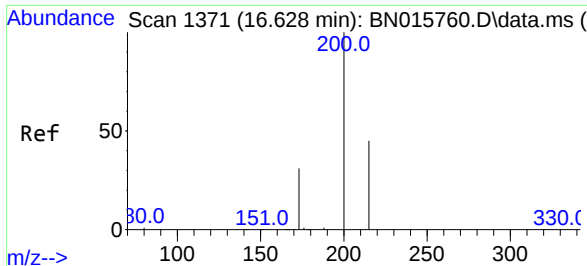

#23
Atrazine
Concen: 0.175 ng
RT: 16.628 min Scan# 1371
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021




Tgt Ion:200 Resp: 11427
Ion Ratio Lower Upper
200 100
173 28.4 25.0 37.6
215 47.1 36.3 54.5

Manual Integrations
APPROVED



mohammad
8/5/2021 5:07:34 PM

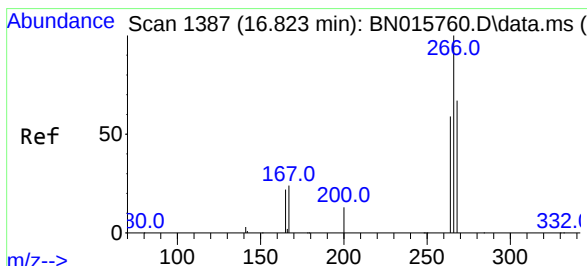


#24
Pentachlorophenol
Concen: 0.146 ng
RT: 16.810 min Scan# 1386
Delta R.T. -0.013 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13



Tgt Ion:266 Resp: 5500
Ion Ratio Lower Upper
266 100
264 62.2 49.7 74.5
268 63.6 51.8 77.6









#25
Phenanthrene
Concen: 0.194 ng
RT: 17.200 min Scan# 1418
Delta R.T. -0.013 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion:178 Resp: 104083
Ion Ratio Lower Upper
178 100
176 18.9 15.1 22.7
179 15.6 12.2 18.4

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021




Manual Integrations
APPROVED


mohammad
8/5/2021 5:07:34 PM




#26
Anthracene
Concen: 0.183 ng
RT: 17.297 min Scan# 1426
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion:178 Resp: 82648
Ion Ratio Lower Upper
178 100
176 18.4 14.6 22.0
179 15.2 12.2 18.4









#27
Fluoranthene-d10
Concen: 0.368 ng
RT: 19.202 min Scan# 1724
Delta R.T. -0.005 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13





Tgt Ion:212 Resp: 172774
Ion Ratio Lower Upper
212 100
106 13.7 10.8 16.2
104 7.6 6.0 9.0



#28
Fluoranthene
Concen: 0.192 ng
RT: 19.231 min Scan# 1730
Delta R.T. -0.005 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13




Tgt Ion:202 Resp: 107489
Ion Ratio Lower Upper
202 100
101 11.7 9.0 13.6
203 17.4 13.8 20.8




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021

Manual Integrations
APPROVED




mohammad
8/5/2021 5:07:34 PM

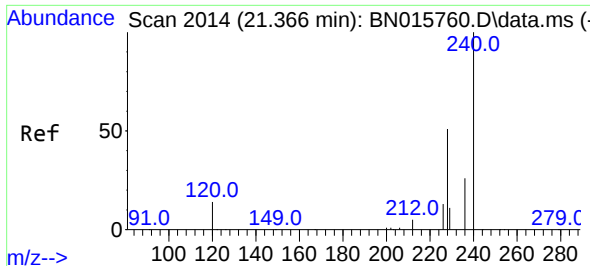


#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.365 min Scan# 2014
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13





Tgt Ion:240 Resp: 160942
Ion Ratio Lower Upper
240 100
120 13.8 11.4 17.0
236 26.6 21.2 31.8



#30
Pyrene
Concen: 0.194 ng
RT: 19.599 min Scan# 1804
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13




Tgt Ion:202 Resp: 104051
Ion Ratio Lower Upper
202 100
200 20.7 16.5 24.7
203 17.5 13.9 20.9



Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Manual Integrations
APPROVED

mohammad
8/5/2021 5:07:34 PM



#31
Terphenyl-d14
Concen: 0.269 ng
RT: 19.807 min Scan# 1846
Delta R.T. -0.005 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021



Tgt Ion:244 Resp: 107322
Ion Ratio Lower Upper
244 100
212 7.6 5.9 8.9
122 13.5 9.7 14.5




Manual Integrations
APPROVED


mohammad
8/5/2021 5:07:34 PM



#32
Benzo(a)anthracene
Concen: 0.185 ng
RT: 21.355 min Scan# 2013
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13


Tgt Ion:228 Resp: 90893
Ion Ratio Lower Upper
228 100
226 26.4 21.2 31.8
229 19.4 15.6 23.4





#33
Chrysene
Concen: 0.193 ng
RT: 21.408 min Scan# 2018
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021




Tgt Ion:228 Resp: 102670
Ion Ratio Lower Upper
228 100
226 28.5 23.3 34.9
229 19.7 15.7 23.5

Manual Integrations
APPROVED



mohammad
8/5/2021 5:07:34 PM



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.156 ng
RT: 21.301 min Scan# 2008
Delta R.T. -0.001 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13




Tgt Ion:149 Resp: 30814
Ion Ratio Lower Upper
149 100
167 26.9 21.2 31.8
279 3.9 3.2 4.8





#35
Perylene-d12
Concen: 0.400 ng
RT: 23.710 min Scan# 2493
Delta R.T. -0.004 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021



Tgt Ion:264 Resp: 156041
Ion Ratio Lower Upper
264 100
260 24.7 19.5 29.3
265 23.1 19.2 28.8




Manual Integrations
APPROVED

mohammad
8/5/2021 5:07:34 PM



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.175 ng
RT: 26.110 min Scan# 3194
Delta R.T. -0.004 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion:276 Resp: 96737
Ion Ratio Lower Upper
276 100
138 28.3 19.6 29.4
277 25.0 20.0 30.0









#37
Benzo(b)fluoranthene
Concen: 0.190 ng
RT: 23.002 min Scan# 2286
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion:252 Resp: 103115
Ion Ratio Lower Upper
252 100
253 22.6 17.7 26.5
125 10.5 8.2 12.4

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021




Manual Integrations
APPROVED

mohammad
8/5/2021 5:07:34 PM



#38
Benzo(k)fluoranthene
Concen: 0.196 ng m
RT: 23.046 min Scan# 2299
Delta R.T. -0.004 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion:252 Resp: 109787
Ion Ratio Lower Upper
252 100
253 23.2 17.8 26.6
125 16.6 8.3 12.5#









#39
Benzo(a)pyrene
Concen: 0.190 ng
RT: 23.607 min Scan# 2463
Delta R.T. -0.000 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion:	252	Resp:	85719
Ion Ratio	Lower	Upper	
252	100		
253	23.0	17.8	26.8
125	11.9	9.0	13.6

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021




Manual Integrations
APPROVED


mohammad
8/5/2021 5:07:34 PM



#40
Dibenzo(a,h)anthracene
Concen: 0.169 ng
RT: 26.127 min Scan# 3199
Delta R.T. -0.004 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13


Tgt Ion:	278	Resp:	78276
Ion Ratio	Lower	Upper	
278	100		
139	29.2	13.1	19.7#
279	24.5	19.1	28.7





#41
Benzo(g,h,i)perylene
Concen: 0.175 ng
RT: 26.839 min Scan# 3407
Delta R.T. -0.007 min
Lab File: BN015792.D
Acq: 04 Aug 2021 14:13

Tgt Ion:	276	Resp:	84739
Ion	Ratio	Lower	Upper
276	100		
277	23.8	19.0	28.6
138	21.4	16.6	24.8



Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021

Manual Integrations
APPROVED

mohammad
8/5/2021 5:07:34 PM