

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080421\
 Data File : BN015810.D
 Acq On : 05 Aug 2021 03:00
 Operator : CG/JU
 Sample : M1458-07
 Misc : LOD-MDL-WATER 0.2ng
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Manual Integrations
 APPROVED

mohammad
 8/5/2021 5:08:22 PM

Quant Time: Aug 05 04:06:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 05 03:12:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	37669	0.400	ng	0.00
7) Naphthalene-d8	10.559	136	167229	0.400	ng	#-0.01
13) Acenaphthene-d10	14.408	164	80794	0.400	ng	0.00
19) Phenanthrene-d10	17.164	188	147435	0.400	ng	0.00
29) Chrysene-d12	21.366	240	125040	0.400	ng	# 0.00
35) Perylene-d12	23.704	264	118685	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.383	112	23782	0.258	ng	0.00
5) Phenol-d6	6.951	99	31704	0.285	ng	0.00
8) Nitrobenzene-d5	8.924	82	36392	0.339	ng	0.00
11) 2-Methylnaphthalene-d10	12.159	152	93035	0.370	ng	0.00
14) 2,4,6-Tribromophenol	15.906	330	6120	0.209	ng	0.00
15) 2-Fluorobiphenyl	13.038	172	88327	0.274	ng	0.00
27) Fluoranthene-d10	19.202	212	134551	0.351	ng	0.00
31) Terphenyl-d14	19.808	244	80820	0.261	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.346	88	802	0.066	ng	# 20
3) n-Nitrosodimethylamine	3.724	42	2009	0.080	ng	# 83
6) bis(2-Chloroethyl)ether	7.218	93	23399	0.232	ng	95
9) Naphthalene	10.610	128	89420	0.204	ng	100
10) Hexachlorobutadiene	10.914	225	16373	0.214	ng	# 100
12) 2-Methylnaphthalene	12.230	142	57019	0.202	ng	99
16) Acenaphthylene	14.129	152	69486	0.209	ng	100
17) Acenaphthene	14.472	154	45769	0.197	ng	96
18) Fluorene	15.462	166	53001	0.191	ng	99
20) 4,6-Dinitro-2-methylph...	15.538	198	418	0.047	ng	# 48
21) 4-Bromophenyl-phenylether	16.361	248	17095	0.197	ng	# 85
22) Hexachlorobenzene	16.470	284	23567	0.237	ng	98
23) Atrazine	16.628	200	7069	0.133	ng	94
24) Pentachlorophenol	16.811	266	4027	0.131	ng	99
25) Phenanthrene	17.200	178	88087	0.201	ng	100
26) Anthracene	17.298	178	68061	0.185	ng	100
28) Fluoranthene	19.232	202	88577	0.194	ng	99
30) Pyrene	19.594	202	77996	0.187	ng	100
32) Benzo(a)anthracene	21.344	228	63438	0.166	ng	98
33) Chrysene	21.398	228	79109	0.191	ng	98
34) Bis(2-ethylhexyl)phtha...	21.291	149	18247	0.119	ng	98
36) Indeno(1,2,3-cd)pyrene	26.103	276	68660	0.163	ng	97
37) Benzo(b)fluoranthene	22.999	252	70023	0.170	ng	99
38) Benzo(k)fluoranthene	23.043	252	85950m	0.201	ng	
39) Benzo(a)pyrene	23.601	252	55175	0.161	ng	98
40) Dibenzo(a,h)anthracene	26.124	278	55107	0.157	ng	# 93
41) Benzo(g,h,i)perylene	26.832	276	58738	0.160	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080421\
 Data File : BN015810.D
 Acq On : 05 Aug 2021 03:00
 Operator : CG/JU
 Sample : M1458-07
 Misc : LOD-MDL-WATER 0.2ng
 ALS Vial : 25 Sample Multiplier: 1


Instrument :
 BNA_N
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Manual Integrations
 APPROVED


mohammad
 8/5/2021 5:08:22 PM

Quant Time: Aug 05 04:06:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 05 03:12:25 2021
 Response via : Initial Calibration



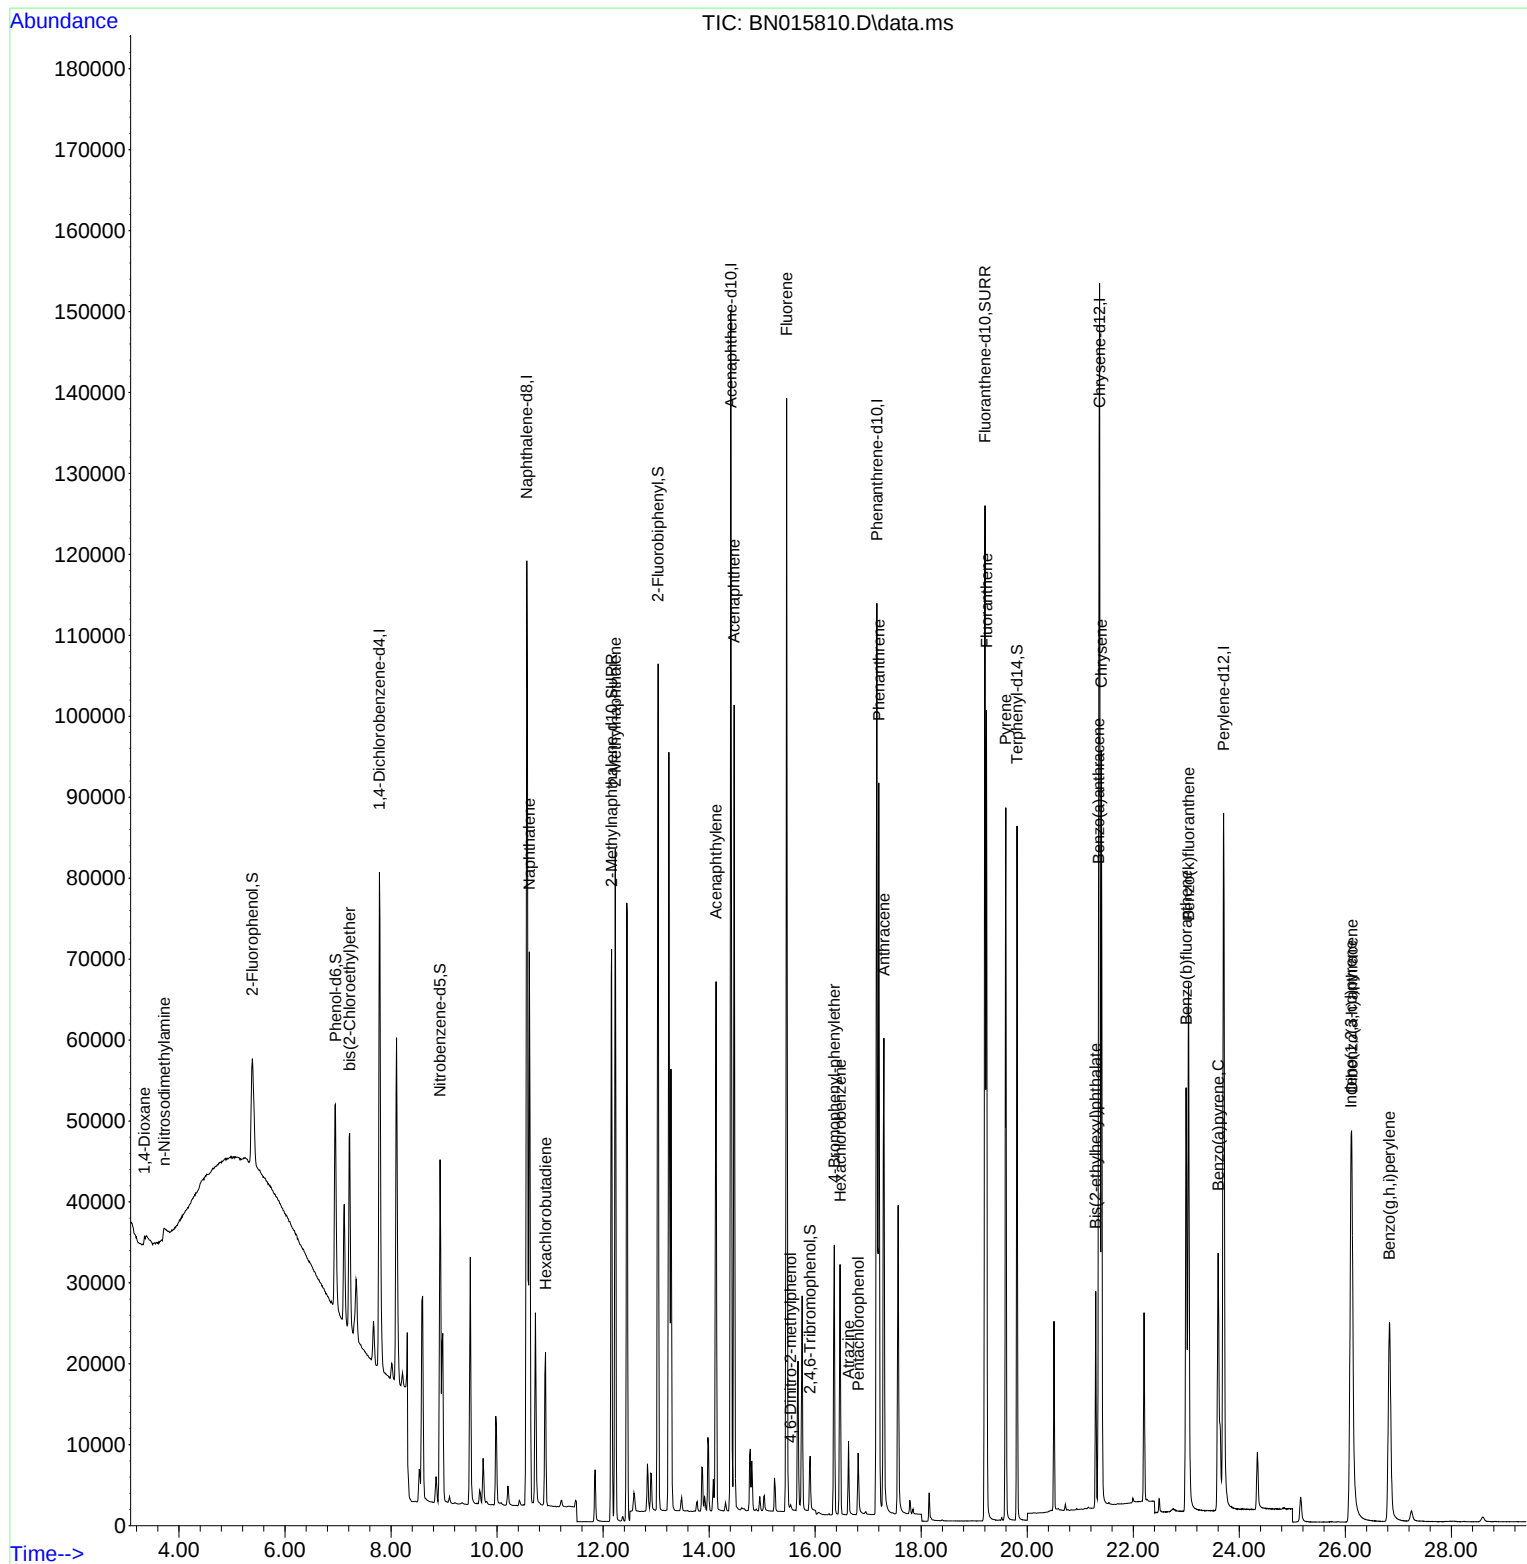





#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.781 min Scan# 510
Delta R.T. -0.009 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00





Tgt Ion:152 Resp: 37669
Ion Ratio Lower Upper
152 100
150 157.3 123.5 185.3
115 61.8 46.8 70.2

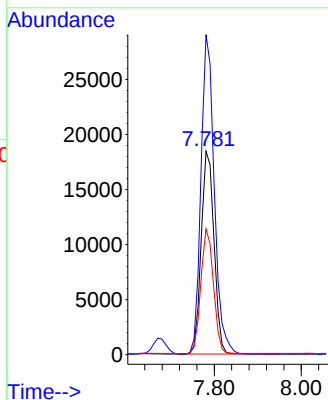

#2
1,4-Dioxane
Concen: 0.066 ng
RT: 3.346 min Scan# 29
Delta R.T. -0.009 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00




Tgt Ion: 88 Resp: 802
Ion Ratio Lower Upper
88 100
43 0.0 23.1 34.7#
58 0.0 62.2 93.4#

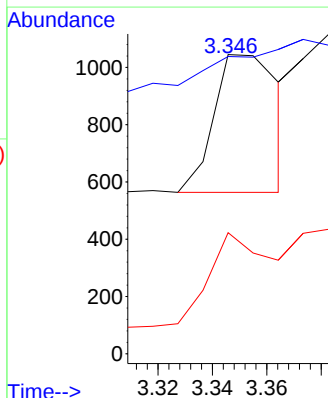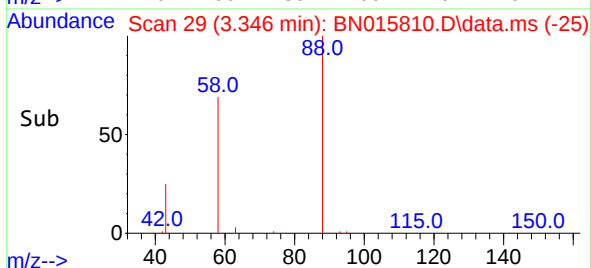

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Manual Integrations
APPROVED

mohammad
8/5/2021 5:08:22 PM

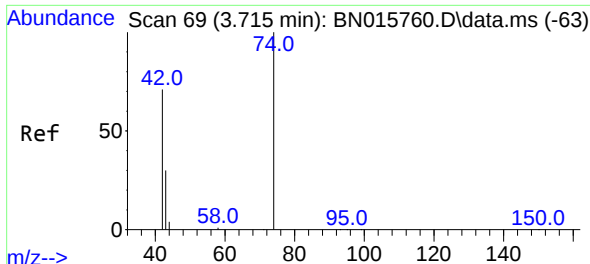





#3
n-Nitrosodimethylamine
Concen: 0.080 ng
RT: 3.724 min Scan# 70
Delta R.T. 0.009 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion: 42 Resp: 2009
Ion Ratio Lower Upper
42 100
74 163.8 114.4 171.6
44 0.0 3.6 5.4#

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




Manual Integrations
APPROVED


mohammad
8/5/2021 5:08:22 PM

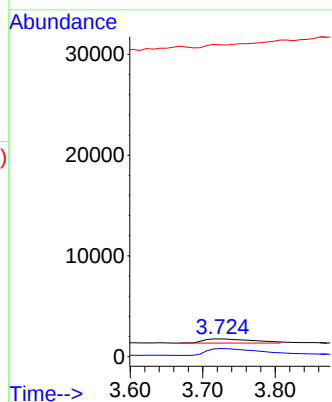

#4
2-Fluorophenol
Concen: 0.258 ng
RT: 5.383 min Scan# 250
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion: 112 Resp: 23782
Ion Ratio Lower Upper
112 100
64 56.6 42.2 63.4
63 29.0 22.2 33.2

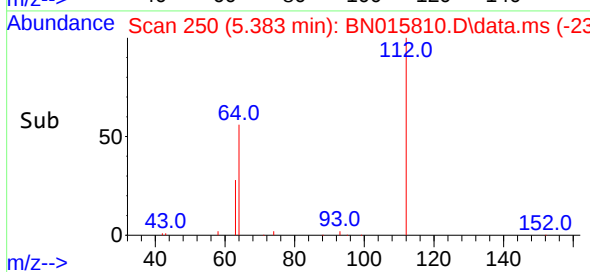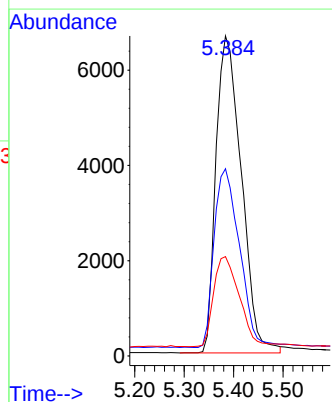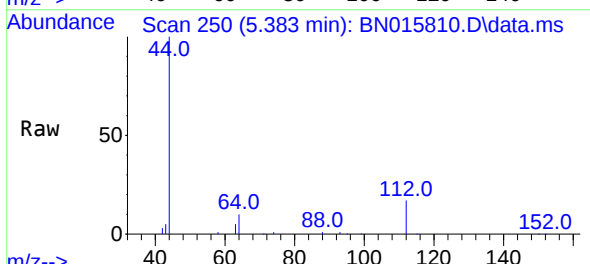

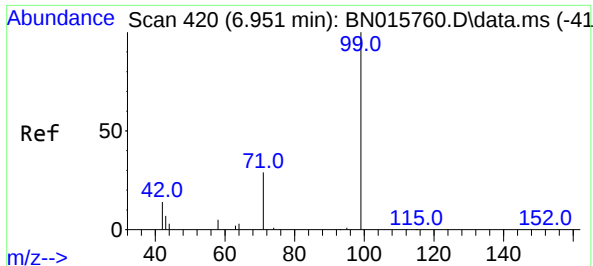

#5
Phenol-d6
Concen: 0.285 ng
RT: 6.951 min Scan# 420
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00





Tgt Ion: 99 Resp: 31704

Ion	Ratio	Lower	Upper
99	100		
42	17.6	13.2	19.8
71	30.0	23.8	35.8

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Manual Integrations
APPROVED




mohammad
8/5/2021 5:08:22 PM

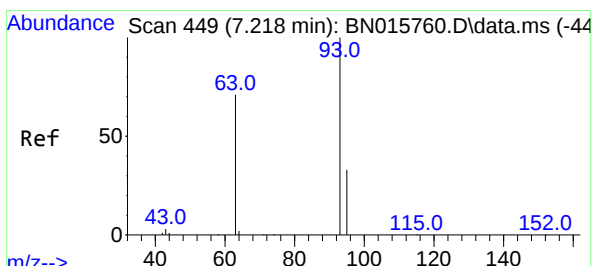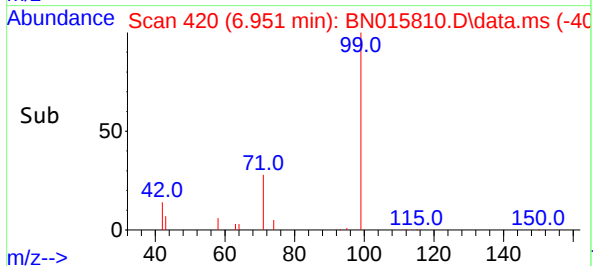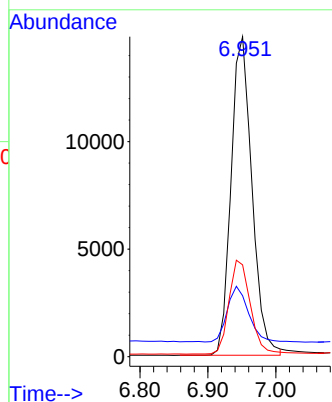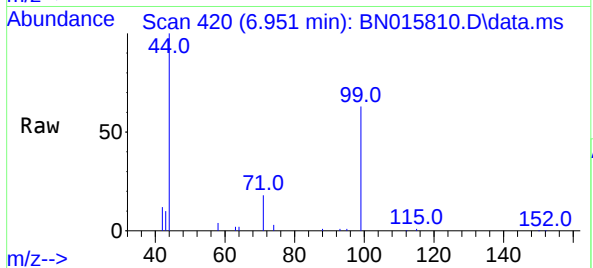


#6
bis(2-Chloroethyl)ether
Concen: 0.232 ng
RT: 7.218 min Scan# 449
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion: 93 Resp: 23399


Ion	Ratio	Lower	Upper
93	100		
63	79.1	58.8	88.2
95	33.4	26.6	39.8

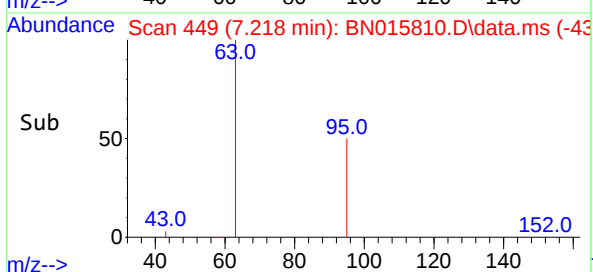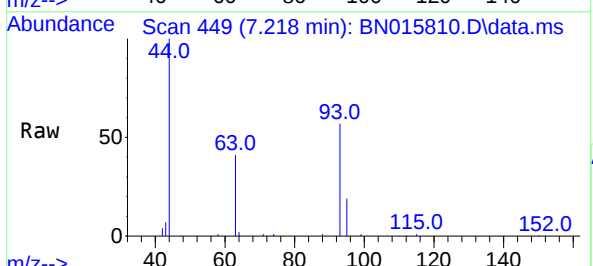



#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.559 min Scan# 745
Delta R.T. -0.013 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021



Tgt Ion:136 Resp: 167229
Ion Ratio Lower Upper
136 100
137 11.0 8.7 13.1
54 9.7 3.9 5.9#
68 7.0 3.3 4.9#




Manual Integrations
APPROVED


mohammad
8/5/2021 5:08:22 PM



#8
Nitrobenzene-d5
Concen: 0.339 ng
RT: 8.924 min Scan# 616
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion: 82 Resp: 36392
Ion Ratio Lower Upper
82 100
128 34.8 26.2 39.4
54 56.6 45.1 67.7

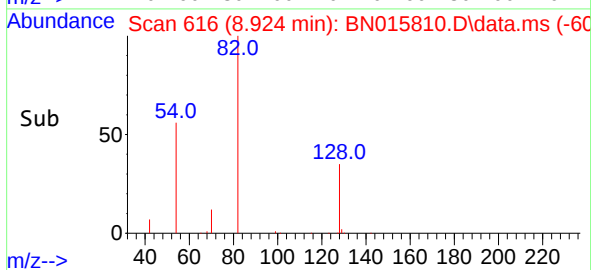







#9
Naphthalene
Concen: 0.204 ng
RT: 10.610 min Scan# 749
Delta R.T. -0.013 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:	128	Resp:	89420
Ion	Ratio	Lower	Upper
128	100		
129	11.0	8.8	13.2
127	13.0	10.2	15.2

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




Manual Integrations
APPROVED

mohammad
8/5/2021 5:08:22 PM



#10
Hexachlorobutadiene
Concen: 0.214 ng
RT: 10.914 min Scan# 773
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:	225	Resp:	16373
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.0	51.5	77.3

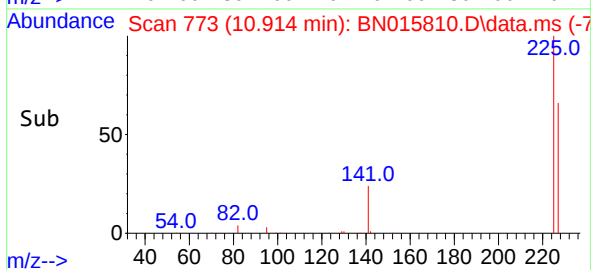







#11
2-Methylnaphthalene-d10
Concen: 0.370 ng
RT: 12.159 min Scan# 966
Delta R.T. -0.004 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:152 Resp: 93035
Ion Ratio Lower Upper
152 100
151 19.0 16.2 24.4

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




Manual Integrations
APPROVED


mohammad
8/5/2021 5:08:22 PM

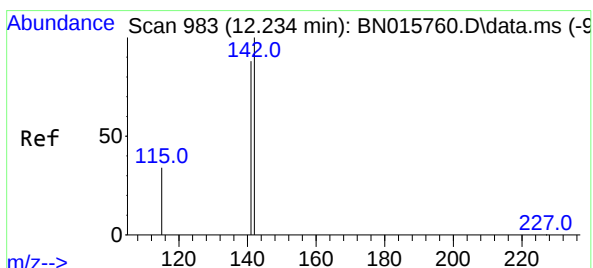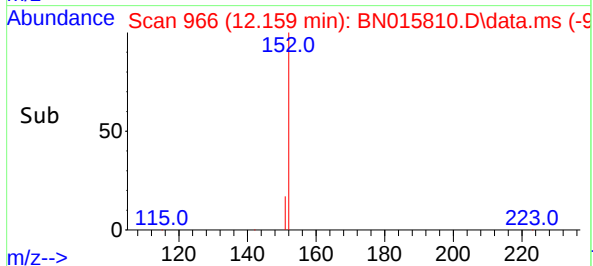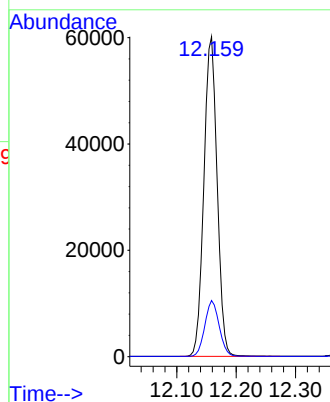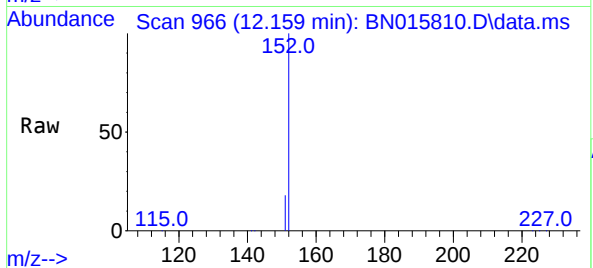

#12
2-Methylnaphthalene
Concen: 0.202 ng
RT: 12.230 min Scan# 982
Delta R.T. -0.004 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00


Tgt Ion:142 Resp: 57019
Ion Ratio Lower Upper
142 100
141 88.3 70.5 105.7
115 34.9 27.4 41.0

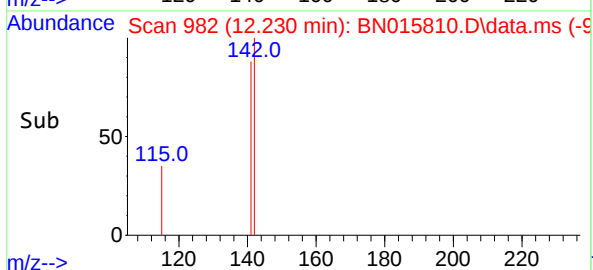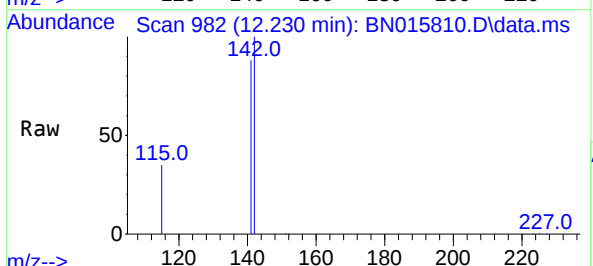

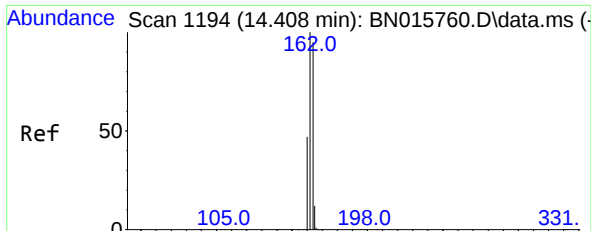

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.408 min Scan# 1194
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

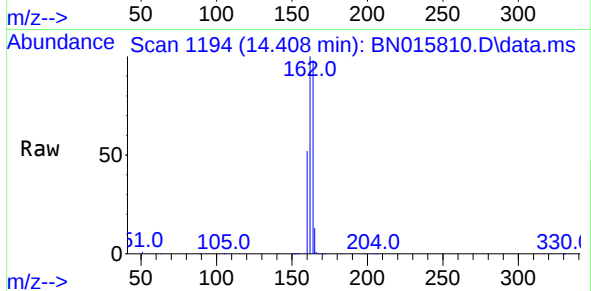

Tgt Ion:164 Resp: 80794
Ion Ratio Lower Upper
164 100
162 102.5 84.2 126.2
160 53.1 39.8 59.6




Manual Integrations
APPROVED


mohammad
8/5/2021 5:08:22 PM

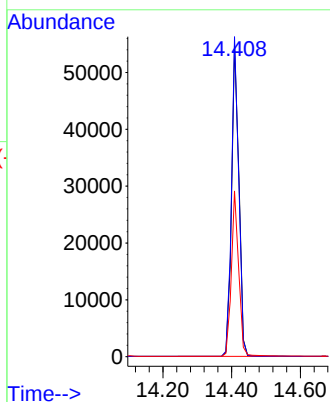

#14
2,4,6-Tribromophenol
Concen: 0.209 ng
RT: 15.906 min Scan# 1312
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:330 Resp: 6120
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 34.5 28.2 42.2

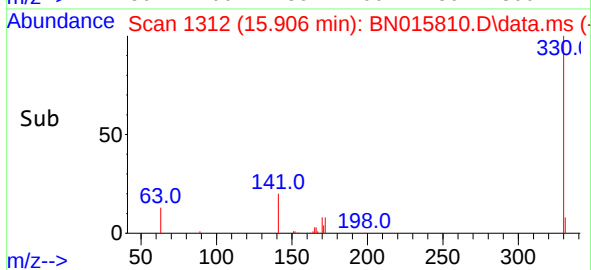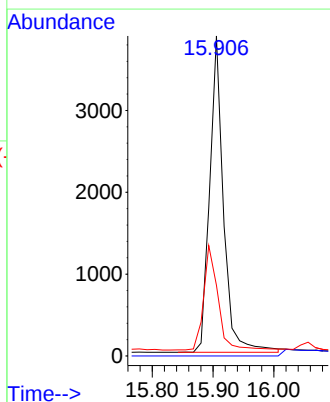







#15
2-Fluorobiphenyl
Concen: 0.274 ng
RT: 13.038 min Scan# 1086
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:172 Resp: 88327
Ion Ratio Lower Upper
172 100
171 33.8 27.8 41.8
170 22.6 18.7 28.1

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




Manual Integrations
APPROVED


mohammad
8/5/2021 5:08:22 PM

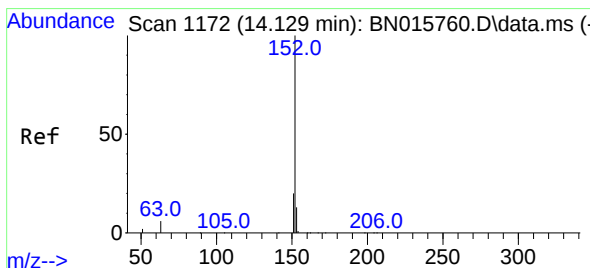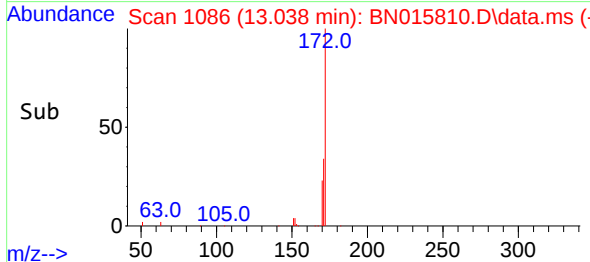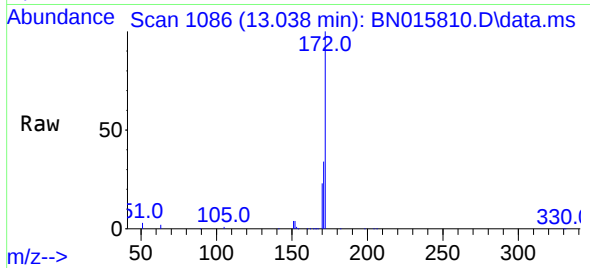

#16
Acenaphthylene
Concen: 0.209 ng
RT: 14.129 min Scan# 1172
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00


Tgt Ion:152 Resp: 69486
Ion Ratio Lower Upper
152 100
151 19.4 15.7 23.5
153 13.2 10.5 15.7

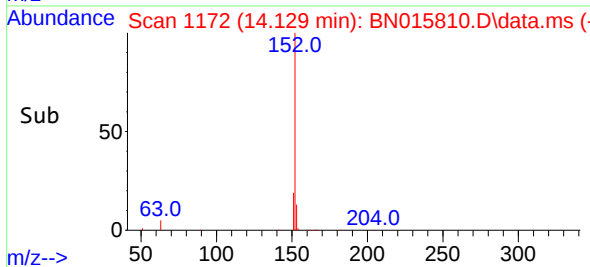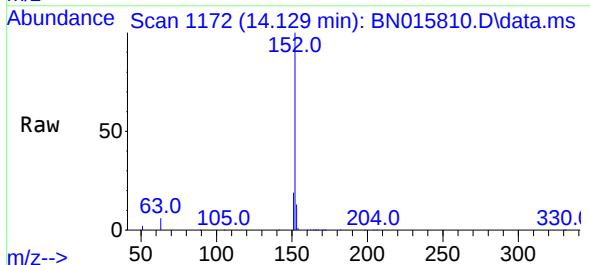



#17
Acenaphthene
Concen: 0.197 ng
RT: 14.472 min Scan# 1199
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00



Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

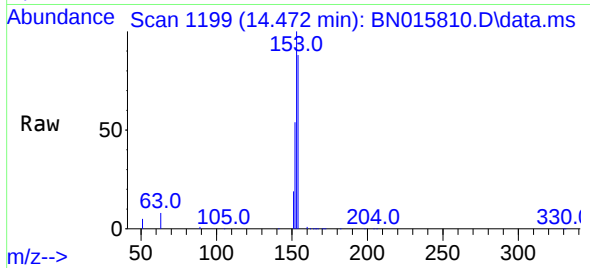


Tgt Ion:154 Resp: 45769
Ion Ratio Lower Upper
154 100
153 113.2 90.5 135.7
152 63.3 44.4 66.6

Manual Integrations
APPROVED



mohammad
8/5/2021 5:08:22 PM

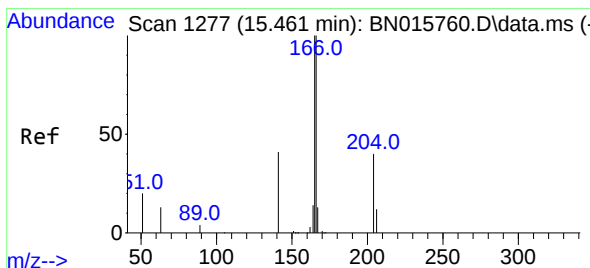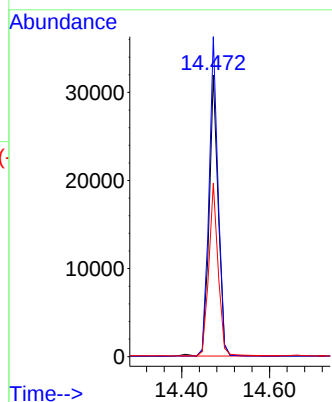


#18
Fluorene
Concen: 0.191 ng
RT: 15.462 min Scan# 1277
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

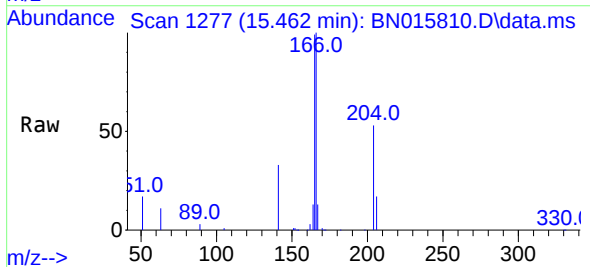

Tgt Ion:166 Resp: 53001
Ion Ratio Lower Upper
166 100
165 98.5 78.2 117.2
167 13.5 10.7 16.1

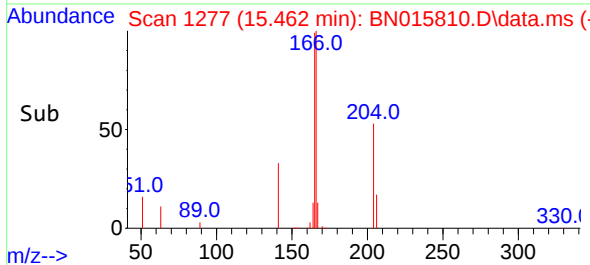







#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.164 min Scan# 1415
Delta R.T. -0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:188 Resp: 147435
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.0 7.7 11.5

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




Manual Integrations
APPROVED


mohammad
8/5/2021 5:08:22 PM

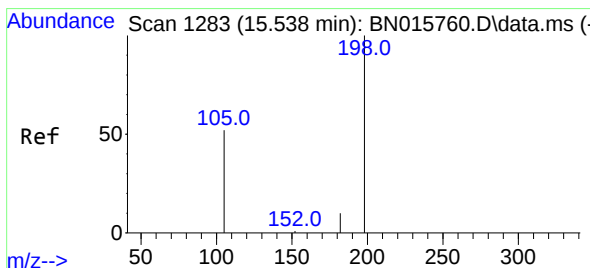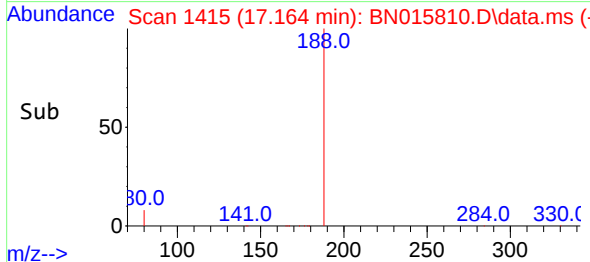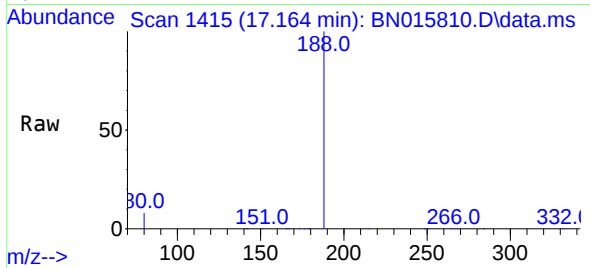


#20
4,6-Dinitro-2-methylphenol
Concen: 0.047 ng
RT: 15.538 min Scan# 1283
Delta R.T. -0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:198 Resp: 418
Ion Ratio Lower Upper
198 100
182 35.1 11.1 16.7#
77 0.0 0.0 0.0

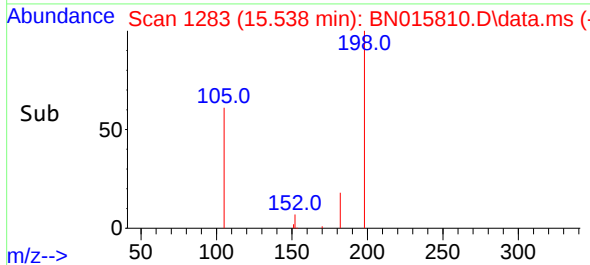

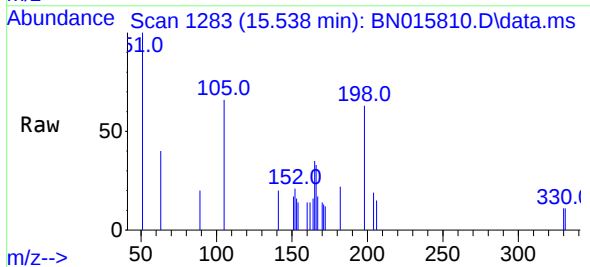





#21
4-Bromophenyl-phenylether
Concen: 0.197 ng
RT: 16.361 min Scan# 1349
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00





Tgt Ion:248 Resp: 17095
Ion Ratio Lower Upper
248 100
250 99.2 75.8 113.6
141 42.0 52.8 79.2#

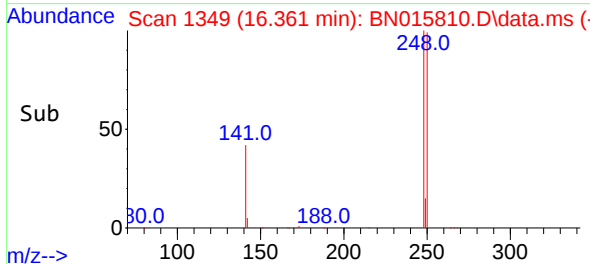

#22
Hexachlorobenzene
Concen: 0.237 ng
RT: 16.470 min Scan# 1358
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

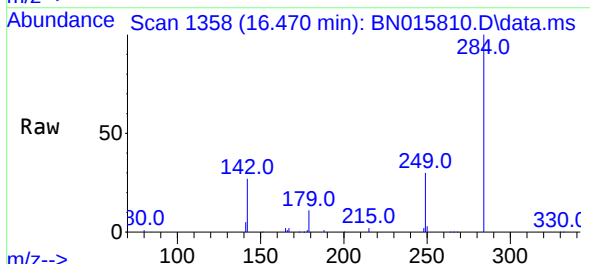


Tgt Ion:284 Resp: 23567
Ion Ratio Lower Upper
284 100
142 35.7 29.4 44.2
249 29.0 23.8 35.6

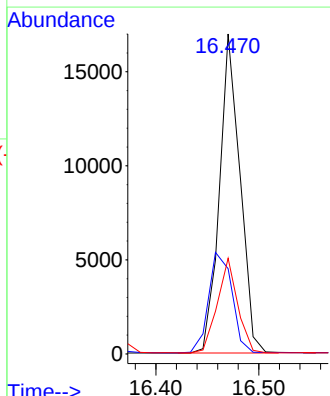

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Manual Integrations
APPROVED

mohammad
8/5/2021 5:08:22 PM

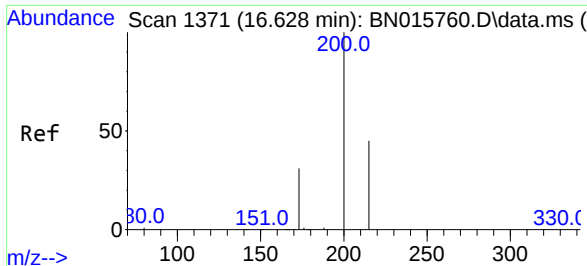

#23
Atrazine
Concen: 0.133 ng
RT: 16.628 min Scan# 1371
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

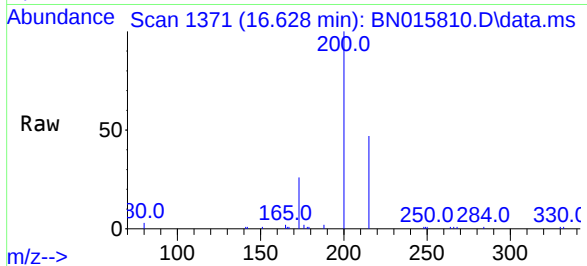


Tgt Ion:200 Resp: 7069
Ion Ratio Lower Upper
200 100
173 25.9 25.0 37.6
215 47.4 36.3 54.5

Manual Integrations
APPROVED



mohammad
8/5/2021 5:08:22 PM

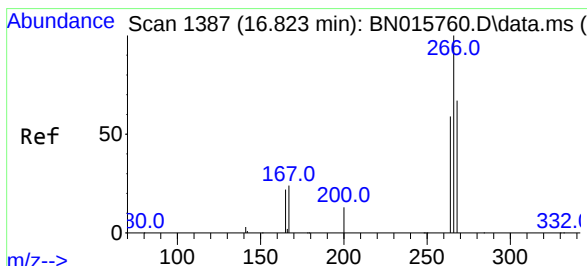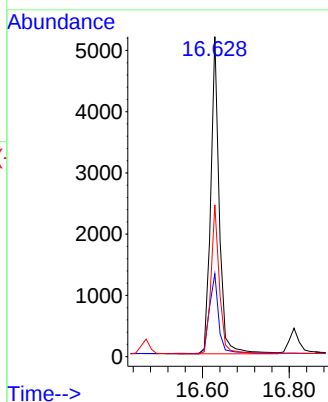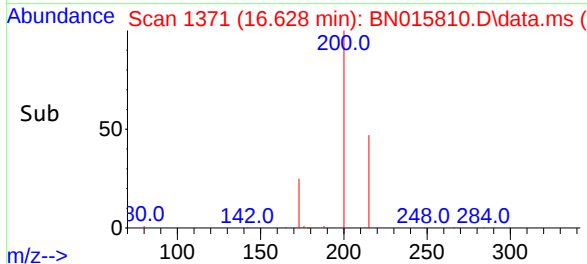


#24
Pentachlorophenol
Concen: 0.131 ng
RT: 16.811 min Scan# 1386
Delta R.T. -0.012 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

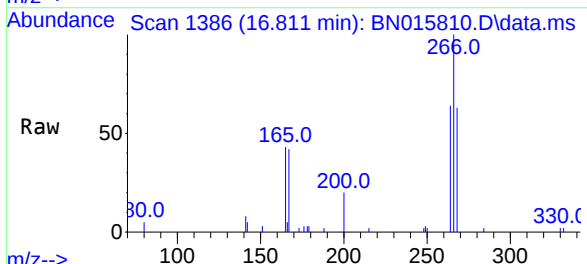

Tgt Ion:266 Resp: 4027
Ion Ratio Lower Upper
266 100
264 63.6 49.7 74.5
268 64.2 51.8 77.6

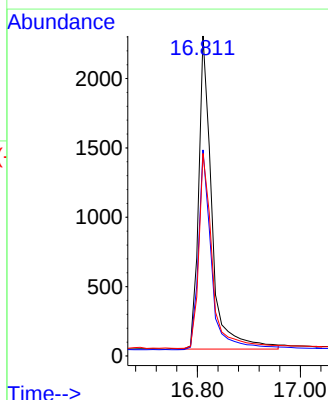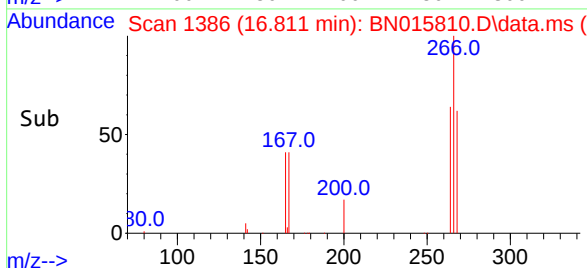







#25
Phenanthrene
Concen: 0.201 ng
RT: 17.200 min Scan# 1418
Delta R.T. -0.012 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:178 Resp: 88087
Ion Ratio Lower Upper
178 100
176 18.9 15.1 22.7
179 15.7 12.2 18.4

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




Manual Integrations
APPROVED


mohammad
8/5/2021 5:08:22 PM




#26
Anthracene
Concen: 0.185 ng
RT: 17.298 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:178 Resp: 68061
Ion Ratio Lower Upper
178 100
176 18.4 14.6 22.0
179 15.3 12.2 18.4

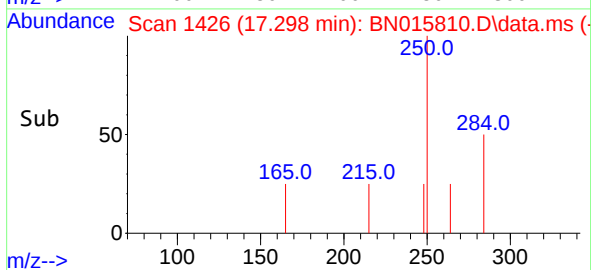







#27
Fluoranthene-d10
Concen: 0.351 ng
RT: 19.202 min Scan# 1724
Delta R.T. -0.005 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

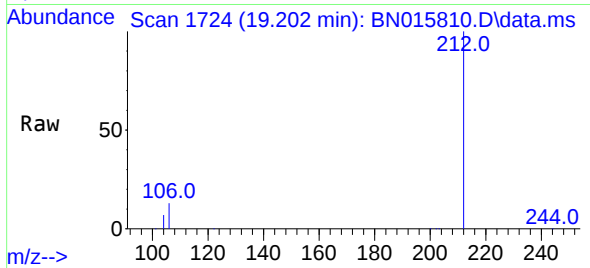



Tgt Ion:212 Resp: 134551
Ion Ratio Lower Upper
212 100
106 14.1 10.8 16.2
104 7.8 6.0 9.0

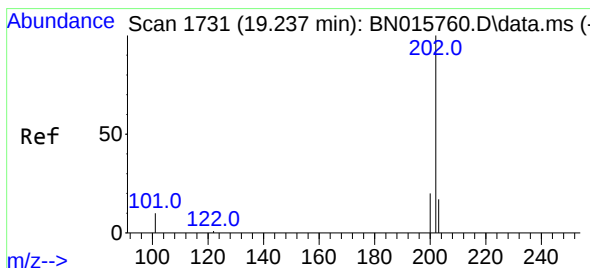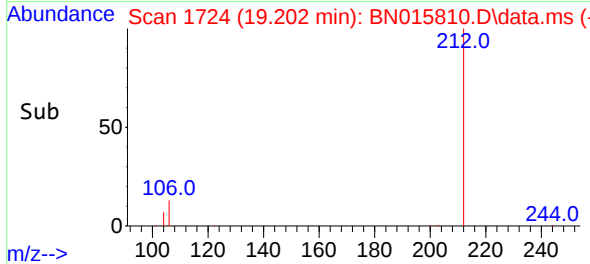

#28
Fluoranthene
Concen: 0.194 ng
RT: 19.232 min Scan# 1730
Delta R.T. -0.005 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

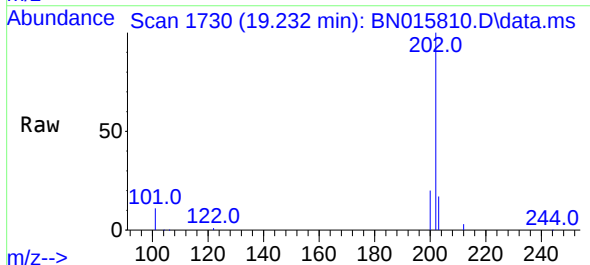


Tgt Ion:202 Resp: 88577
Ion Ratio Lower Upper
202 100
101 12.0 9.0 13.6
203 17.3 13.8 20.8

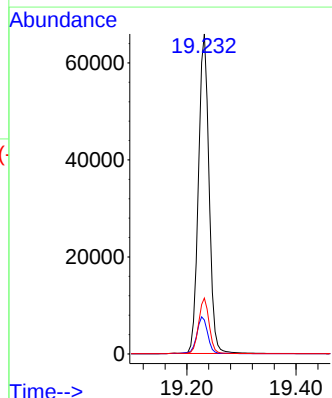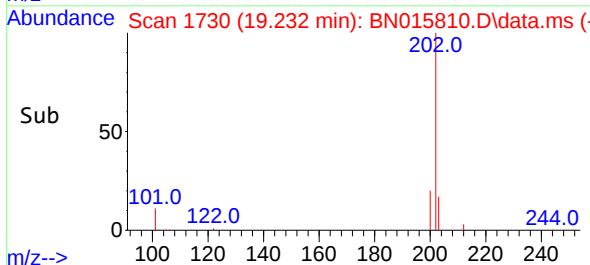

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Manual Integrations
APPROVED

mohammad
8/5/2021 5:08:22 PM

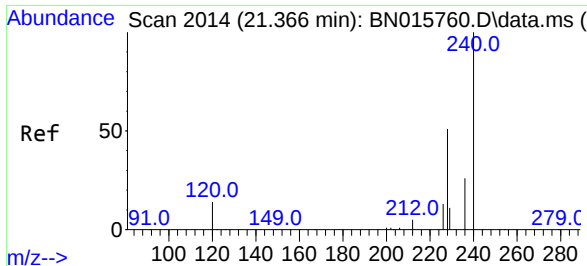





#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.366 min Scan# 2014
Delta R.T. 0.000 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:240 Resp: 125040
Ion Ratio Lower Upper
240 100
120 8.6 11.4 17.0#
236 26.1 21.2 31.8

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




Manual Integrations
APPROVED


mohammad
8/5/2021 5:08:22 PM

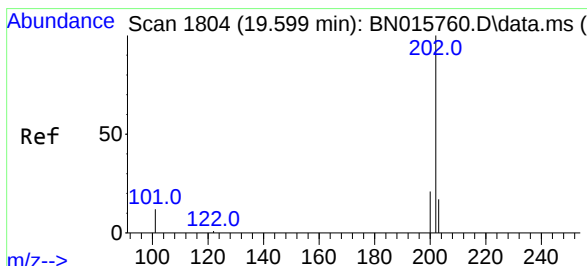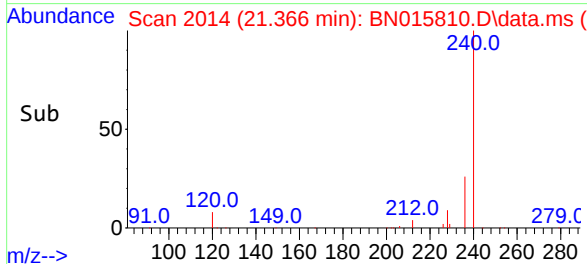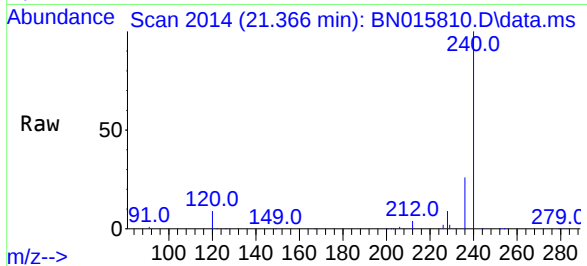

#30
Pyrene
Concen: 0.187 ng
RT: 19.594 min Scan# 1803
Delta R.T. -0.005 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00


Tgt Ion:202 Resp: 77996
Ion Ratio Lower Upper
202 100
200 20.6 16.5 24.7
203 17.4 13.9 20.9

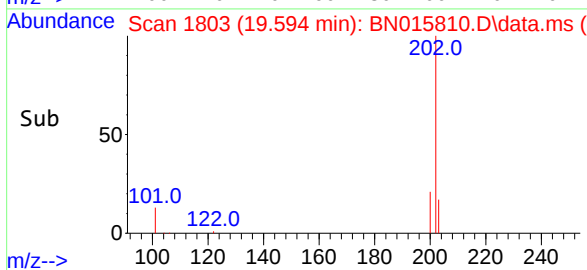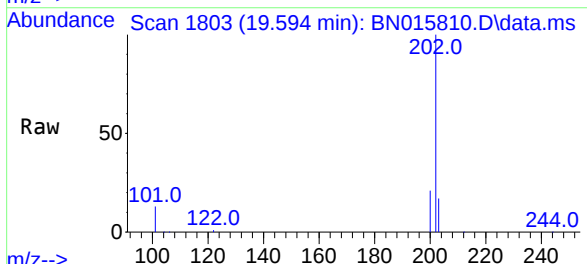



#31
Terphenyl-d14
Concen: 0.261 ng
RT: 19.808 min Scan# 1846
Delta R.T. -0.005 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

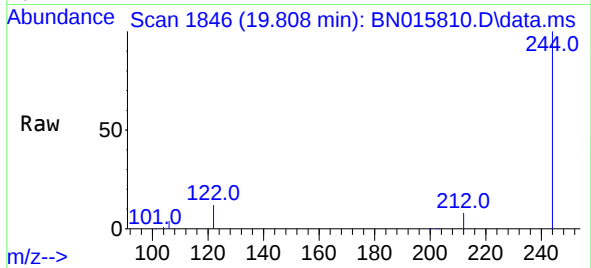

Tgt Ion:244 Resp: 80820
Ion Ratio Lower Upper
244 100
212 7.6 5.9 8.9
122 12.4 9.7 14.5




Manual Integrations
APPROVED


mohammad
8/5/2021 5:08:22 PM

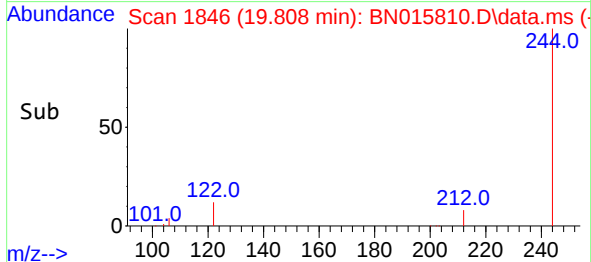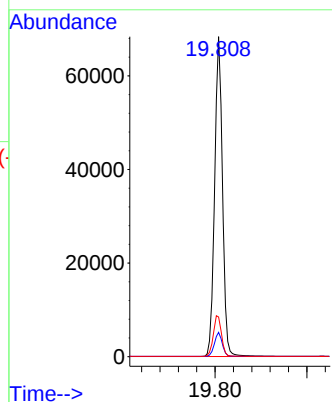

#32
Benzo(a)anthracene
Concen: 0.166 ng
RT: 21.344 min Scan# 2012
Delta R.T. -0.011 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:228 Resp: 63438
Ion Ratio Lower Upper
228 100
226 27.9 21.2 31.8
229 19.2 15.6 23.4

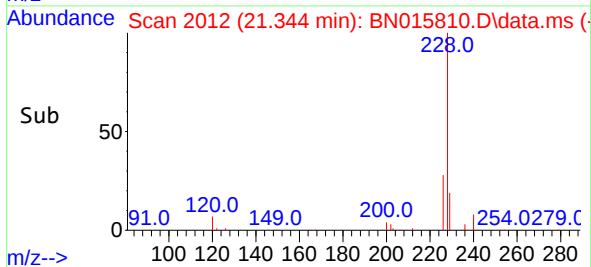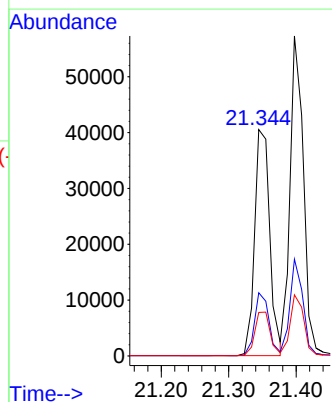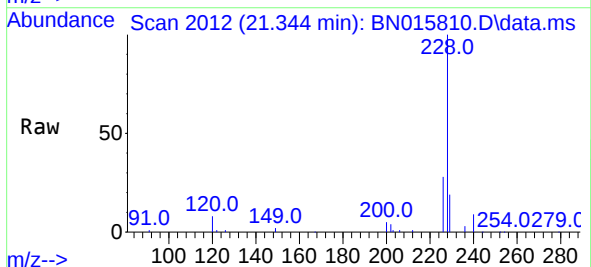







#33
Chrysene
Concen: 0.191 ng
RT: 21.398 min Scan# 2017
Delta R.T. -0.011 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:	228	Resp:	79109
Ion Ratio	Lower	Upper	
228	100		
226	30.3	23.3	34.9
229	19.1	15.7	23.5

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




Manual Integrations
APPROVED

mohammad
8/5/2021 5:08:22 PM

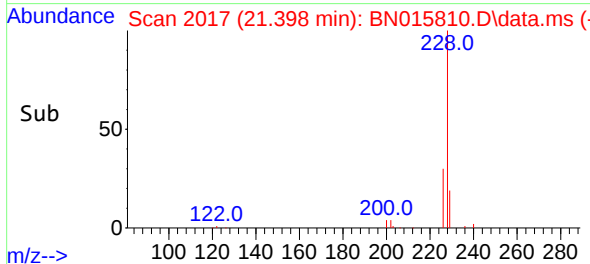


#34
Bis(2-ethylhexyl)phthalate
Concen: 0.119 ng
RT: 21.291 min Scan# 2007
Delta R.T. -0.011 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:	149	Resp:	18247
Ion Ratio	Lower	Upper	
149	100		
167	25.6	21.2	31.8
279	3.7	3.2	4.8

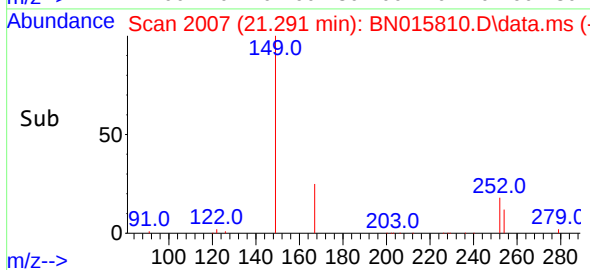
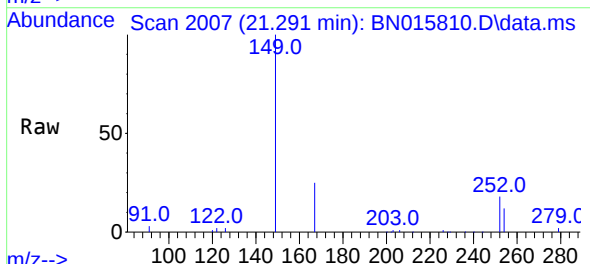





#35
Perylene-d12
Concen: 0.400 ng
RT: 23.704 min Scan# 2491
Delta R.T. -0.010 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00



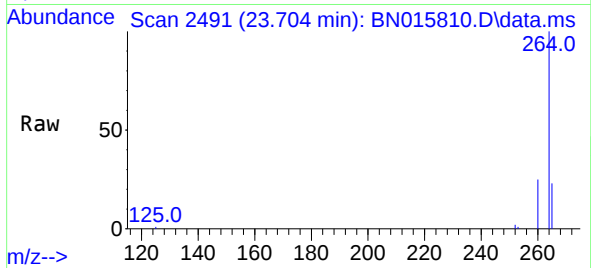


Tgt Ion:264 Resp: 118685
Ion Ratio Lower Upper
264 100
260 24.6 19.5 29.3
265 22.9 19.2 28.8

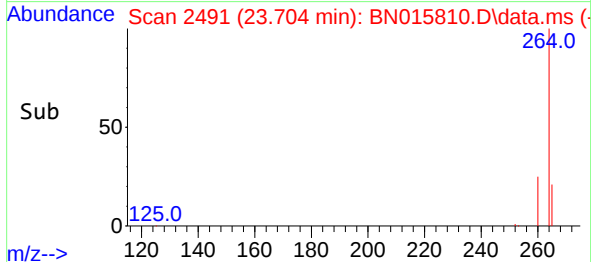

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.163 ng
RT: 26.103 min Scan# 3192
Delta R.T. -0.010 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:276 Resp: 68660
Ion Ratio Lower Upper
276 100
138 27.1 19.6 29.4
277 24.9 20.0 30.0

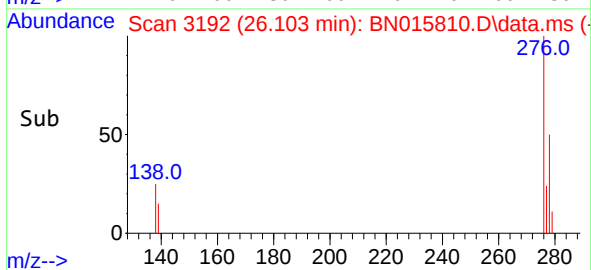

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Manual Integrations
APPROVED

mohammad
8/5/2021 5:08:22 PM







#37
Benzo(b)fluoranthene
Concen: 0.170 ng
RT: 22.999 min Scan# 2285
Delta R.T. -0.003 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:252 Resp: 70023
Ion Ratio Lower Upper
252 100
253 22.3 17.7 26.5
125 10.8 8.2 12.4

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




Manual Integrations
APPROVED

mohammad
8/5/2021 5:08:22 PM

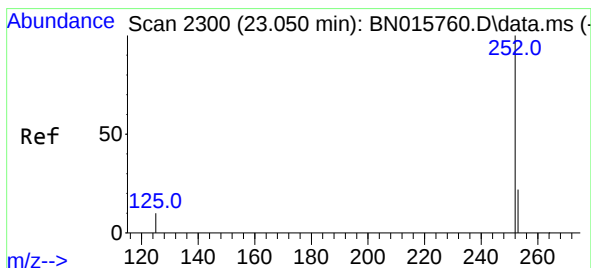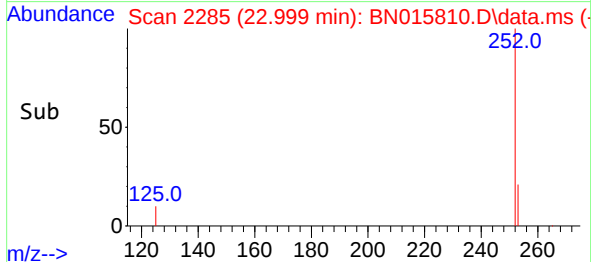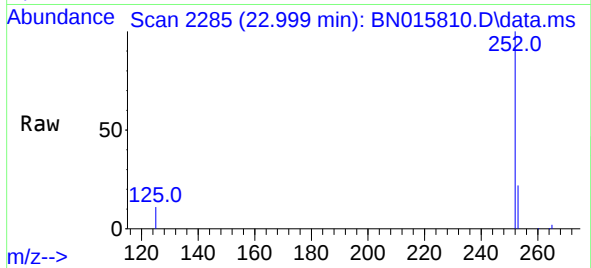


#38
Benzo(k)fluoranthene
Concen: 0.201 ng m
RT: 23.043 min Scan# 2298
Delta R.T. -0.007 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:252 Resp: 85950
Ion Ratio Lower Upper
252 100
253 22.8 17.8 26.6
125 13.0 8.3 12.5#

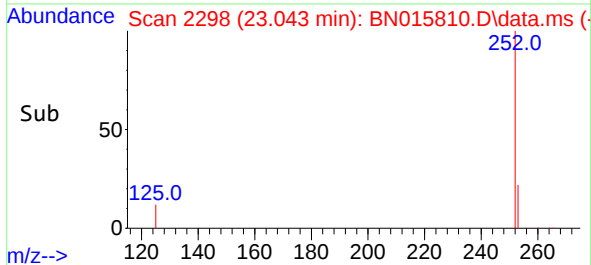

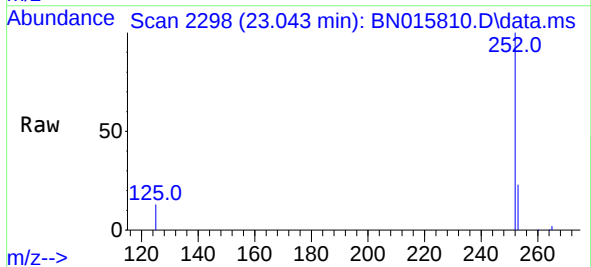





#39
Benzo(a)pyrene
Concen: 0.161 ng
RT: 23.601 min Scan# 2461
Delta R.T. -0.007 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

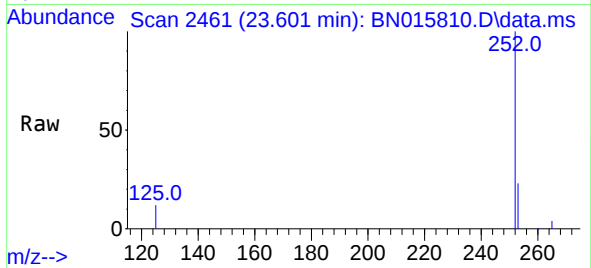



Tgt Ion:252 Resp: 55175
Ion Ratio Lower Upper
252 100
253 22.8 17.8 26.8
125 12.3 9.0 13.6

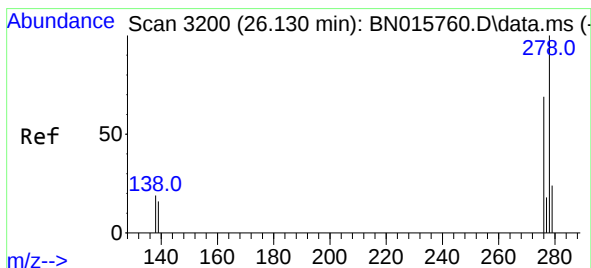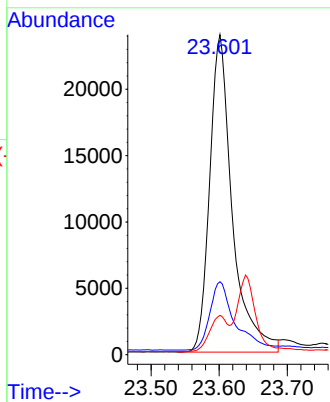

#40
Dibenzo(a,h)anthracene
Concen: 0.157 ng
RT: 26.124 min Scan# 3198
Delta R.T. -0.007 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

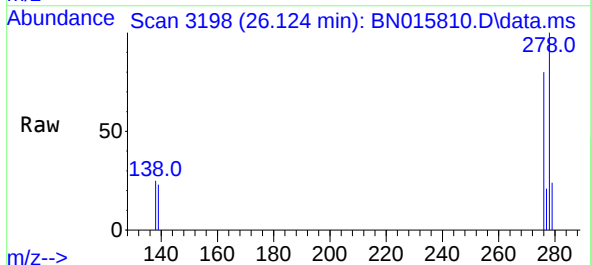


Tgt Ion:278 Resp: 55107
Ion Ratio Lower Upper
278 100
139 23.1 13.1 19.7#
279 24.4 19.1 28.7

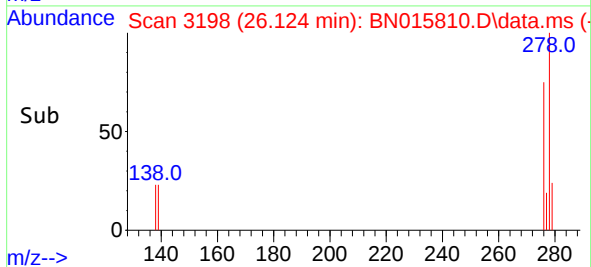

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Manual Integrations
APPROVED

mohammad
8/5/2021 5:08:22 PM

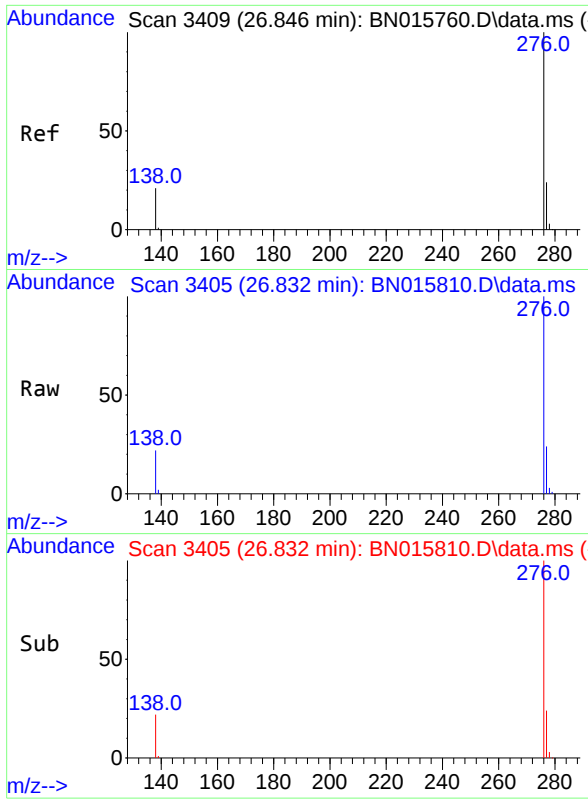

#41
Benzo(g,h,i)perylene
Concen: 0.160 ng
RT: 26.832 min Scan# 3405
Delta R.T. -0.014 min
Lab File: BN015810.D
Acq: 05 Aug 2021 03:00

Tgt Ion:	276	Resp:	58738
Ion	Ratio	Lower	Upper
276	100		
277	24.3	19.0	28.6
138	22.4	16.6	24.8

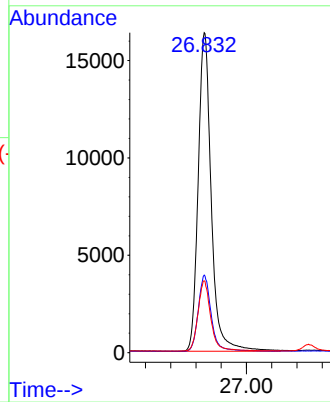

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Manual Integrations
APPROVED

mohammad
8/5/2021 5:08:22 PM