
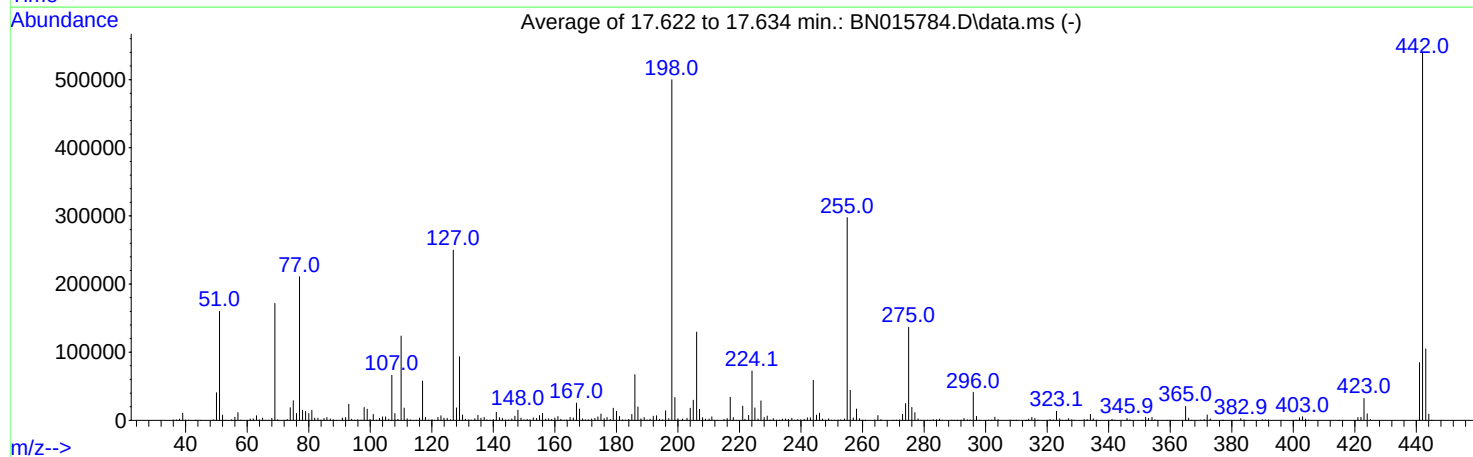


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080421\
 Data File : BN015784.D
 Acq On : 04 Aug 2021 09:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 02 14:09:59 2021

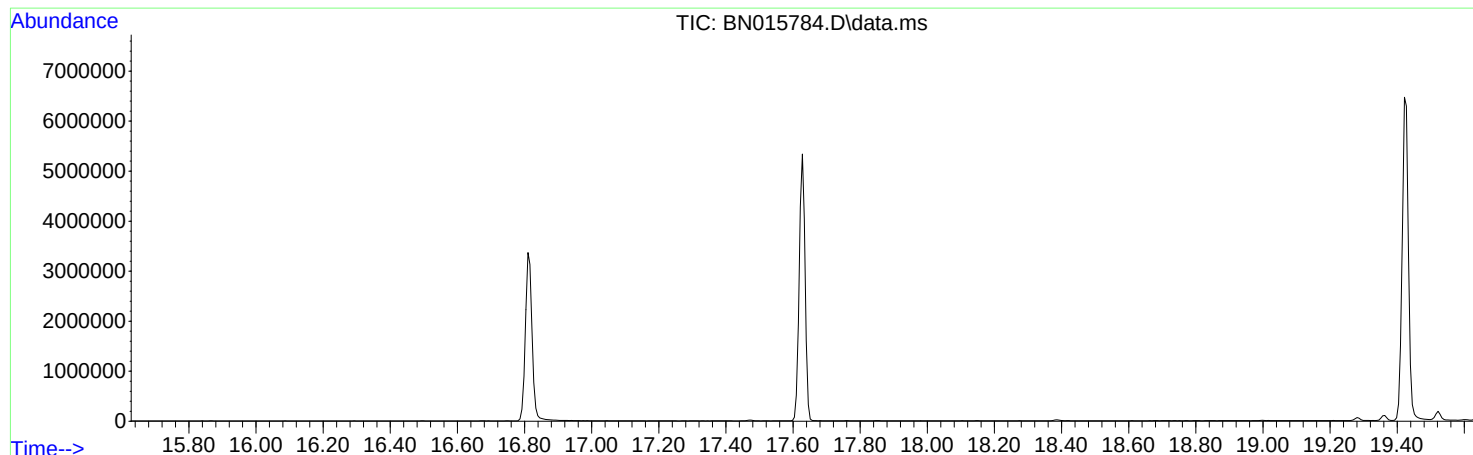




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	159947	PASS
68	69	0.00	2	1.7	2976	PASS
69	198	0.00	100	34.4	171733	PASS
70	69	0.00	2	0.6	1003	PASS
127	198	10	80	50.0	249920	PASS
197	198	0.00	2	0.5	2636	PASS
198	198	100	100	100.0	499861	PASS
199	198	5	9	6.7	33707	PASS
275	198	10	60	27.3	136627	PASS
365	198	1	100	4.1	20456	PASS
441	198	0.01	100	17.0	84805	PASS
442	442	50	100	100.0	539840	PASS
443	442	15	24	19.5	105003	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080421\
Data File : BN015784.D
Acq On : 04 Aug 2021 09:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 04 11:00:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 04:52:40 2021
Response via : Initial Calibration

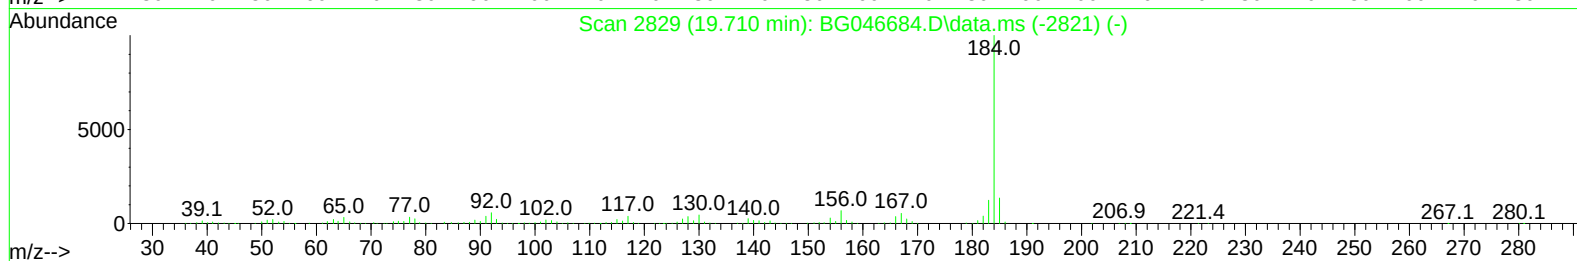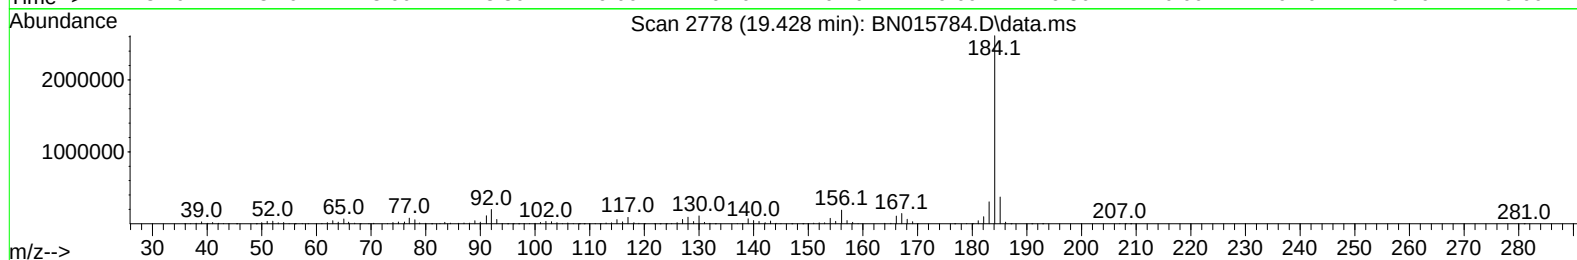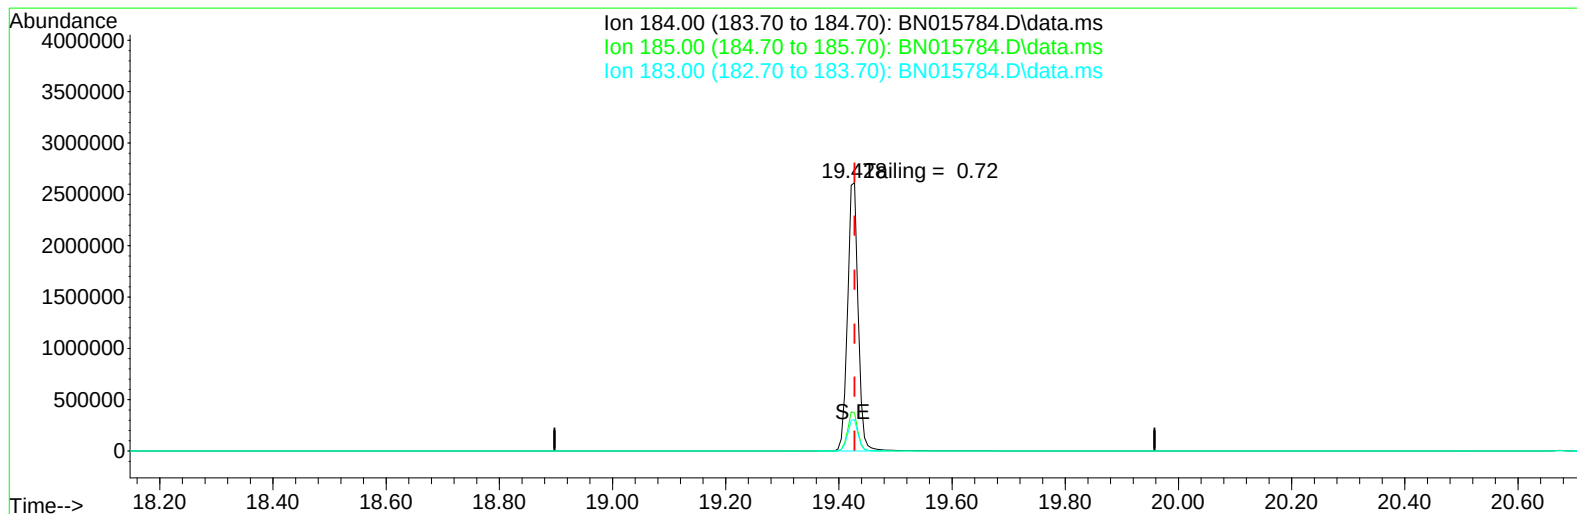

TIC: BN015784.D\data.ms

(77) Benzidine

19.428min (+ 0.000) 0.00 ng




response 3420286

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.21
183.00	13.20	11.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080421\
 Data File : BN015784.D
 Acq On : 04 Aug 2021 09:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 04 11:00:07 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 04:52:40 2021
 Response via : Initial Calibration

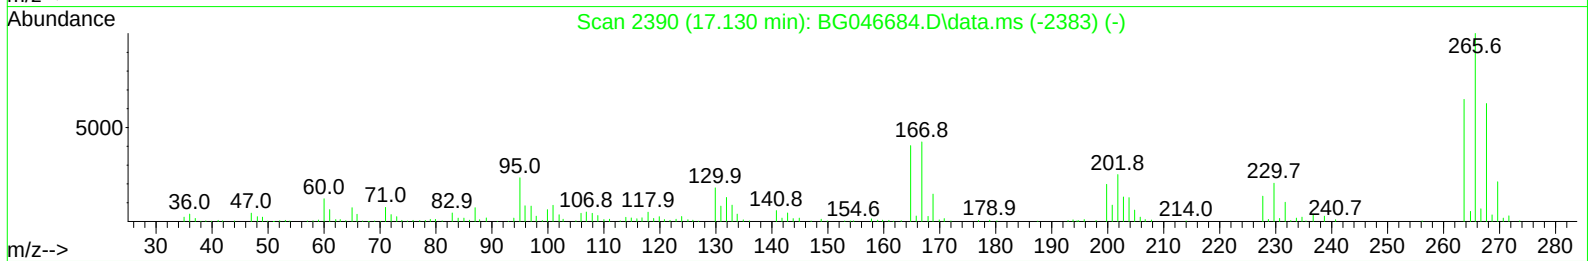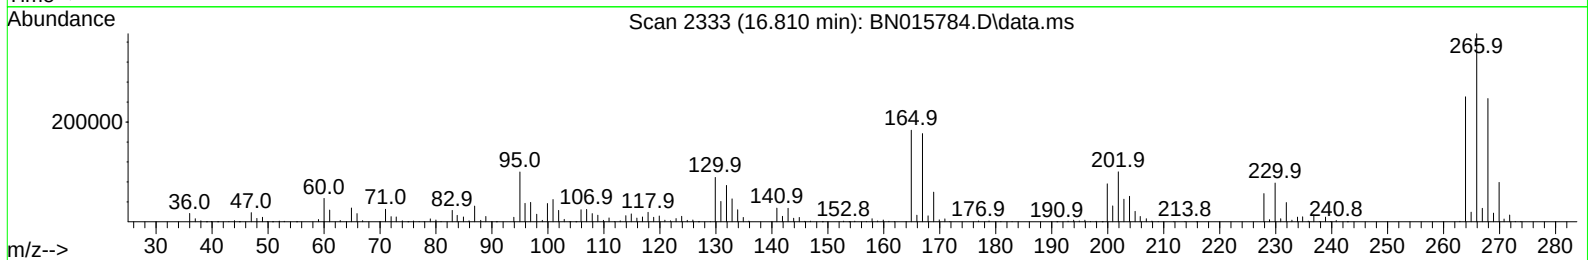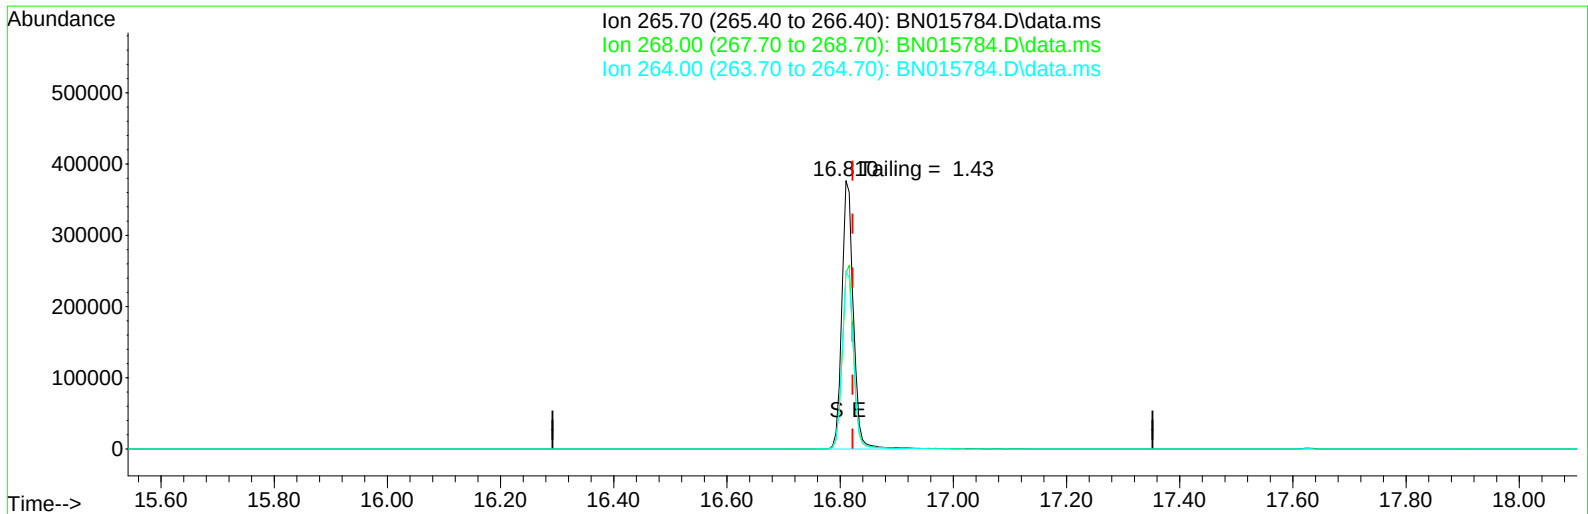

TIC: BN015784.D\data.ms

(70) Pentachlorophenol (C)

16.810min (-0.012) 20648.49 ng

response 535394

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.53
264.00	61.60	66.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/4/2021	BNA_N	<u>BN015784.D</u>
Compound Name	Response	Retention Time
DDT	1644335	20.67
DDD	17151	20.22
DDE	1951	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19102	1663437	1.15

Instrument :
BNA_N
ClientSampleId :
DFTPP