


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081519\
 Data File : BN007199.D
 Acq On : 15 Aug 2019 16:46
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 13 12:12:02 2019

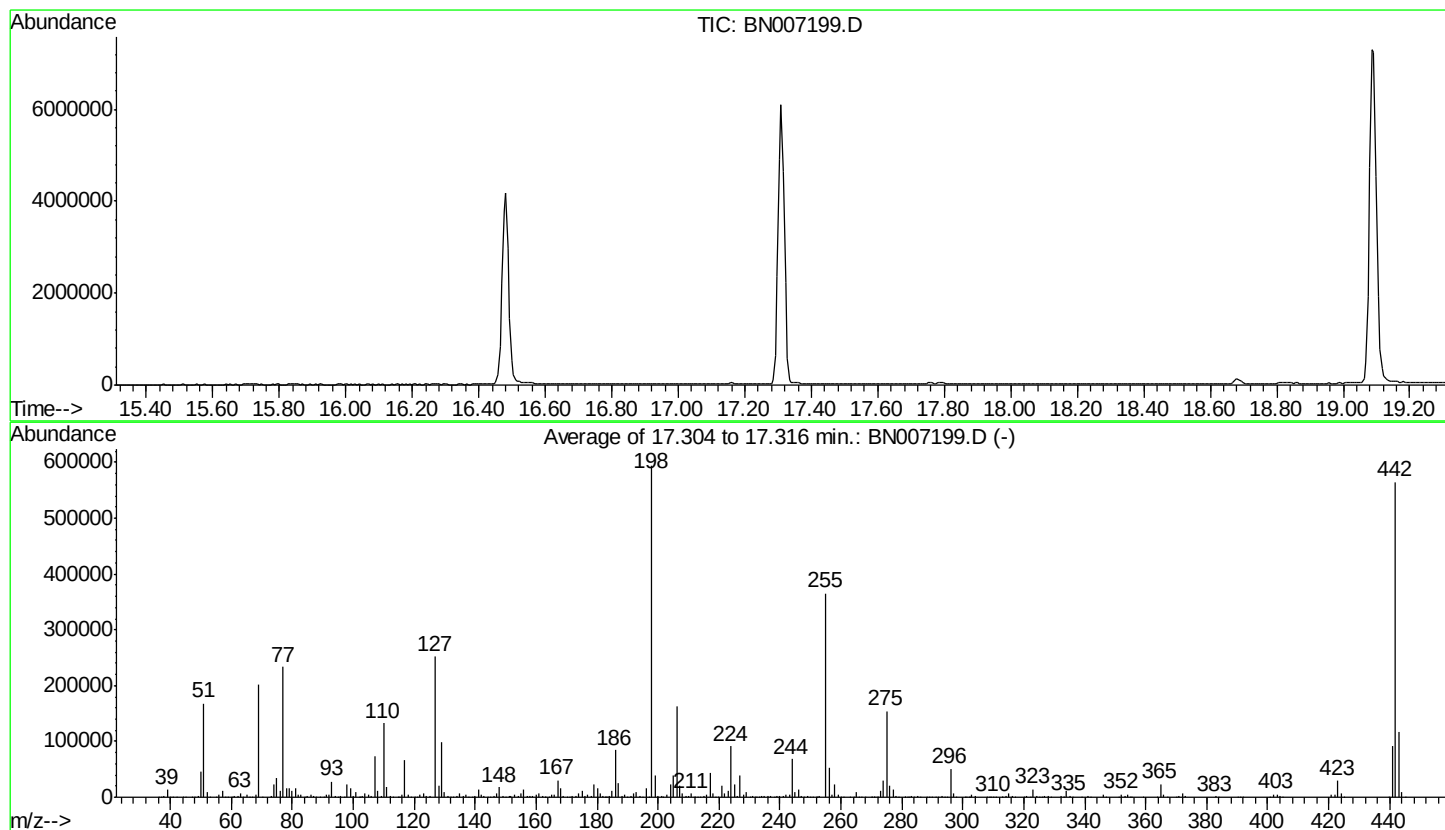

AutoFind: Scans 2434, 2435, 2436; Background Corrected with Scan 2427

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	168426	PASS
68	69	0.00	2	1.9	3860	PASS
69	198	0.00	100	34.1	202408	PASS
70	69	0.00	2	0.6	1223	PASS
127	198	10	80	42.4	252074	PASS
197	198	0.00	2	0.2	1195	PASS
198	198	100	100	100.0	594197	PASS
199	198	5	9	6.6	39077	PASS
275	198	10	60	26.1	154880	PASS
365	198	1	100	4.0	23565	PASS
441	198	0.01	100	15.4	91261	PASS
442	198	50	100	95.1	564992	PASS
443	442	15	24	20.8	117504	PASS